

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048396.D
 Acq On : 03 May 2022 17:30
 Operator : SY/MD
 Sample : N2668-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	103	rBV	237844	321934	16.31%	2.218%
2	1.900	167	174	205	rVB	180157	285710	14.47%	1.969%
3	2.488	356	357	365	rVB2	481	419	0.02%	0.003%
4	2.565	368	381	398	rBV	428504	702319	35.58%	4.840%
5	2.707	423	425	428	rVB3	440	235	0.01%	0.002%
6	2.742	432	436	439	rBV2	488	346	0.02%	0.002%
7	2.787	447	450	454	rVB4	582	435	0.02%	0.003%
8	2.826	459	462	467	rBV2	478	479	0.02%	0.003%
9	2.890	478	482	487	rBV2	330	320	0.02%	0.002%
10	2.964	496	505	510	rBV3	608	1026	0.05%	0.007%
11	3.044	524	530	539	rVB4	1039	1644	0.08%	0.011%
12	3.089	539	544	546	rBV	438	271	0.01%	0.002%
13	3.186	563	574	589	rBV	5093	12030	0.61%	0.083%
14	3.292	603	607	616	rBV3	200	205	0.01%	0.001%
15	3.523	675	679	683	rBV2	210	176	0.01%	0.001%
16	3.559	683	690	694	rVV	160	176	0.01%	0.001%
17	3.591	695	700	703	rBV2	205	208	0.01%	0.001%
18	3.662	719	722	728	rVB2	221	166	0.01%	0.001%
19	3.871	780	787	789	rBV2	206	272	0.01%	0.002%
20	4.154	870	875	879	rBV2	171	204	0.01%	0.001%
21	4.266	906	910	915	rVB2	210	207	0.01%	0.001%
22	4.295	915	919	923	rBV	239	190	0.01%	0.001%
23	4.443	962	965	968	rBV	322	232	0.01%	0.002%
24	4.523	987	990	993	rBV	234	172	0.01%	0.001%
25	4.626	1008	1022	1061	rBV	194994	503690	25.52%	3.471%
26	5.063	1140	1158	1193	rBV	370687	811620	41.12%	5.593%
27	5.218	1203	1206	1210	rVB4	819	529	0.03%	0.004%
28	5.250	1213	1216	1219	rBV2	347	211	0.01%	0.001%
29	5.282	1223	1226	1228	rBV3	412	217	0.01%	0.001%
30	5.337	1237	1243	1247	rBV4	412	555	0.03%	0.004%
31	5.465	1275	1283	1286	rBV	168	187	0.01%	0.001%
32	5.607	1323	1327	1332	rBV	312	308	0.02%	0.002%
33	5.726	1341	1364	1398	rBV2	739526	1973959	100.00%	13.602%
34	5.935	1426	1429	1434	rVB	435	327	0.02%	0.002%
35	5.970	1434	1440	1444	rBV4	1019	1375	0.07%	0.009%
36	6.035	1457	1460	1463	rBV2	503	394	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048396.D
 Acq On : 03 May 2022 17:30
 Operator : SY/MD
 Sample : N2668-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.118	1479	1486	1494	rVV3	661	968	0.05%	0.007%
38	6.250	1512	1527	1566	rBV	492532	942288	47.74%	6.493%
39	6.530	1605	1614	1626	rBV5	2549	4862	0.25%	0.034%
40	6.607	1636	1638	1641	rVB2	673	395	0.02%	0.003%
41	6.690	1649	1664	1691	rBV	449320	877617	44.46%	6.048%
42	6.877	1718	1722	1726	rVB2	231	174	0.01%	0.001%
43	6.993	1753	1758	1760	rBV2	254	167	0.01%	0.001%
44	7.144	1801	1805	1807	rBV	280	243	0.01%	0.002%
45	7.186	1808	1818	1835	rVB5	5263	10724	0.54%	0.074%
46	7.568	1923	1937	1957	rBV	230451	408348	20.69%	2.814%
47	7.687	1966	1974	1982	rVB6	1870	2788	0.14%	0.019%
48	7.761	1992	1997	1999	rBV2	329	223	0.01%	0.002%
49	7.899	2025	2040	2056	rBV	892300	1546152	78.33%	10.654%
50	8.179	2115	2127	2153	rBV	159343	278515	14.11%	1.919%
51	8.517	2228	2232	2236	rVB3	494	296	0.01%	0.002%
52	8.636	2256	2269	2309	rBV2	611853	1137569	57.63%	7.839%
53	8.822	2325	2327	2331	rVB4	299	199	0.01%	0.001%
54	8.886	2343	2347	2350	rBV3	435	362	0.02%	0.002%
55	8.948	2364	2366	2371	rVB3	271	260	0.01%	0.002%
56	8.973	2371	2374	2378	rVB3	335	306	0.02%	0.002%
57	8.996	2378	2381	2382	rBV	411	210	0.01%	0.001%
58	9.054	2395	2399	2402	rBV2	325	248	0.01%	0.002%
59	9.128	2418	2422	2423	rBV	296	211	0.01%	0.001%
60	9.163	2429	2433	2434	rBV3	486	358	0.02%	0.002%
61	9.343	2486	2489	2493	rVB2	358	223	0.01%	0.002%
62	9.417	2498	2512	2554	rBV	693225	1172343	59.39%	8.079%
63	9.565	2554	2558	2560	rBV	445	354	0.02%	0.002%
64	9.632	2573	2579	2580	rBV2	419	343	0.02%	0.002%
65	9.694	2594	2598	2604	rVV3	666	730	0.04%	0.005%
66	9.838	2639	2643	2652	rVB2	326	298	0.02%	0.002%
67	9.948	2675	2677	2680	rBV2	298	195	0.01%	0.001%
68	9.996	2689	2692	2696	rVB2	225	182	0.01%	0.001%
69	10.108	2723	2727	2733	rVB4	564	477	0.02%	0.003%
70	10.237	2765	2767	2772	rVB2	336	213	0.01%	0.001%
71	10.411	2818	2821	2824	rVB2	282	181	0.01%	0.001%
72	10.591	2872	2877	2880	rBV2	166	169	0.01%	0.001%
73	10.674	2894	2903	2914	rVB4	2649	4063	0.21%	0.028%
74	10.758	2915	2929	2951	rBV	690177	1103469	55.90%	7.604%
75	10.893	2964	2971	2980	rVV4	956	1883	0.10%	0.013%
76	10.973	2993	2996	3000	rVV3	395	330	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048396.D
 Acq On : 03 May 2022 17:30
 Operator : SY/MD
 Sample : N2668-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.993	3000	3002	3007	rVB3	324	204	0.01%	0.001%
78	11.115	3036	3040	3049	rVV3	865	997	0.05%	0.007%
79	11.182	3059	3061	3067	rVB2	248	182	0.01%	0.001%
80	11.308	3096	3100	3103	rVB2	288	226	0.01%	0.002%
81	11.410	3131	3132	3139	rVV2	601	551	0.03%	0.004%
82	11.462	3139	3148	3159	rVV5	1842	3295	0.17%	0.023%
83	11.517	3163	3165	3173	rVB2	280	229	0.01%	0.002%
84	11.552	3173	3176	3181	rBV2	373	377	0.02%	0.003%
85	11.697	3215	3221	3231	rVB5	1105	1348	0.07%	0.009%
86	11.755	3236	3239	3240	rBV2	442	231	0.01%	0.002%
87	11.812	3244	3257	3279	rBV	655866	1044938	52.94%	7.201%
88	11.919	3288	3290	3293	rBV3	487	318	0.02%	0.002%
89	11.941	3293	3297	3302	rVV5	700	728	0.04%	0.005%
90	12.111	3347	3350	3353	rBV2	432	278	0.01%	0.002%
91	12.195	3358	3376	3395	rBV	807046	1323967	67.07%	9.123%
92	12.459	3453	3458	3462	rBV3	582	692	0.04%	0.005%
93	12.545	3482	3485	3487	rBV2	341	220	0.01%	0.002%
94	12.610	3501	3505	3506	rBV2	417	277	0.01%	0.002%
95	12.681	3524	3527	3531	rBV2	389	272	0.01%	0.002%
96	12.732	3541	3543	3545	rBV2	309	184	0.01%	0.001%
97	12.774	3547	3556	3566	rVV3	5837	9075	0.46%	0.063%
98	12.912	3592	3599	3601	rBV2	434	589	0.03%	0.004%
99	13.012	3624	3630	3634	rBV2	433	442	0.02%	0.003%
100	14.558	4108	4111	4113	rBV2	728	562	0.03%	0.004%




Sum of corrected areas: 14511866

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048396.D
Acq On : 03 May 2022 17:30
Operator : SY/MD
Sample : N2668-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

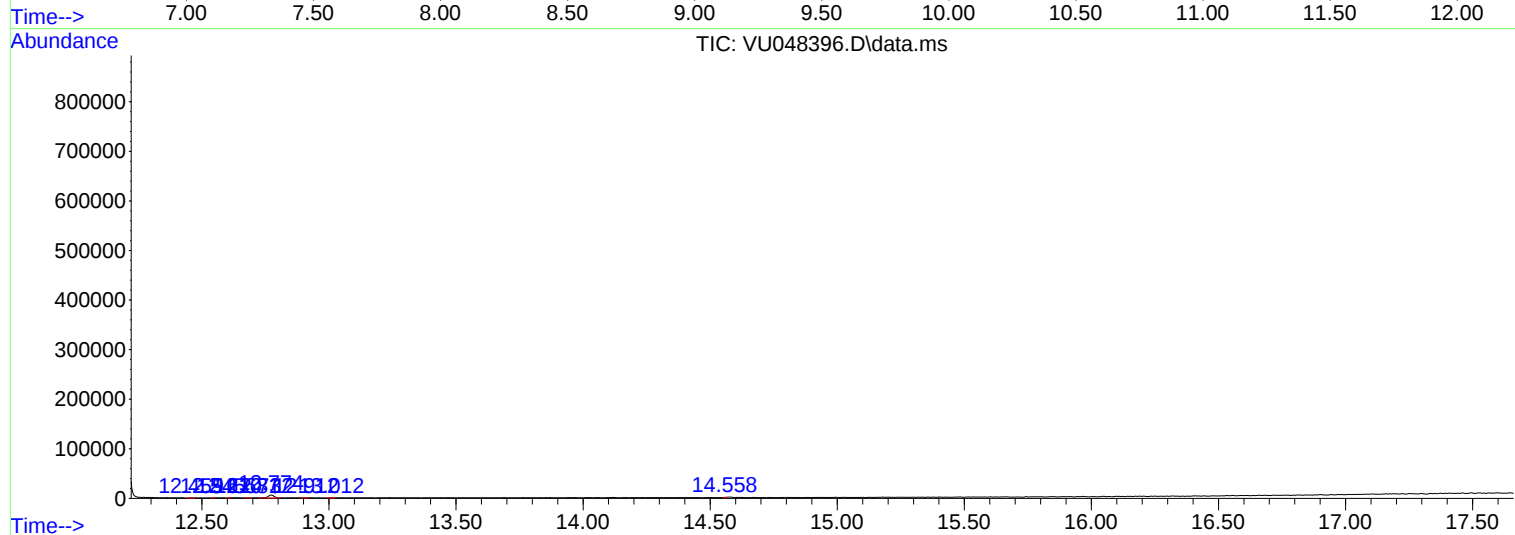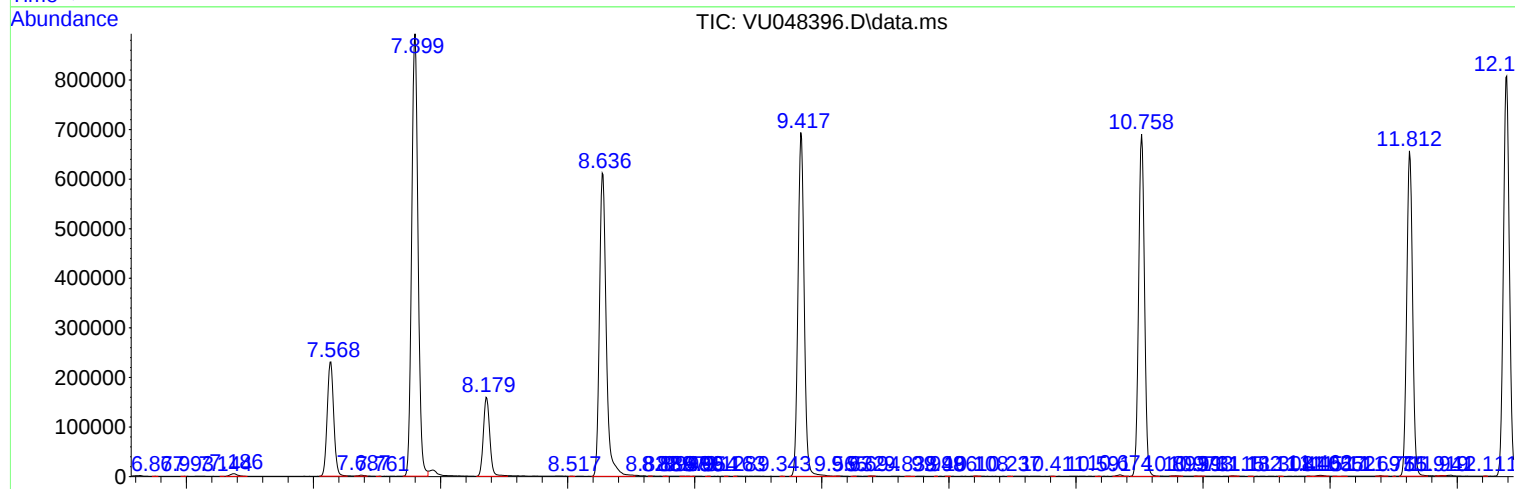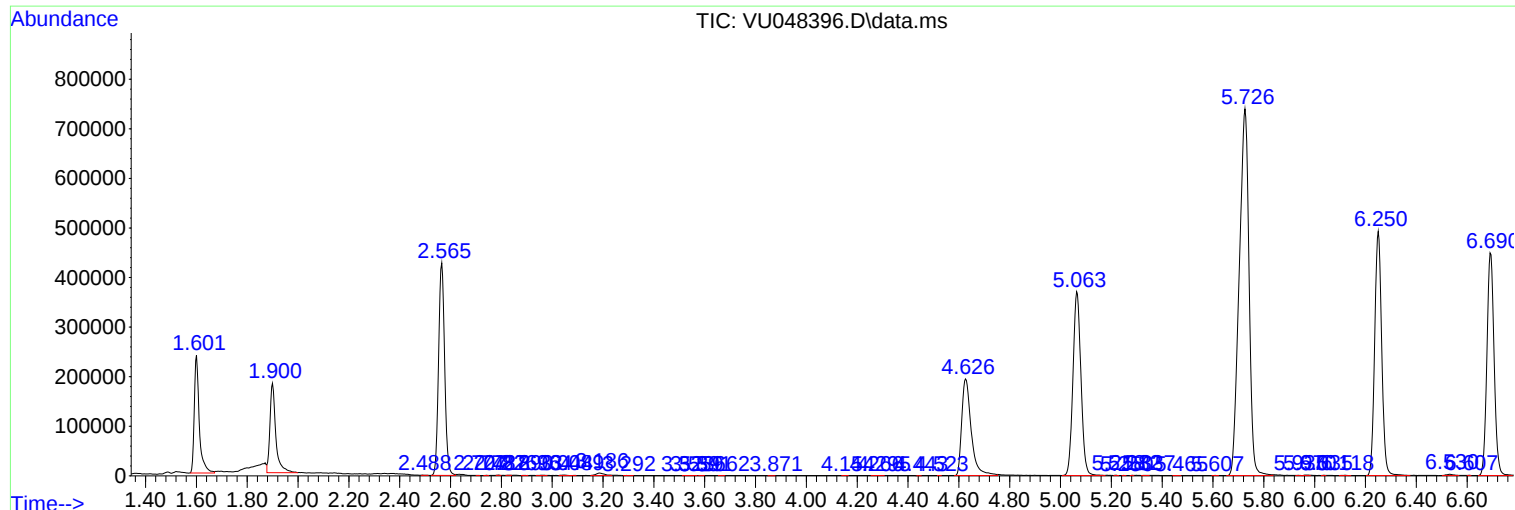

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048396.D
Acq On : 03 May 2022 17:30
Operator : SY/MD
Sample : N2668-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048396.D
Acq On : 03 May 2022 17:30
Operator : SY/MD
Sample : N2668-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc