

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048399.D
 Acq On : 03 May 2022 18:42
 Operator : SY/MD
 Sample : N2668-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	52	rBV3	5717	6570	0.32%	0.044%
2	1.600	73	81	100	rBV	268023	339803	16.79%	2.269%
3	1.900	166	174	186	rBV	177688	253664	12.53%	1.694%
4	2.565	368	381	396	rBV	437966	714982	35.33%	4.774%
5	2.671	412	414	419	rVB	383	263	0.01%	0.002%
6	2.771	434	445	446	rBV5	2184	2882	0.14%	0.019%
7	2.835	462	465	469	rVB3	359	267	0.01%	0.002%
8	2.912	486	489	492	rBV2	357	231	0.01%	0.002%
9	2.951	496	501	505	rBV2	576	776	0.04%	0.005%
10	3.041	524	529	530	rBV2	773	584	0.03%	0.004%
11	3.092	540	545	547	rBV	260	218	0.01%	0.001%
12	3.182	562	573	576	rBV3	1844	2857	0.14%	0.019%
13	3.292	604	607	609	rBV	233	166	0.01%	0.001%
14	3.340	619	622	625	rVB2	278	166	0.01%	0.001%
15	3.366	628	630	635	rVV2	296	249	0.01%	0.002%
16	3.388	635	637	640	rVV	213	143	0.01%	0.001%
17	3.465	659	661	664	rVB2	256	150	0.01%	0.001%
18	3.546	679	686	687	rBV2	164	163	0.01%	0.001%
19	3.661	718	722	725	rBV2	266	220	0.01%	0.001%
20	3.700	732	734	737	rVB	406	213	0.01%	0.001%
21	3.719	738	740	745	rVB2	287	143	0.01%	0.001%
22	4.012	828	831	836	rVB2	203	209	0.01%	0.001%
23	4.051	836	843	855	rBV2	187	398	0.02%	0.003%
24	4.163	873	878	881	rBV	266	227	0.01%	0.002%
25	4.237	898	901	905	rBV2	280	244	0.01%	0.002%
26	4.317	924	926	933	rVB	224	192	0.01%	0.001%
27	4.391	945	949	953	rVB2	165	148	0.01%	0.001%
28	4.488	975	979	986	rVB2	200	184	0.01%	0.001%
29	4.620	1006	1020	1045	rBV	211773	507300	25.07%	3.388%
30	4.880	1096	1101	1105	rBV3	383	410	0.02%	0.003%
31	4.938	1115	1119	1122	rVB2	297	203	0.01%	0.001%
32	5.063	1141	1158	1180	rBV	358780	779642	38.53%	5.206%
33	5.218	1204	1206	1217	rVB4	649	709	0.04%	0.005%
34	5.292	1223	1229	1231	rBV	575	639	0.03%	0.004%
35	5.337	1235	1243	1252	rVB2	1083	2096	0.10%	0.014%
36	5.546	1305	1308	1312	rBV	163	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048399.D
 Acq On : 03 May 2022 18:42
 Operator : SY/MD
 Sample : N2668-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	5.575	1312	1317	1323	rVB2	143	172	0.01%	0.001%
38	5.726	1342	1364	1395	rBV2	756356	2023647	100.00%	13.513%
39	5.957	1433	1436	1437	rBV	453	222	0.01%	0.001%
40	6.102	1477	1481	1482	rBV	199	145	0.01%	0.001%
41	6.250	1511	1527	1551	rBV	496039	949646	46.93%	6.342%
42	6.420	1577	1580	1584	rVB2	267	225	0.01%	0.002%
43	6.497	1602	1604	1606	rBV2	288	183	0.01%	0.001%
44	6.533	1606	1615	1626	rVB4	2153	4248	0.21%	0.028%
45	6.578	1628	1629	1633	rVB2	261	142	0.01%	0.001%
46	6.597	1633	1635	1638	rBV2	448	278	0.01%	0.002%
47	6.690	1648	1664	1689	rBV	463058	901432	44.54%	6.020%
48	6.848	1710	1713	1721	rVB3	535	480	0.02%	0.003%
49	6.954	1741	1746	1752	rBV	516	752	0.04%	0.005%
50	7.105	1787	1793	1798	rBV2	346	432	0.02%	0.003%
51	7.185	1804	1818	1827	rBV5	3923	7632	0.38%	0.051%
52	7.449	1897	1900	1903	rVB2	252	147	0.01%	0.001%
53	7.565	1922	1936	1955	rBV	240567	420501	20.78%	2.808%
54	7.687	1968	1974	1985	rVB4	2157	4018	0.20%	0.027%
55	7.732	1985	1988	1989	rBV2	288	183	0.01%	0.001%
56	7.784	2000	2004	2005	rBV2	474	306	0.02%	0.002%
57	7.841	2019	2022	2025	rBV2	246	216	0.01%	0.001%
58	7.899	2025	2040	2057	rBV	929795	1601454	79.14%	10.694%
59	8.134	2110	2113	2115	rBV2	239	183	0.01%	0.001%
60	8.179	2115	2127	2144	rBV	167122	281598	13.92%	1.880%
61	8.436	2203	2207	2211	rBV3	228	216	0.01%	0.001%
62	8.472	2211	2218	2227	rVB3	2188	3318	0.16%	0.022%
63	8.555	2231	2244	2256	rBV	101158	170372	8.42%	1.138%
64	8.632	2256	2268	2301	rBV2	615518	1156600	57.15%	7.723%
65	8.832	2326	2330	2334	rVB4	677	588	0.03%	0.004%
66	8.893	2345	2349	2351	rBV3	408	337	0.02%	0.002%
67	8.925	2355	2359	2360	rBV2	394	248	0.01%	0.002%
68	8.976	2371	2375	2377	rBV3	368	271	0.01%	0.002%
69	9.111	2411	2417	2420	rBV3	464	410	0.02%	0.003%
70	9.250	2458	2460	2464	rVB2	322	199	0.01%	0.001%
71	9.417	2498	2512	2547	rBV	718946	1195658	59.08%	7.984%
72	9.555	2552	2555	2556	rVV	336	173	0.01%	0.001%
73	9.568	2556	2559	2566	rVB	746	621	0.03%	0.004%
74	9.639	2578	2581	2590	rVB3	480	634	0.03%	0.004%
75	9.693	2592	2598	2606	rBV3	858	1319	0.07%	0.009%
76	9.819	2634	2637	2640	rVB	281	152	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048399.D
 Acq On : 03 May 2022 18:42
 Operator : SY/MD
 Sample : N2668-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	9.938	2671	2674	2676	rBV2	208	142	0.01%	0.001%
78	9.976	2683	2686	2691	rVB	351	260	0.01%	0.002%
79	10.076	2713	2717	2720	rBV2	313	248	0.01%	0.002%
80	10.099	2720	2724	2725	rBV2	359	244	0.01%	0.002%
81	10.182	2746	2750	2753	rBV2	432	328	0.02%	0.002%
82	10.333	2793	2797	2801	rBV2	268	304	0.02%	0.002%
83	10.668	2896	2901	2910	rVB3	2399	3163	0.16%	0.021%
84	10.758	2915	2929	2951	rBV	718856	1161000	57.37%	7.753%
85	10.893	2963	2971	2979	rVB2	4637	6225	0.31%	0.042%
86	11.015	3006	3009	3012	rBV2	320	222	0.01%	0.001%
87	11.034	3012	3015	3018	rBV2	277	186	0.01%	0.001%
88	11.115	3036	3040	3047	rBV4	687	873	0.04%	0.006%
89	11.455	3140	3146	3147	rBV2	1476	1215	0.06%	0.008%
90	11.523	3163	3167	3169	rBV	202	184	0.01%	0.001%
91	11.687	3215	3218	3219	rBV	354	212	0.01%	0.001%
92	11.812	3244	3257	3281	rBV	675057	1075689	53.16%	7.183%
93	11.976	3302	3308	3314	rVB5	1689	2323	0.11%	0.016%
94	12.066	3327	3336	3339	rBV5	1510	1855	0.09%	0.012%
95	12.195	3359	3376	3397	rBV	844391	1368654	67.63%	9.140%
96	12.330	3414	3418	3424	rVB5	931	888	0.04%	0.006%
97	12.436	3448	3451	3456	rBV3	466	454	0.02%	0.003%
98	12.513	3471	3475	3477	rBV2	270	224	0.01%	0.001%
99	12.770	3548	3555	3563	rBV2	1775	2977	0.15%	0.020%
100	14.957	4233	4235	4238	rBV	522	389	0.02%	0.003%




Sum of corrected areas: 14975081

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048399.D
Acq On : 03 May 2022 18:42
Operator : SY/MD
Sample : N2668-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

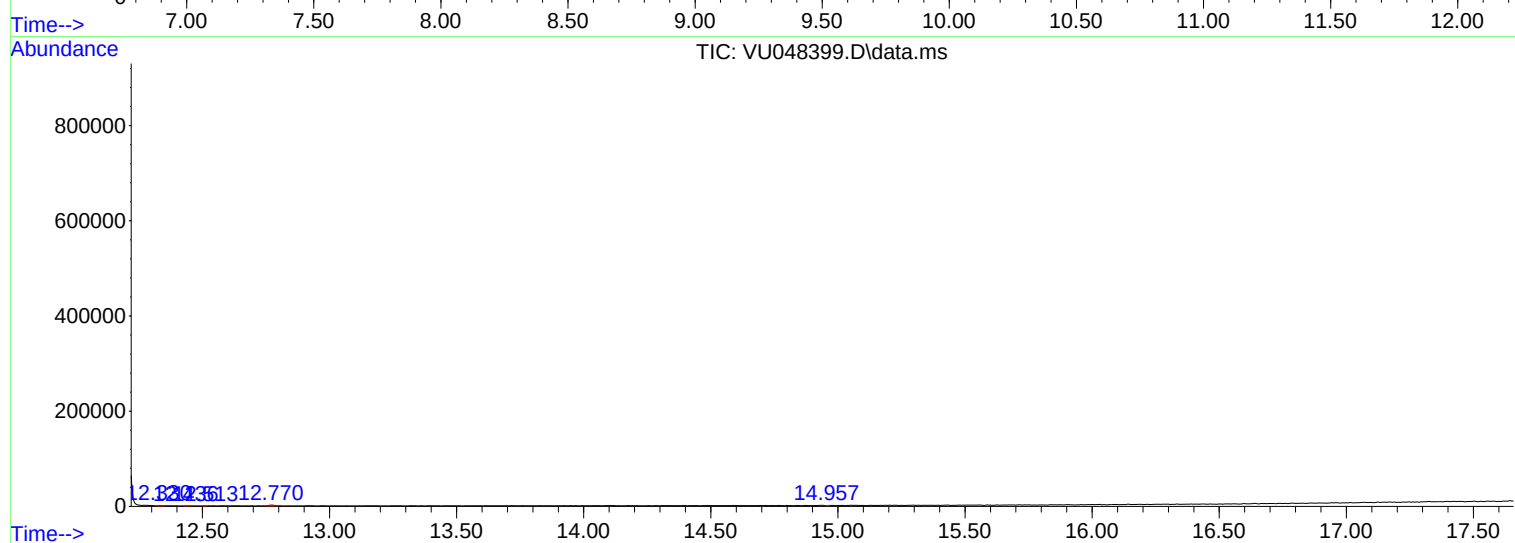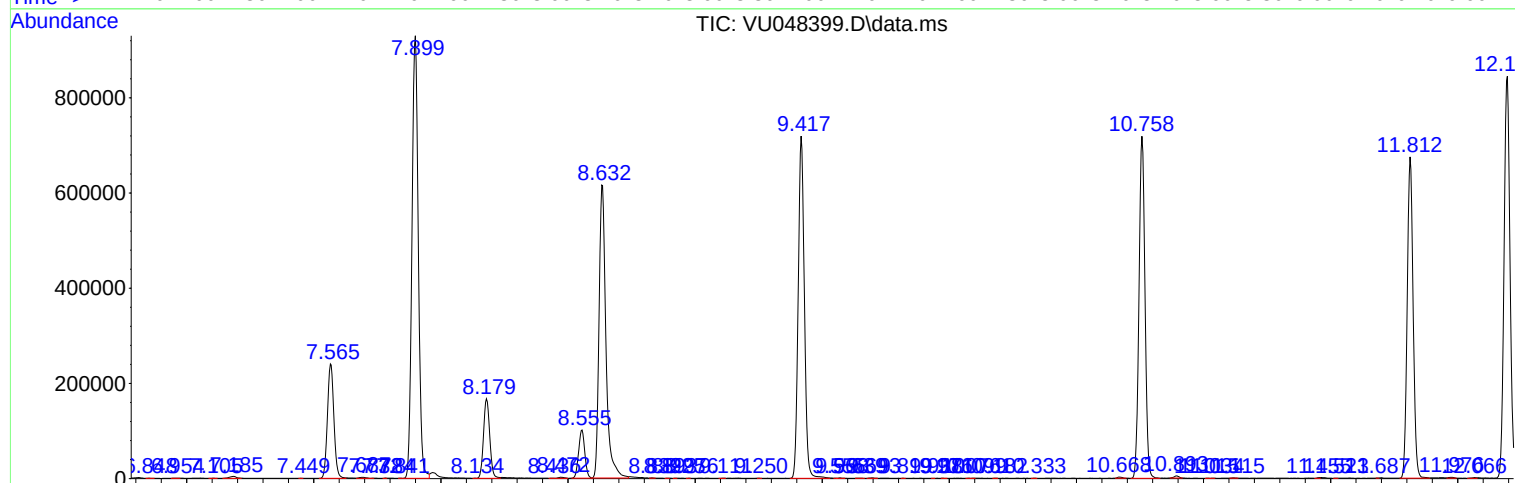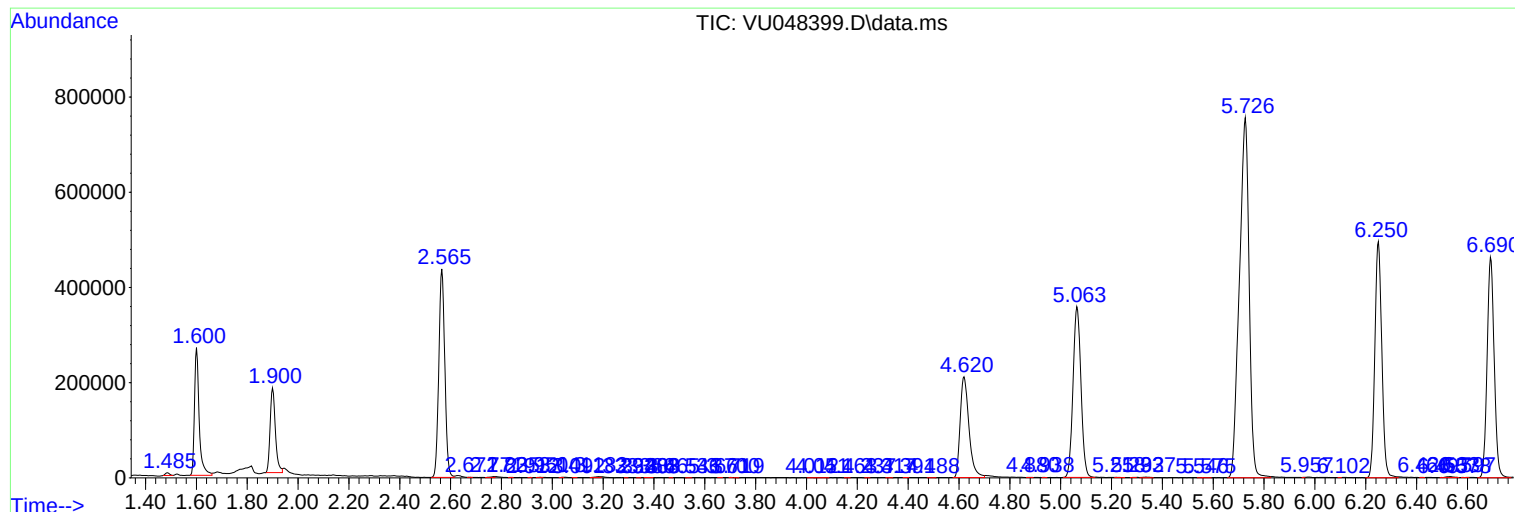

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048399.D
Acq On : 03 May 2022 18:42
Operator : SY/MD
Sample : N2668-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048399.D
Acq On : 03 May 2022 18:42
Operator : SY/MD
Sample : N2668-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------