


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048381.D
 Acq On : 03 May 2022 09:05
 Operator : SY/MD
 Sample : BFB078
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB078

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis
 Last Update : Thu May 05 02:16:45 2022

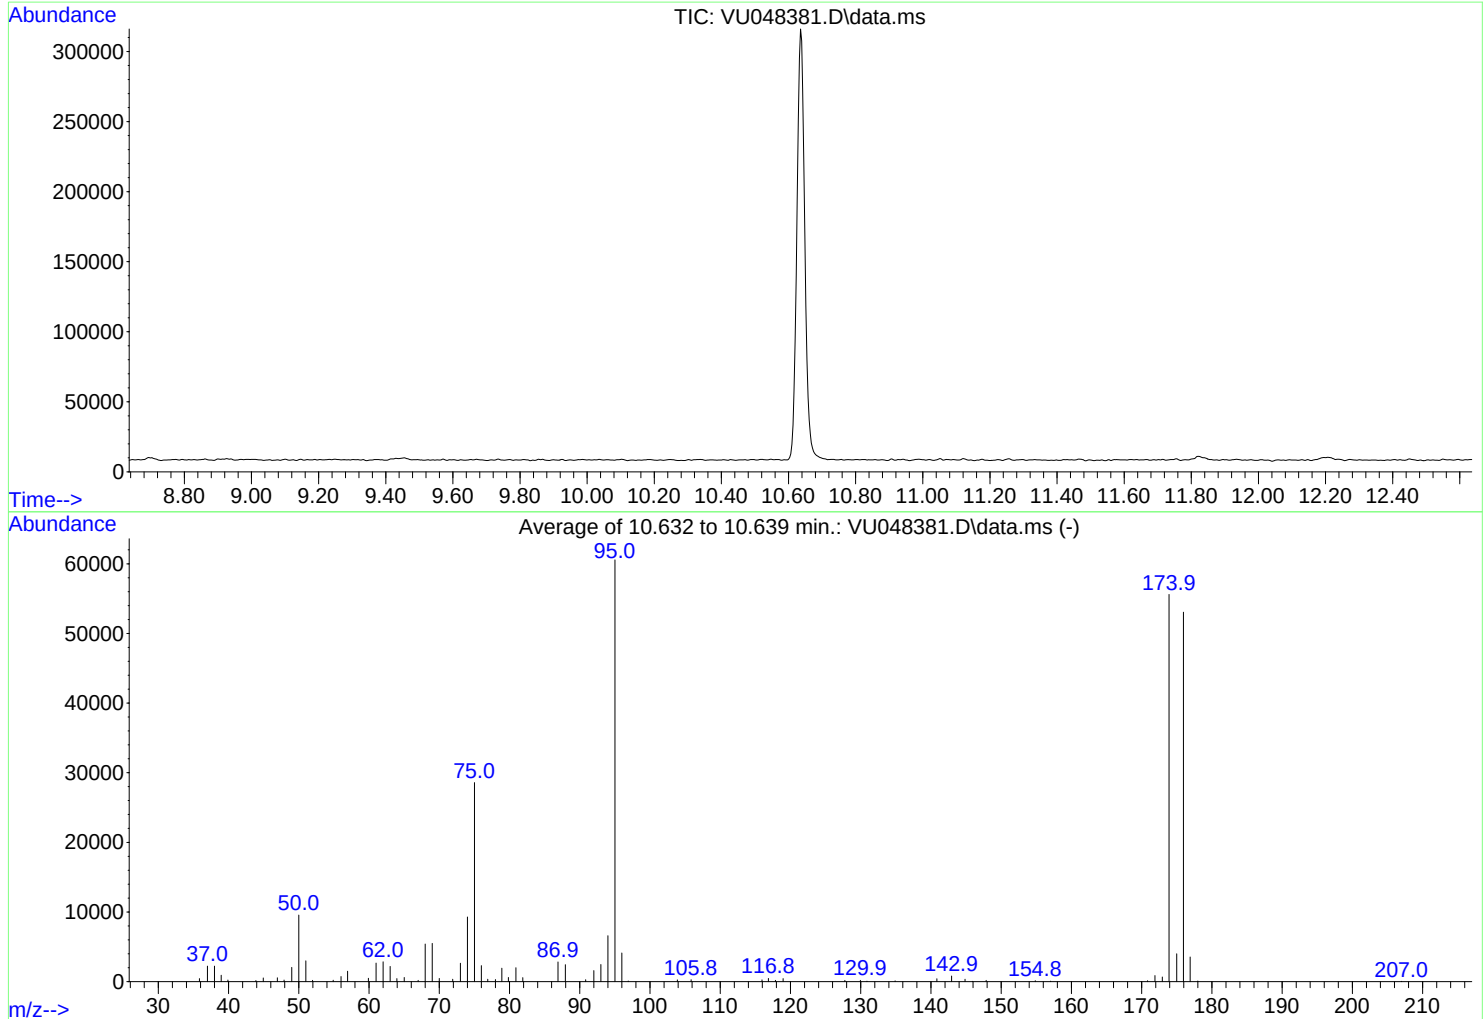

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	9567	PASS
75	95	30	80	47.2	28584	PASS
95	95	100	100	100.0	60568	PASS
96	95	5	9	6.8	4111	PASS
173	174	0.00	2	1.2	661	PASS
174	95	50	120	91.8	55597	PASS
175	174	5	9	7.2	4003	PASS
176	174	95	101	95.4	53059	PASS
177	176	5	9	6.7	3529	PASS

m/z	Abundance
35.00	433.0
37.00	2203.0
38.00	2112.0
38.90	1024.0
39.90	8134.0
44.00	656.0
45.00	443.0
47.00	511.0
49.00	2027.0
50.00	9418.0
51.00	2928.0
52.00	176.0
54.90	205.0
56.00	706.0
56.90	1481.0
59.90	490.0
61.00	2566.0
62.00	2789.0
63.00	2168.0
64.00	433.0
65.00	649.0
67.00	187.0
68.00	5362.0
69.00	5296.0
70.00	428.0
71.90	359.0
73.00	2617.0
74.00	9010.0
75.00	28144.0
76.00	2351.0
76.90	351.0
78.00	318.0
78.90	1852.0
79.90	612.0
80.90	1946.0
81.90	526.0
86.90	2763.0
87.90	2414.0
90.90	248.0
92.00	1442.0
93.00	2438.0
94.00	6410.0
95.00	58792.0
96.00	3975.0
96.90	104.0
103.90	261.0
105.80	273.0
116.00	264.0
116.90	416.0
117.90	188.0
119.00	386.0
127.80	167.0
130.00	189.0
135.00	120.0
140.80	405.0
142.90	810.0
144.80	364.0
145.90	116.0
147.80	194.0
154.80	128.0
170.80	125.0
171.90	786.0
173.00	685.0
173.90	52560.0
175.00	4013.0
175.90	49872.0
176.90	3383.0
178.00	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB078

m/z	Abundance
39.90	8000.0
43.90	511.0

Instrument :
MSVOA_U
ClientSampleId :
BFB078

m/z	Abundance
35.90	440.0
37.00	2353.0
38.00	2340.0
38.90	931.0
39.90	8269.0
43.90	687.0
44.90	571.0
47.00	603.0
47.90	296.0
49.00	2120.0
50.00	9880.0
51.00	3104.0
52.00	201.0
54.90	217.0
56.00	780.0
56.90	1555.0
59.90	484.0
61.00	2774.0
62.00	2991.0
63.00	2251.0
64.00	444.0
65.00	622.0
67.00	186.0
68.00	5544.0
69.00	5573.0
70.00	492.0
71.90	367.0
73.00	2734.0
74.00	9606.0
75.00	29472.0
76.00	2393.0
76.90	345.0
78.00	301.0
78.90	1993.0
79.80	605.0
80.90	2070.0
81.90	596.0
86.90	2934.0
88.00	2511.0
90.80	284.0
92.00	1661.0
93.00	2556.0
94.00	6847.0
95.00	62560.0
96.00	4226.0
96.90	111.0
103.90	269.0
105.90	269.0
115.90	272.0
116.90	489.0
117.90	196.0
118.90	445.0
127.70	190.0
130.00	209.0
130.90	116.0
134.90	107.0
140.80	430.0
143.00	859.0
144.80	352.0
147.80	196.0
154.80	140.0
157.00	111.0
170.90	148.0
171.90	858.0
172.90	661.0
173.90	57344.0
175.00	4173.0
175.90	54536.0
176.90	3661.0
178.00	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB078

m/z	Abundance
35.90	419.0
37.00	2161.0
38.00	2258.0
39.00	803.0
39.90	8284.0
43.90	701.0
45.00	602.0
46.90	574.0
47.90	392.0
49.00	2016.0
50.00	9403.0
51.00	2930.0
51.90	207.0
54.90	187.0
56.00	727.0
57.00	1420.0
59.90	466.0
61.00	2644.0
62.00	2785.0
63.00	2111.0
63.90	401.0
65.00	534.0
67.00	170.0
68.00	5309.0
69.00	5613.0
70.00	473.0
71.90	311.0
73.00	2597.0
74.00	9213.0
75.00	28136.0
76.00	2166.0
76.90	311.0
78.00	258.0
78.90	1936.0
79.90	581.0
80.90	1999.0
81.90	608.0
86.90	2775.0
88.00	2393.0
90.80	267.0
92.00	1676.0
93.00	2402.0
94.00	6564.0
95.00	60352.0
96.00	4131.0
96.90	100.0
103.90	243.0
105.90	265.0
115.90	241.0
116.80	479.0
117.80	170.0
118.90	447.0
127.70	177.0
129.90	183.0
130.90	115.0
134.80	107.0
140.90	438.0
142.90	776.0
144.90	327.0
147.90	156.0
154.90	159.0
157.10	117.0
170.90	153.0
171.90	953.0
172.90	636.0
173.90	56888.0
175.00	3824.0
176.00	54768.0
176.90	3542.0
207.00	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB078