
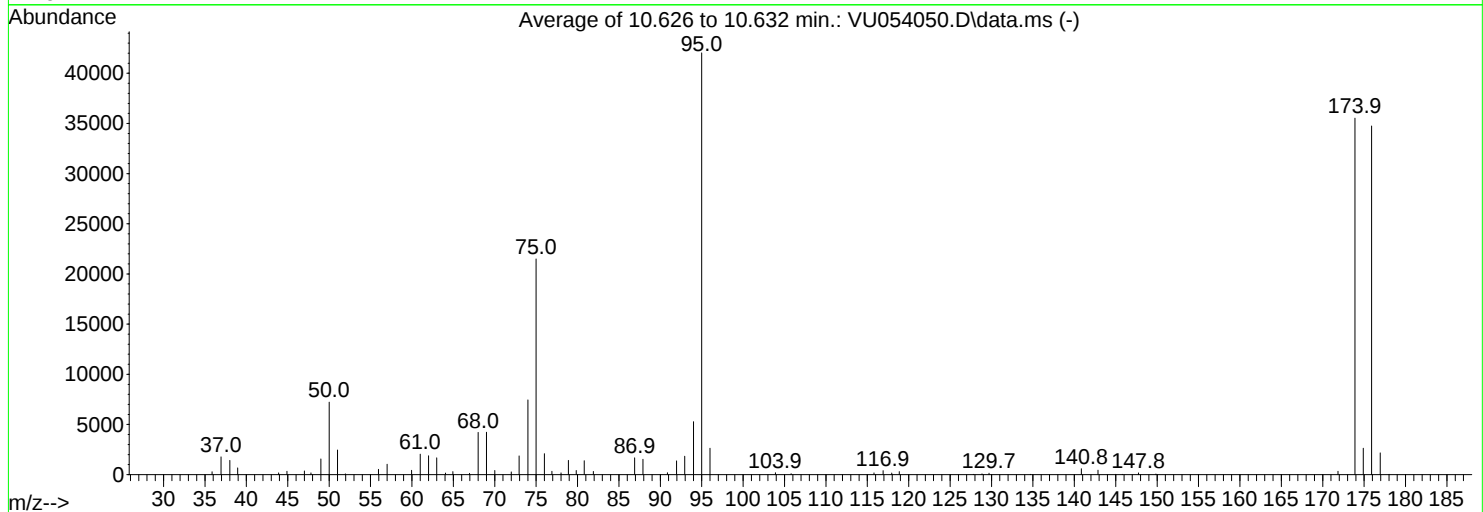


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050323\
Data File : VU054050.D
Acq On : 03 May 2023 09:07
Operator : JC/MD
Sample : BFB022
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB022

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM042723.M
Title : TRACE VOA SOM01.0
Last Update : Thu Apr 27 08:10:40 2023

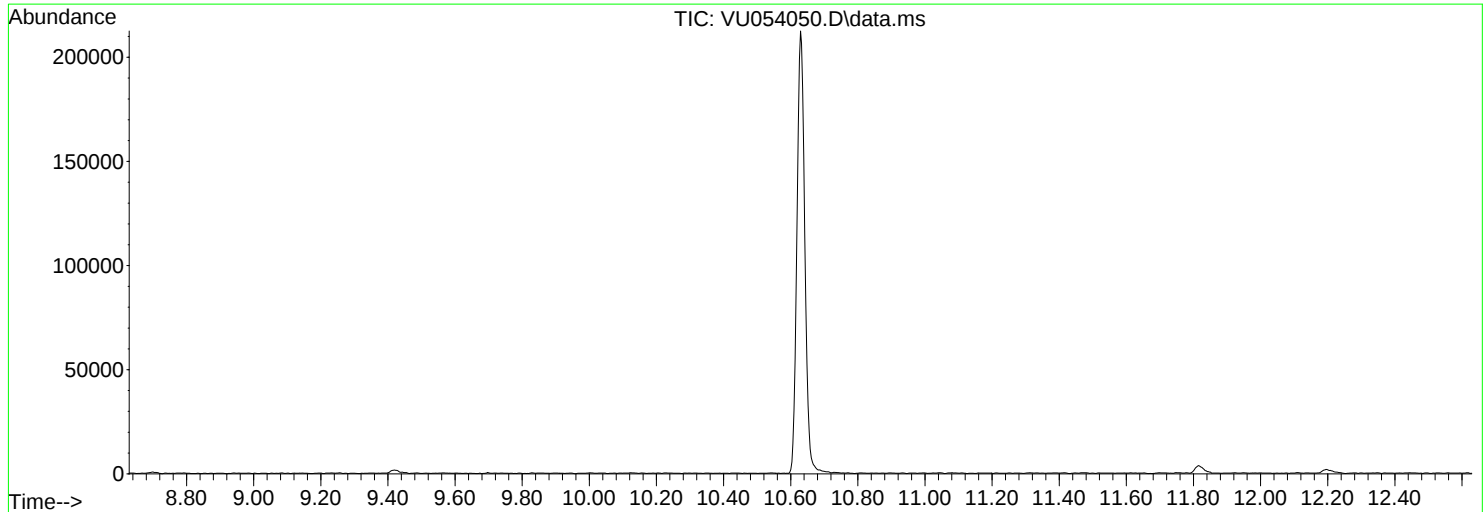

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	7230	PASS
75	95	30	80	51.2	21501	PASS
95	95	100	100	100.0	42035	PASS
96	95	5	9	6.2	2625	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.5	35531	PASS
175	174	5	9	7.4	2627	PASS
176	174	95	101	97.8	34747	PASS
177	176	5	9	6.2	2165	PASS

m/z	Abundance
39.90	104.0
44.00	224.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.80	285.0
37.00	1604.0
38.00	1390.0
39.00	707.0
39.90	132.0
43.90	379.0
44.90	336.0
47.00	409.0
47.80	168.0
49.00	1524.0
50.00	7175.0
51.00	2315.0
55.90	599.0
57.00	1075.0
59.90	427.0
61.00	1946.0
62.00	1910.0
63.00	1499.0
64.10	151.0
65.00	291.0
67.00	153.0
68.00	4065.0
69.00	4163.0
70.00	439.0
72.00	230.0
72.90	1885.0
74.00	7369.0
75.00	20656.0
76.00	1858.0
76.90	303.0
78.00	193.0
78.90	1355.0
79.90	387.0
80.80	1290.0
81.90	280.0
86.90	1675.0
87.90	1328.0
90.90	217.0
92.00	1319.0
92.90	1828.0
94.00	4878.0
95.00	41160.0
96.00	2752.0
103.90	189.0
105.80	142.0
115.80	178.0
116.90	337.0
117.90	126.0
118.80	316.0
129.70	180.0
140.90	557.0
142.80	365.0
145.00	108.0
147.80	190.0
149.80	100.0
171.80	270.0
173.90	33776.0
174.90	2447.0
175.90	33352.0
177.00	2116.0
178.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	303.0
37.00	1835.0
38.00	1466.0
38.90	715.0
39.90	115.0
43.90	412.0
44.90	366.0
47.00	374.0
47.80	179.0
49.00	1620.0
50.00	7415.0
51.00	2565.0
51.90	102.0
55.90	540.0
57.00	1045.0
60.00	435.0
61.00	2083.0
62.00	1899.0
63.00	1758.0
64.10	160.0
64.90	314.0
67.00	148.0
68.00	4390.0
69.00	4360.0
70.00	430.0
72.00	272.0
73.00	1946.0
74.00	7683.0
75.00	22176.0
76.00	2128.0
76.90	352.0
78.00	172.0
78.90	1484.0
79.90	438.0
80.80	1437.0
81.90	331.0
86.90	1737.0
87.90	1568.0
90.90	214.0
91.90	1428.0
92.90	1885.0
94.00	5482.0
95.00	43368.0
96.00	2675.0
103.90	198.0
105.80	139.0
115.80	175.0
116.90	424.0
118.00	173.0
118.90	301.0
128.80	110.0
129.70	147.0
140.80	632.0
142.80	446.0
147.70	175.0
149.90	102.0
171.80	361.0
173.90	36640.0
174.90	2708.0
175.90	35840.0
176.90	2190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	279.0
36.90	1858.0
38.00	1420.0
38.90	604.0
43.90	412.0
44.90	308.0
47.00	329.0
47.80	190.0
49.00	1531.0
50.00	7101.0
51.00	2469.0
52.00	129.0
56.00	457.0
57.00	989.0
60.00	418.0
61.00	2095.0
62.00	1849.0
63.00	1780.0
63.90	156.0
65.00	318.0
66.90	107.0
68.00	4169.0
69.00	4133.0
70.00	363.0
72.00	305.0
72.90	1785.0
74.00	7310.0
75.00	21672.0
76.00	2259.0
76.90	330.0
78.00	166.0
78.90	1436.0
79.80	418.0
80.80	1440.0
81.90	335.0
86.90	1629.0
87.90	1698.0
90.80	156.0
91.90	1382.0
93.00	1808.0
94.00	5502.0
95.00	41576.0
96.00	2449.0
103.90	180.0
115.80	154.0
116.90	443.0
117.90	199.0
118.90	274.0
127.80	104.0
128.90	118.0
129.70	103.0
134.70	104.0
140.80	570.0
142.90	508.0
145.80	100.0
147.70	156.0
171.90	393.0
173.90	36176.0
174.90	2726.0
175.90	35048.0
176.90	2190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022