

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050418\
 Data File : VU023640.D
 Acq On : 04 May 2018 19:44
 Operator : MD/SY
 Sample : J2630-11
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: May 05 01:31:51 2018
 Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 05 01:17:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	151993	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	158871	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	70800	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	52311	4.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.80%
7) Chloroethane-d5	1.68	69	42242	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.20%
11) 1,1-Dichloroethene-d2	2.27	63	71916	3.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.20%
20) 2-Butanone-d5	4.20	46	169660	53.19	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.38%
24) Chloroform-d	4.65	84	100137	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.32	65	55420	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
32) Benzene-d6	5.34	84	195630	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
36) 1,2-Dichloropropane-d6	6.34	67	69113	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.57	98	161545	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
43) trans-1,3-Dichloropropene-	7.86	79	21746	4.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.00%
46) 2-Hexanone-d5	8.32	63	131641	50.24	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.48%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	54774	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.20%
64) 1,2-Dichlorobenzene-d4	11.87	152	69262	5.26	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.20%


Target Compounds					Ovalue
13) Acetone	2.33	43	10824	5.94 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050418\
Data File : VU023640.D
Acq On : 04 May 2018 19:44
Operator : MD/SY
Sample : J2630-11
Misc : 25mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Quant Time: May 05 01:31:51 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 05 01:17:03 2018
Response via : Initial Calibration

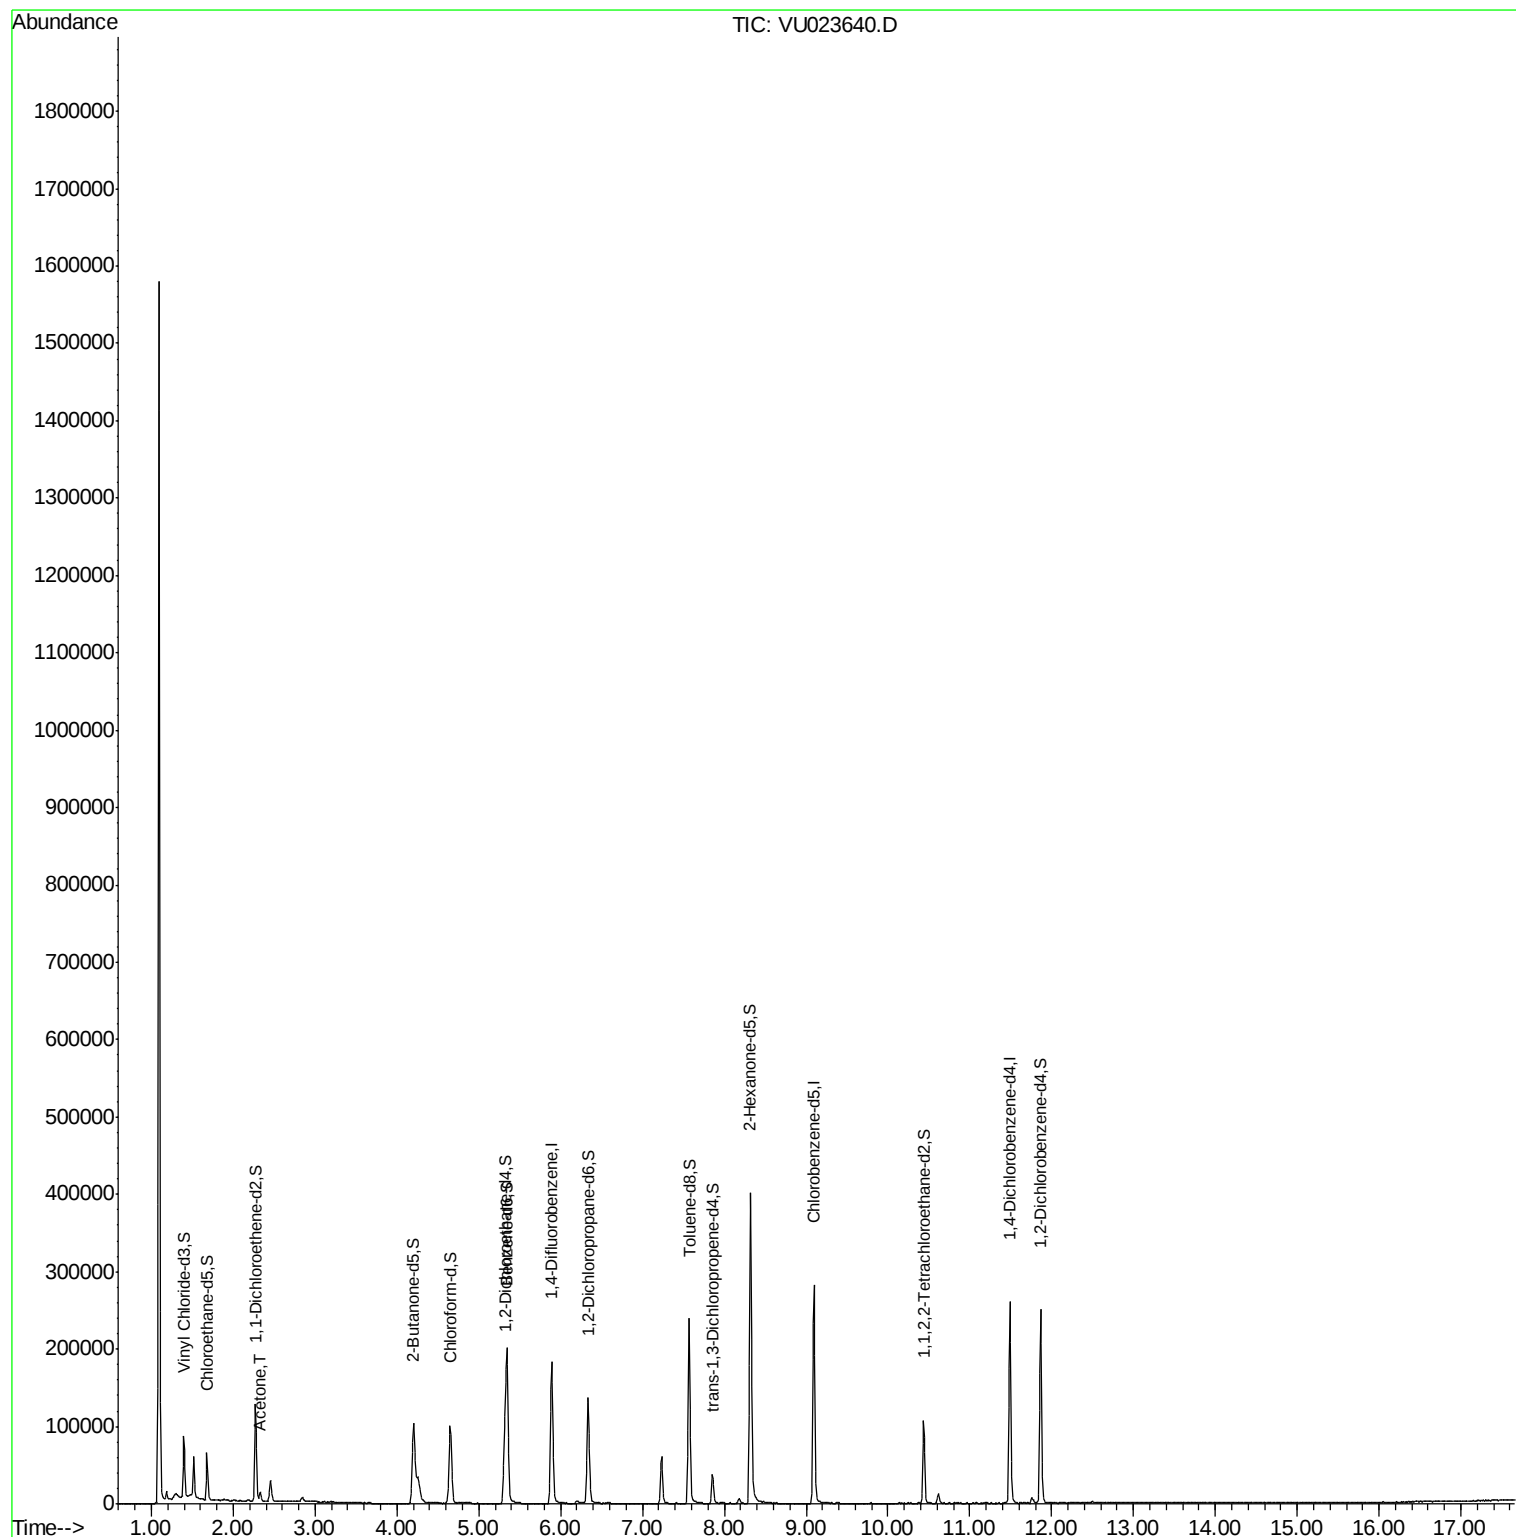

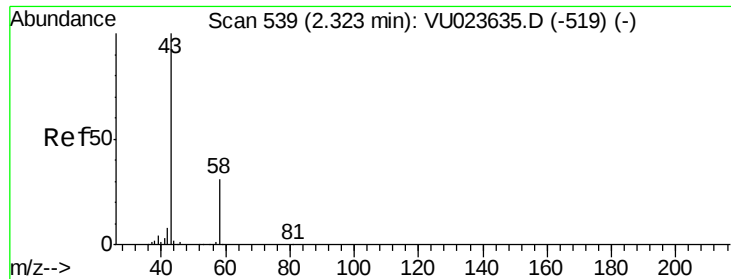

#13

Acetone

Concen: 5.94 ug/L

RT: 2.33 min Scan# 540

Delta R.T. 0.00 min

Lab File: VU023640.D

Acq: 04 May 2018 19:44

Tot Ion: 43 Resp: 10824

Ion Ratio Lower Upper

43 100

58 30.5 0.0 63.8

