

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050418\
 Data File : VU023641.D
 Acq On : 04 May 2018 20:10
 Operator : MD/SY
 Sample : J2630-14
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Quant Time: May 05 01:33:19 2018
 Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 05 01:17:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	149620	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	153782	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	67723	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	48887	4.50	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.00%
7) Chloroethane-d5	1.68	69	40139	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.27	63	67583	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	4.20	46	156876	49.97	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.94%
24) Chloroform-d	4.65	84	93796	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
26) 1,2-Dichloroethane-d4	5.32	65	51698	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.34	84	180399	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.40%
36) 1,2-Dichloropropane-d6	6.34	67	63914	4.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.20%
41) Toluene-d8	7.57	98	154436	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.40%
43) trans-1,3-Dichloropropene-	7.86	79	20213	4.08	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.60%
46) 2-Hexanone-d5	8.32	63	120769	47.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.22%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	50857	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.00%
64) 1,2-Dichlorobenzene-d4	11.87	152	63686	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
13) Acetone	2.33	43	8896	4.96 ug/L	94
17) Methyl tert-butyl Ether	3.01	73	39815	1.75 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050418\
Data File : VU023641.D
Acq On : 04 May 2018 20:10
Operator : MD/SY
Sample : J2630-14
Misc : 25mL/MSVOA U/WATER
ALS Vial : 38 Sample Multiplier: 1

Quant Time: May 05 01:33:19 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 05 01:17:03 2018
Response via : Initial Calibration

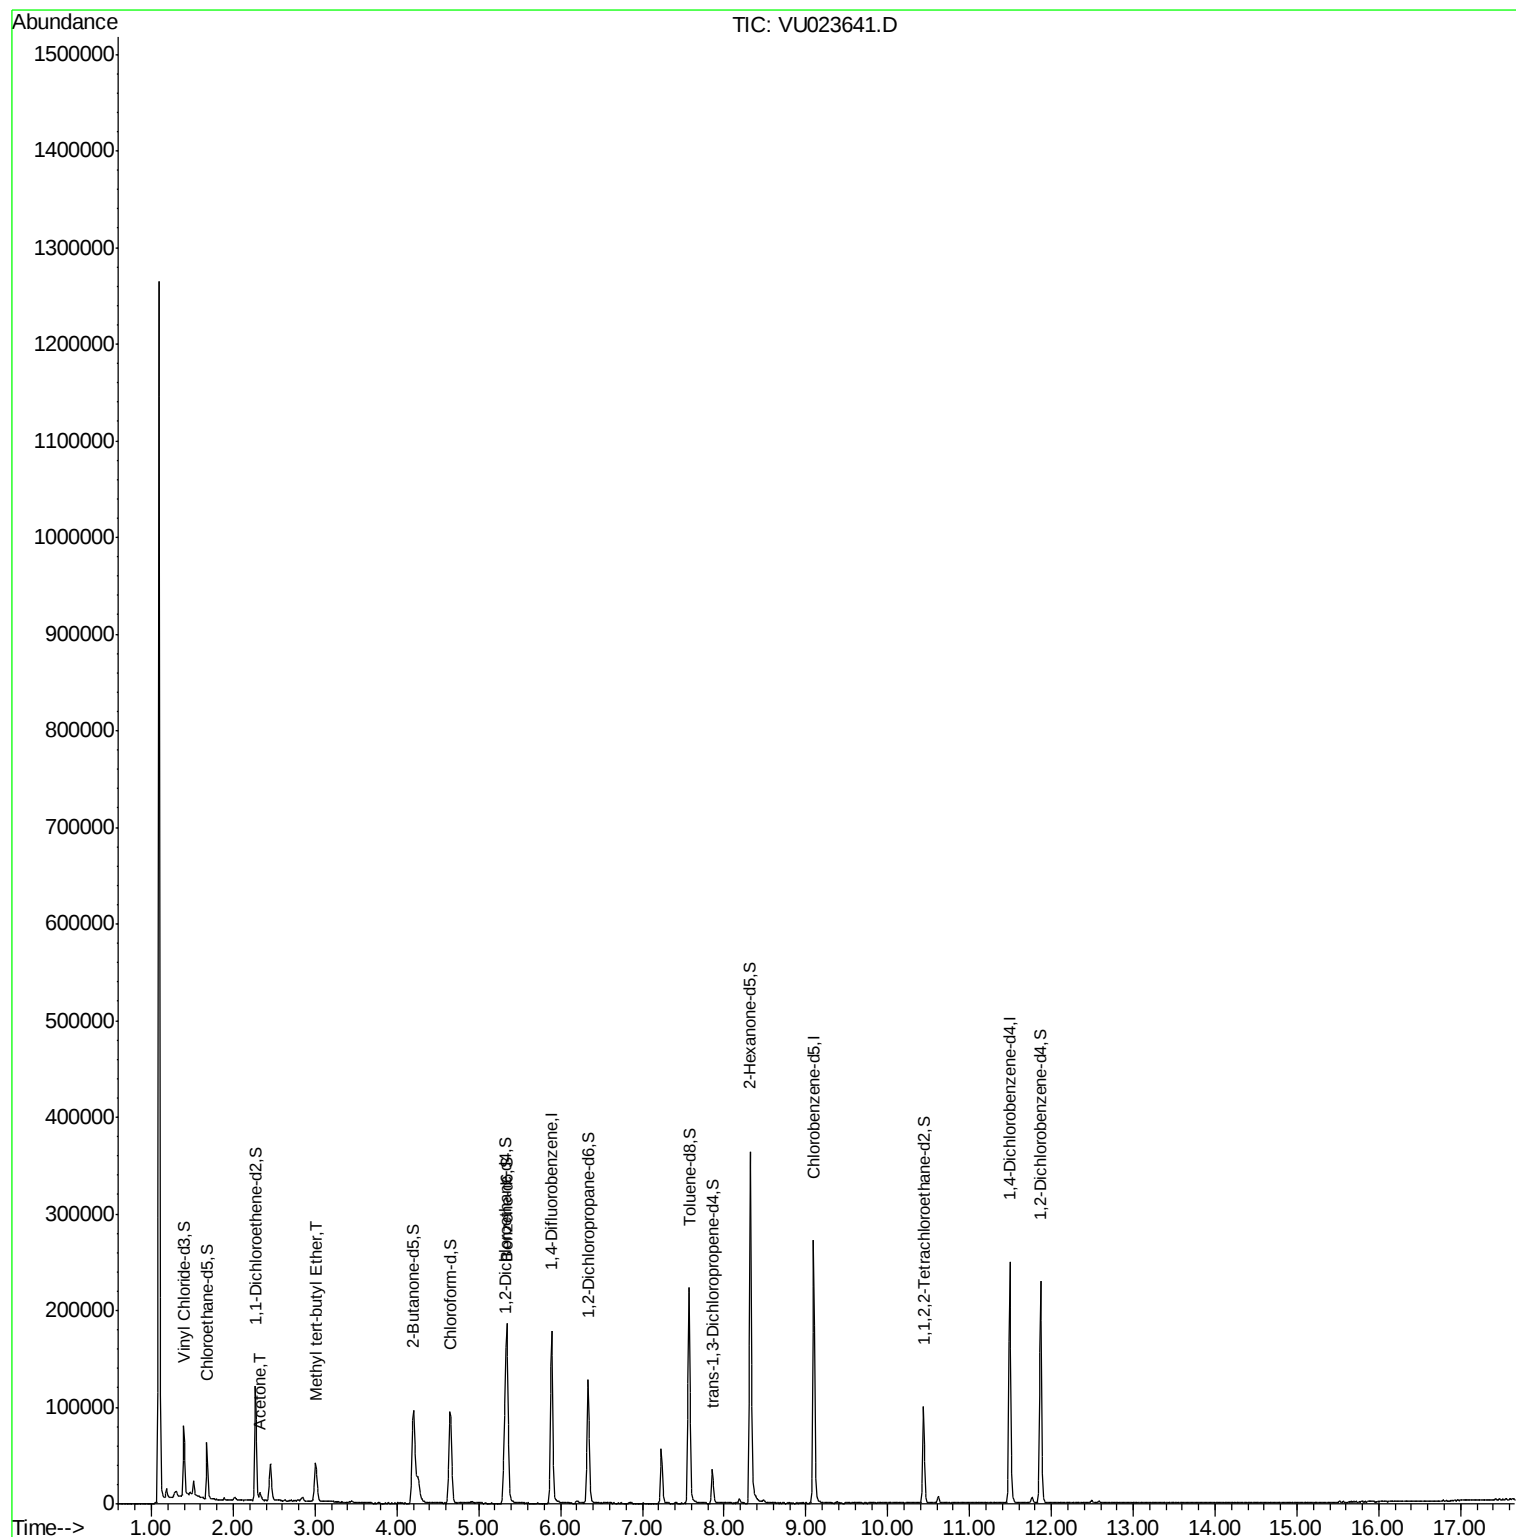

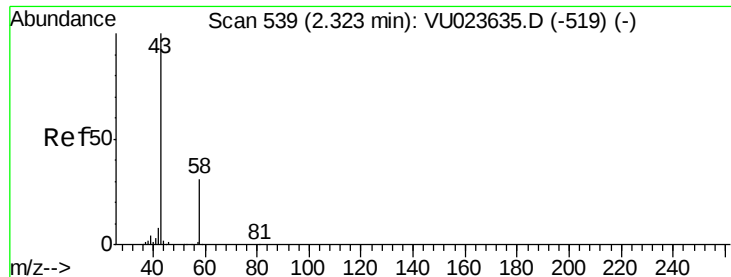

#13

Acetone

Concen: 4.96 ug/L

RT: 2.33 min Scan# 540

Delta R.T. 0.00 min

Lab File: VU023641.D





Acq: 04 May 2018 20:10

Tot Ion: 43 Resp: 8896

Ion Ratio Lower Upper

43 100

58 28.5 0.0 63.8

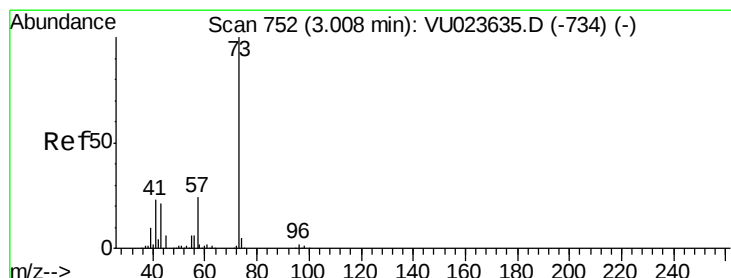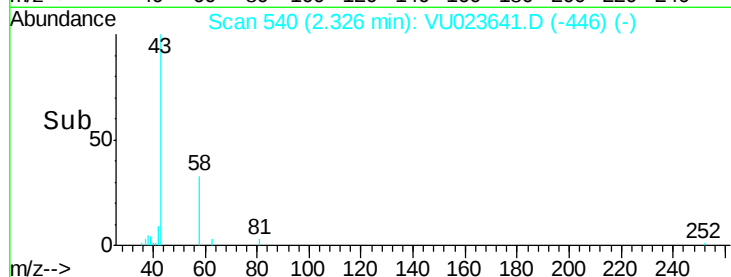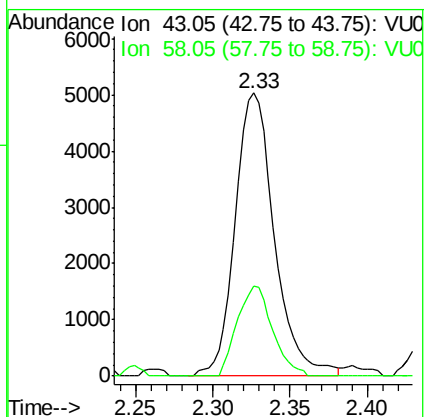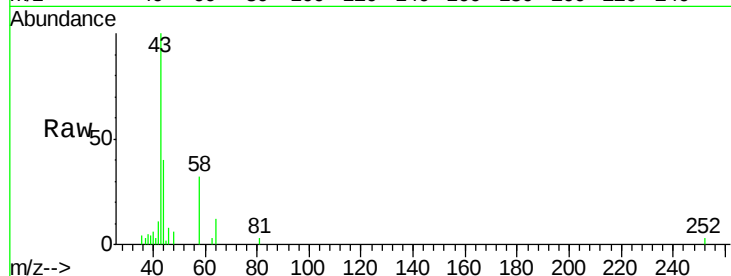

#17

Methyl tert-butyl Ether

Concen: 1.75 ug/L

RT: 3.01 min Scan# 752

Delta R.T. -0.00 min

Lab File: VU023641.D

Acq: 04 May 2018 20:10

Tgt Ion: 73 Resp: 39815

Ion Ratio Lower Upper

73 100

43 22.2 16.6 25.0

57 24.4 19.4 29.0

