

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050418\
 Data File : VU023650.D
 Acq On : 05 May 2018 00:01
 Operator : MD/SY
 Sample : J2630-17DL 50X
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Quant Time: May 05 01:52:30 2018
 Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 05 01:17:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	140614	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	144272	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	62391	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	44757	4.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.80%
7) Chloroethane-d5	1.68	69	38776	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.40%
11) 1,1-Dichloroethene-d2	2.27	63	67392	3.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.00%
20) 2-Butanone-d5	4.20	46	153260	51.94	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.88%
24) Chloroform-d	4.65	84	92069	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.32	65	51386	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.34	84	179762	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.34	67	63631	5.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.00%
41) Toluene-d8	7.57	98	150023	4.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.40%
43) trans-1,3-Dichloropropene-	7.86	79	18992	4.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.80%
46) 2-Hexanone-d5	8.32	63	119224	50.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.20%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	50013	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.60%
64) 1,2-Dichlorobenzene-d4	11.87	152	61454	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds


					Ovalue
5) Vinyl chloride	1.40	62	5975	0.45 ug/L	# 1
22) cis-1,2-Dichloroethene	4.23	96	82831	7.62 ug/L	99
34) Trichloroethene	6.19	95	2297	0.20 ug/L	86
47) Tetrachloroethene	8.23	164	2274	0.25 ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050418\
Data File : VU023650.D
Acq On : 05 May 2018 00:01
Operator : MD/SY
Sample : J2630-17DL 50X
Misc : 25mL/MSVOA U/WATER
ALS Vial : 47 Sample Multiplier: 1

Quant Time: May 05 01:52:30 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 05 01:17:03 2018
Response via : Initial Calibration

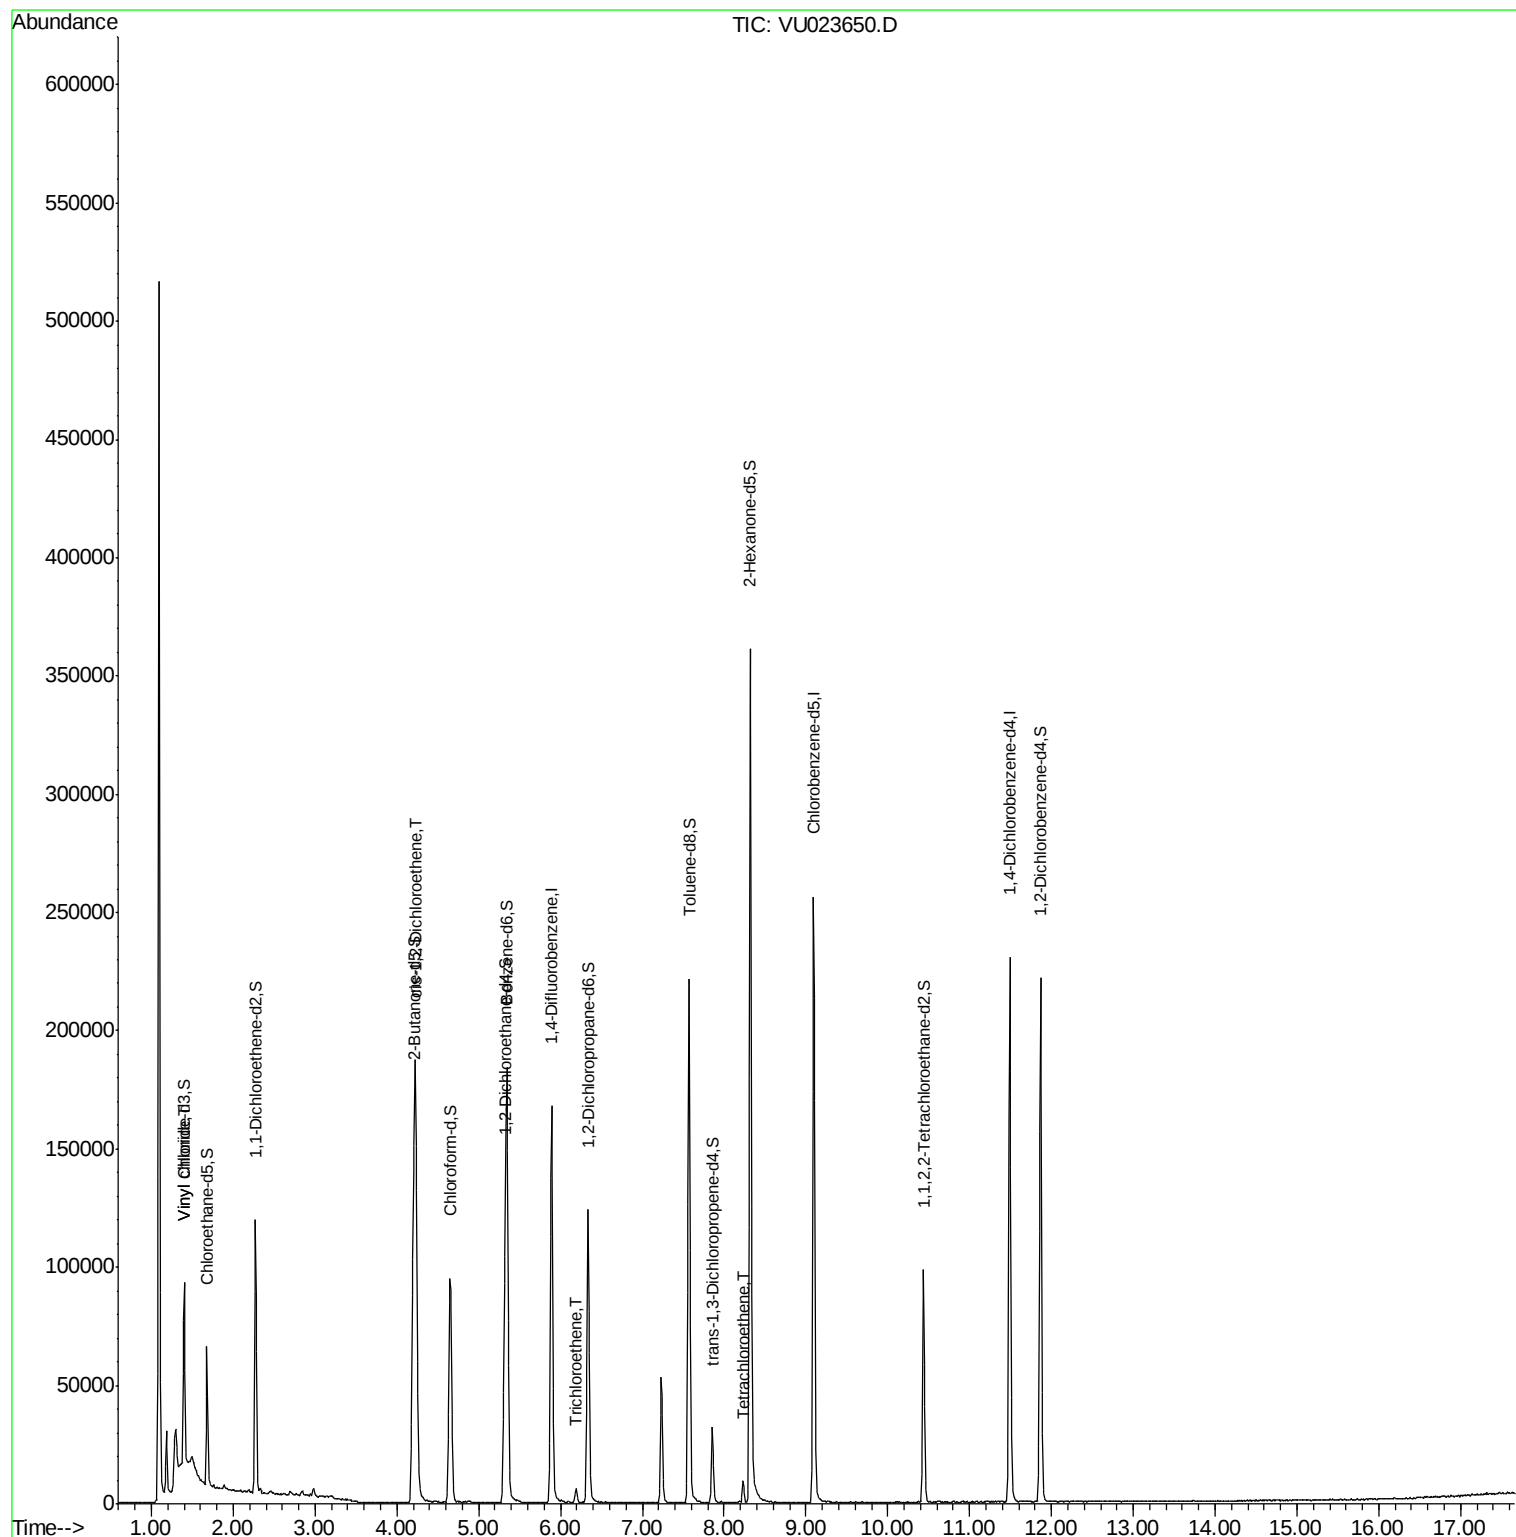

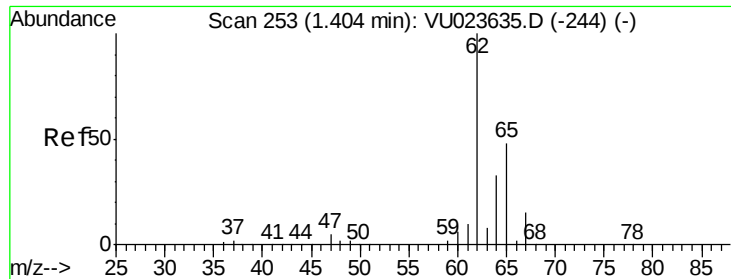

#5

Vinyl chloride

Concen: 0.45 ug/L

RT: 1.40 min Scan# 253

Delta R.T. 0.00 min

Lab File: VU023650.D


Acq: 05 May 2018 00:01

Tot Ion: 62 Resp: 5975

Ion Ratio Lower Upper




62 100

64 182.3 26.9 49.9#

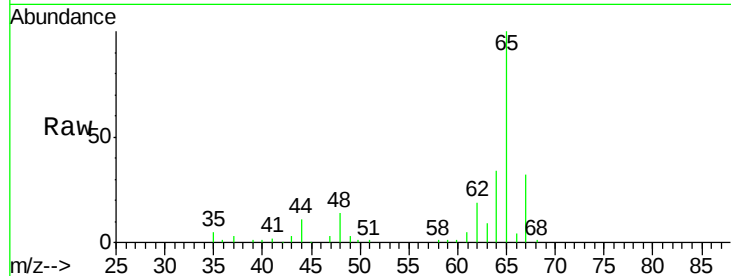

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 64.10 (63.80 to 64.80): VU0

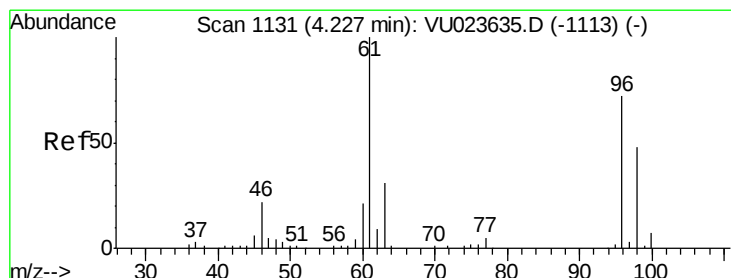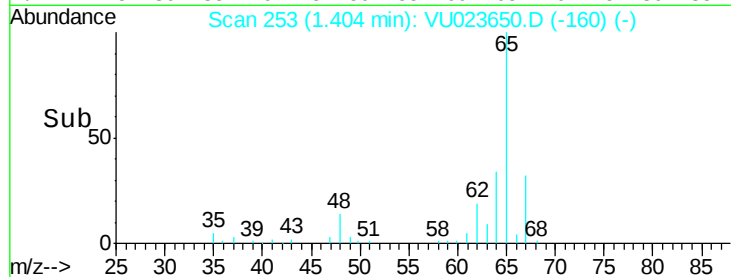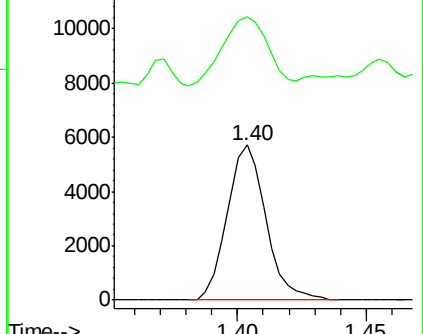

#22

cis-1,2-Dichloroethene

Concen: 7.62 ug/L

RT: 4.23 min Scan# 1131

Delta R.T. 0.00 min

Lab File: VU023650.D

Acq: 05 May 2018 00:01


Tgt Ion: 96 Resp: 82831

Ion Ratio Lower Upper

96 100

61 136.8 94.6 175.6



68 0.0 0.0 0.0

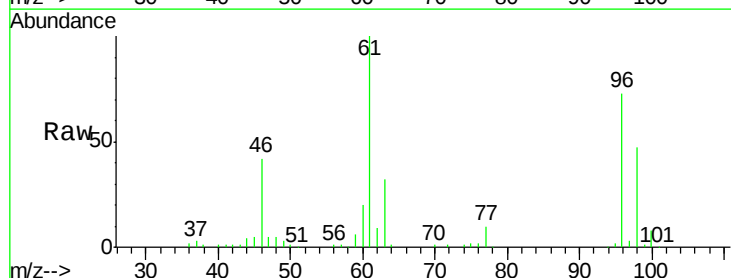


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 68.15 (67.85 to 68.85): VU0

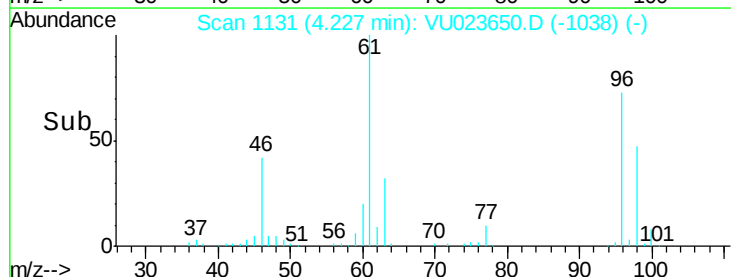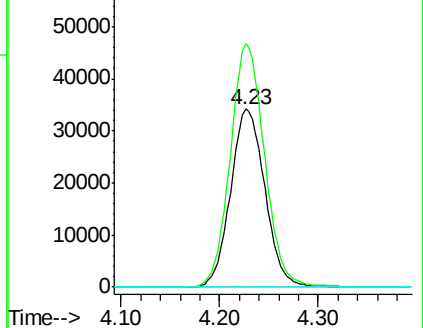

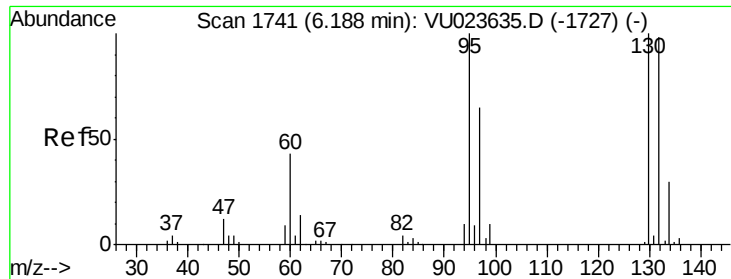

#34

Trichloroethene

Concen: 0.20 ug/L

RT: 6.19 min Scan# 1742

Delta R.T. 0.00 min

Lab File: VU023650.D

Acq: 05 May 2018 00:01

Tot Ion: 95 Resp: 2297



Ion Ratio Lower Upper

95 100

97 57.5 46.0 85.4

132 85.3 68.1 126.5

130 80.9 70.1 130.1

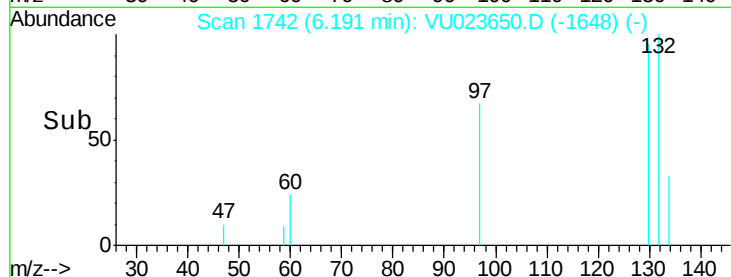
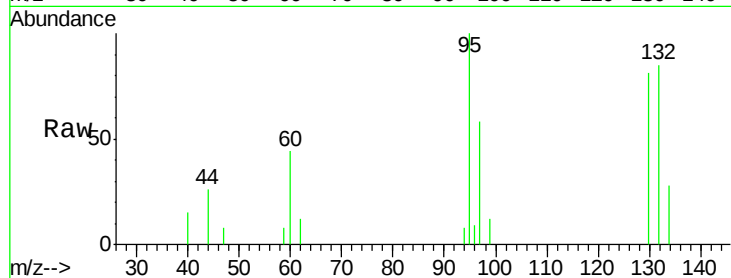


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

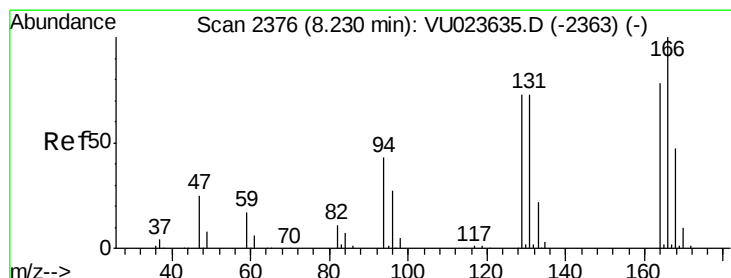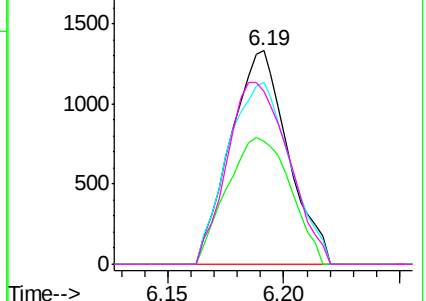

#47

Tetrachloroethene

Concen: 0.25 ug/L

RT: 8.23 min Scan# 2376

Delta R.T. 0.00 min

Lab File: VU023650.D

Acq: 05 May 2018 00:01

Tgt Ion: 164 Resp: 2274



Ion Ratio Lower Upper

164 100

129 100.3 64.4 119.6

131 89.6 63.9 118.7

166 134.9 90.0 167.2

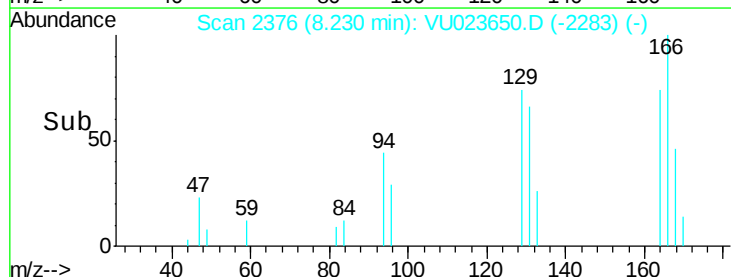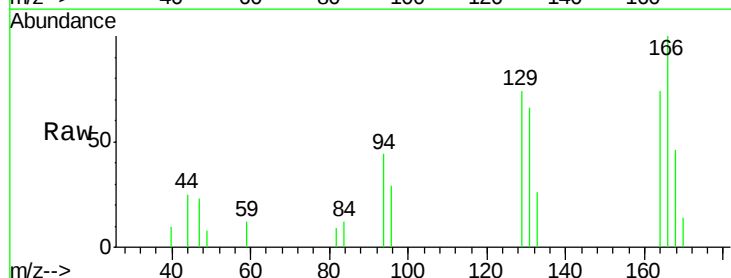

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

