


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050418\
Data File : VU023605.D
Acq On : 03 May 2018 16:36
Operator : MD/SY
Sample : BFB40
Misc : 25mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMUTR050418WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sun May 06 01:00:29 2018

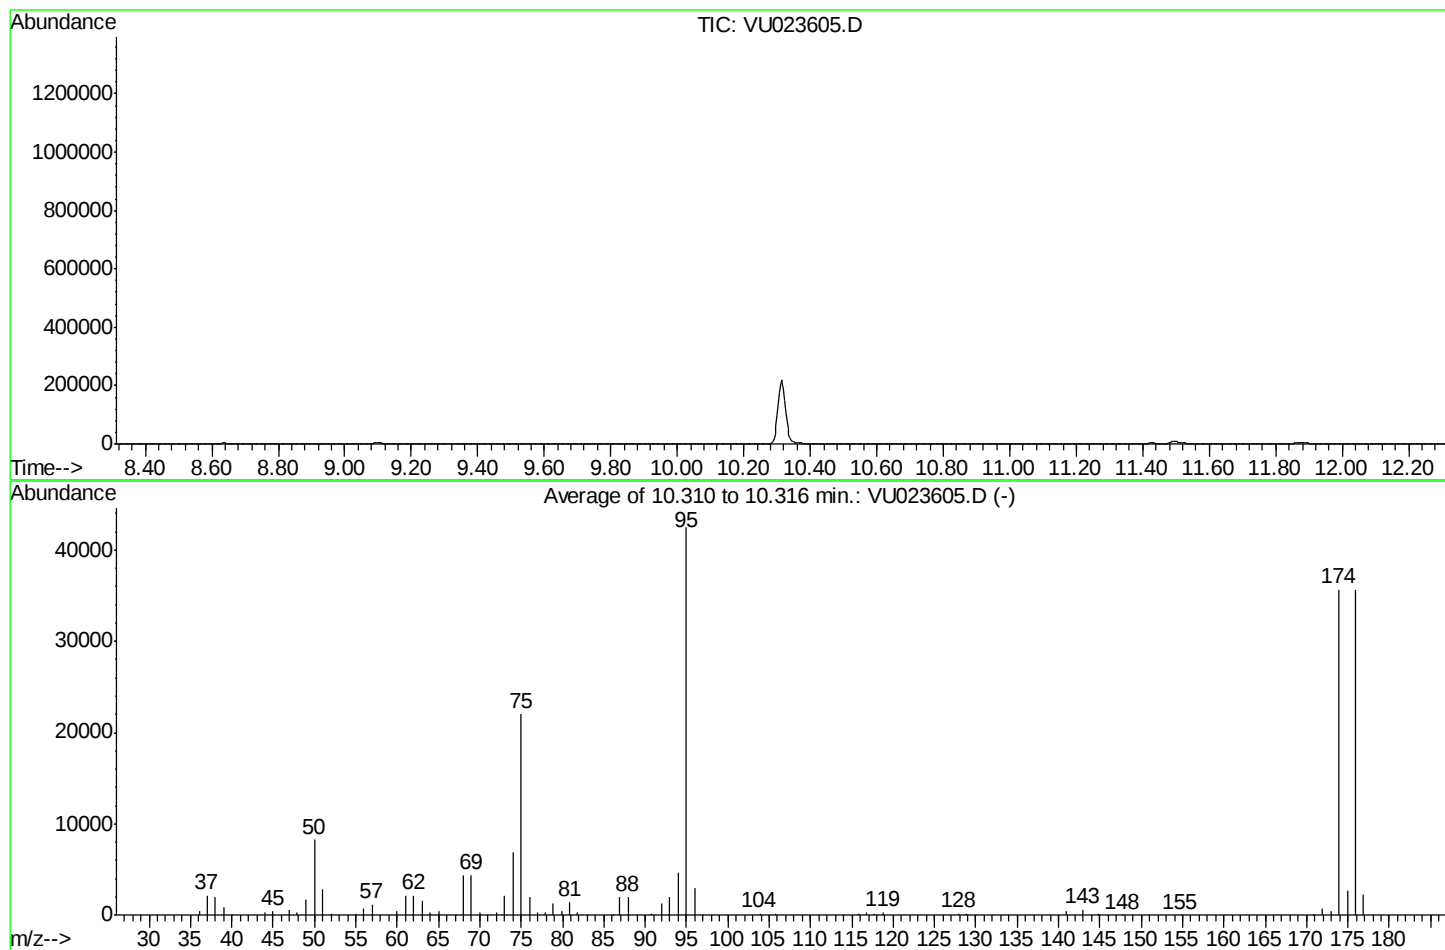

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	8216	PASS
75	95	30	80	51.9	22074	PASS
95	95	100	100	100.0	42498	PASS
96	95	5	9	6.8	2908	PASS
173	174	0.00	2	1.0	360	PASS
174	95	50	120	84.0	35714	PASS
175	174	5	9	7.5	2679	PASS
176	174	95	101	99.7	35616	PASS
177	176	5	9	6.4	2286	PASS

Scan 3011 (10.271 min): VU023605.D
BFB40

m/z	Abundance
39.90	206.0
44.00	636.0

m/z	Abundance
36.00	450.0
37.00	2087.0
38.00	1869.0
39.00	878.0
40.00	227.0
44.00	916.0
45.00	424.0
47.00	496.0
47.90	214.0
49.00	1719.0
50.00	8165.0
51.00	2750.0
52.00	155.0
54.90	127.0
56.00	671.0
57.00	1161.0
59.90	431.0
61.00	2161.0
62.00	2013.0
63.00	1629.0
63.90	270.0
65.00	515.0
68.00	4277.0
69.00	4435.0
69.90	321.0
72.00	249.0
73.00	2028.0
74.00	6778.0
75.00	21928.0
76.00	1979.0
77.00	281.0
77.90	214.0
78.90	1301.0
79.90	393.0
80.90	1344.0
81.80	321.0
86.90	2020.0
87.90	1920.0
90.80	171.0
92.00	1224.0
93.00	1897.0
94.00	4613.0
95.00	41472.0
96.00	3004.0
103.90	200.0
105.80	141.0
115.90	129.0
116.80	245.0
117.70	152.0
118.80	309.0
127.90	187.0
130.00	106.0
140.90	349.0
143.00	545.0
144.80	157.0
171.90	568.0
173.90	33744.0
174.90	2574.0
175.90	34248.0
176.90	2081.0

m/z	Abundance
36.00	421.0
37.00	2241.0
38.00	2034.0
39.00	906.0
40.00	221.0
44.00	927.0
44.90	439.0
47.00	551.0
48.00	232.0
49.00	1707.0
50.00	8473.0
51.00	2909.0
52.00	189.0
55.00	134.0
56.00	738.0
57.00	1176.0
59.90	419.0
61.00	2197.0
62.00	2201.0
63.00	1662.0
63.90	310.0
65.00	488.0
67.00	101.0
68.00	4458.0
69.00	4518.0
70.00	303.0
72.00	248.0
73.00	2180.0
74.00	7139.0
75.00	22760.0
76.00	2001.0
77.00	233.0
77.90	269.0
78.90	1332.0
79.90	423.0
80.90	1475.0
81.90	332.0
86.90	2011.0
87.90	2041.0
90.80	185.0
92.00	1339.0
93.00	2015.0
94.00	4739.0
95.00	43784.0
96.00	3024.0
97.00	103.0
103.90	189.0
105.90	150.0
115.80	143.0
116.80	282.0
117.70	171.0
118.80	318.0
128.00	203.0
128.80	113.0
129.80	107.0
140.90	406.0
142.90	581.0
144.80	160.0
147.80	100.0
154.80	104.0
170.80	101.0
171.90	665.0
173.00	555.0
173.90	36936.0
174.90	2736.0
175.90	36792.0
176.90	2361.0

Scan 3025 (10.316 min): VU023605.D
BFB40

m/z	Abundance
36.10	366.0
37.00	2151.0
38.00	1959.0
39.00	874.0
40.00	225.0
44.00	897.0
44.90	418.0
47.00	593.0
48.00	210.0
49.00	1519.0
50.00	8010.0
51.00	2614.0
52.00	166.0
55.00	121.0
56.00	688.0
57.00	1106.0
59.90	338.0
61.00	1932.0
62.00	2126.0
63.00	1555.0
64.00	321.0
65.00	447.0
67.00	115.0
68.00	4206.0
69.00	4159.0
70.00	265.0
72.00	215.0
73.00	2083.0
74.00	6924.0
75.00	21536.0
76.00	1864.0
77.00	210.0
77.90	279.0
78.90	1204.0
79.90	393.0
80.90	1423.0
81.90	302.0
86.10	102.0
86.90	1773.0
87.90	2031.0
90.80	190.0
92.00	1276.0
93.00	1925.0
94.00	4730.0
95.00	42240.0
96.00	2697.0
97.00	101.0
103.80	195.0
105.90	133.0
115.80	160.0
116.80	318.0
117.80	176.0
118.90	280.0
128.00	185.0
128.80	121.0
140.90	419.0
142.90	591.0
144.90	146.0
147.80	103.0
154.80	105.0
171.90	704.0
172.90	527.0
173.90	36464.0
174.90	2728.0
175.90	35808.0
176.90	2418.0