


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050418\
 Data File : VU023634.D
 Acq On : 04 May 2018 16:09
 Operator : MD/SY
 Sample : BFB41
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMUTR050418WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sun May 06 01:00:29 2018

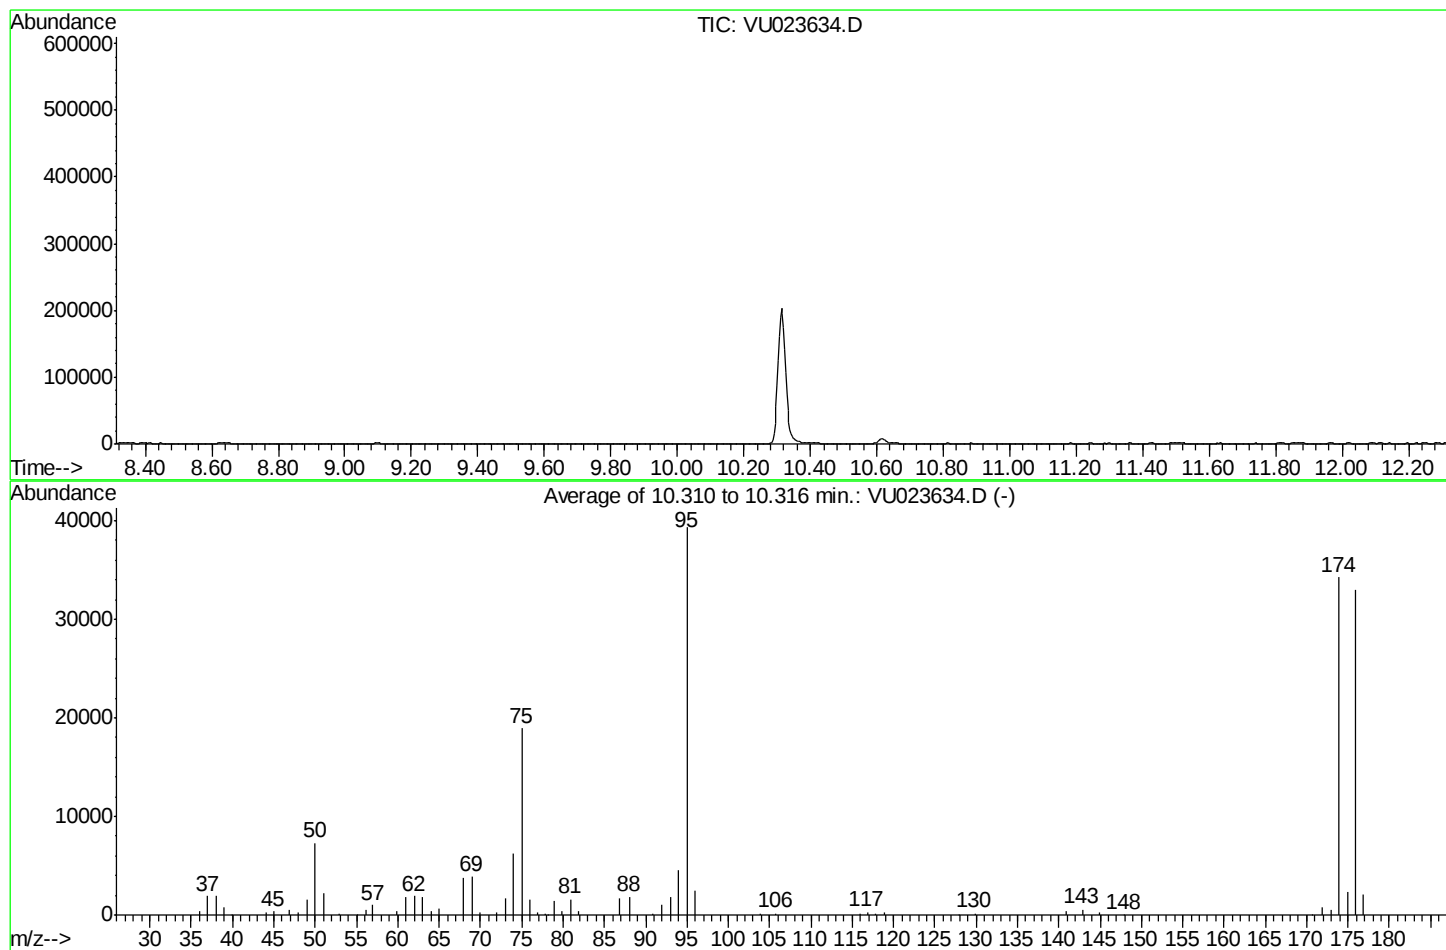

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	7271	PASS
75	95	30	80	48.2	18944	PASS
95	95	100	100	100.0	39317	PASS
96	95	5	9	6.4	2506	PASS
173	174	0.00	2	1.5	523	PASS
174	95	50	120	87.1	34232	PASS
175	174	5	9	6.8	2321	PASS
176	174	95	101	96.4	33008	PASS
177	176	5	9	6.2	2030	PASS

Scan 3011 (10.271 min): VU023634.D
BFB41

m/z	Abundance
39.90	182.0
44.00	489.0
206.90	101.0

m/z	Abundance
35.90	348.0
37.00	1845.0
38.00	1883.0
39.00	775.0
39.90	246.0
44.00	751.0
45.00	350.0
46.90	576.0
47.90	252.0
49.00	1628.0
50.00	7322.0
51.00	2271.0
52.80	123.0
55.00	109.0
56.10	537.0
57.00	992.0
59.90	384.0
61.00	1867.0
62.00	1867.0
63.00	1745.0
64.00	351.0
65.00	588.0
68.00	3766.0
69.00	3896.0
70.00	276.0
71.90	235.0
73.00	1688.0
74.00	6137.0
75.00	18248.0
76.00	1546.0
76.90	281.0
77.80	151.0
78.90	1329.0
79.80	332.0
80.90	1587.0
81.80	290.0
86.90	1617.0
88.00	1843.0
90.90	132.0
92.00	1029.0
92.90	1868.0
94.00	4420.0
95.00	38192.0
96.00	2427.0
103.80	127.0
105.80	164.0
115.90	148.0
116.80	262.0
117.80	141.0
118.80	279.0
127.90	103.0
129.80	153.0
140.90	324.0
142.90	607.0
144.80	211.0
147.90	103.0
171.90	696.0
172.90	535.0
173.90	32440.0
174.90	2170.0
175.90	31144.0
176.90	1938.0

m/z	Abundance
35.90	333.0
37.00	1948.0
38.00	1989.0
39.00	802.0
39.90	251.0
44.00	781.0
45.00	334.0
46.90	613.0
47.90	230.0
49.00	1604.0
50.00	7457.0
51.00	2311.0
52.80	116.0
56.10	575.0
57.00	1070.0
59.90	423.0
61.00	1859.0
62.00	1937.0
63.00	1863.0
64.00	384.0
65.00	700.0
68.00	3923.0
69.00	4011.0
70.00	281.0
71.90	197.0
73.00	1791.0
74.00	6495.0
75.00	19512.0
76.00	1589.0
76.90	299.0
77.80	148.0
78.90	1398.0
79.90	352.0
80.90	1649.0
81.80	394.0
86.90	1824.0
88.00	1950.0
90.90	139.0
92.00	1045.0
92.90	1897.0
94.00	4754.0
95.00	40640.0
96.00	2574.0
103.90	116.0
105.80	188.0
115.90	156.0
116.80	317.0
117.90	136.0
118.80	273.0
129.90	158.0
140.90	363.0
142.90	549.0
144.90	226.0
147.90	104.0
171.90	777.0
172.90	541.0
173.90	35328.0
174.90	2396.0
175.90	34144.0
176.90	2098.0
206.90	109.0

m/z	Abundance
36.00	314.0
37.00	1956.0
38.00	1853.0
39.00	798.0
39.90	224.0
44.00	781.0
45.00	308.0
46.90	558.0
47.90	209.0
49.00	1464.0
50.00	7034.0
51.00	2150.0
52.90	100.0
56.10	536.0
56.90	1012.0
59.90	404.0
61.00	1719.0
62.00	1880.0
63.00	1801.0
64.00	363.0
65.00	725.0
68.00	3803.0
69.00	3769.0
69.90	283.0
72.00	195.0
73.00	1723.0
74.00	6207.0
75.00	19072.0
76.00	1565.0
76.90	285.0
78.10	158.0
78.90	1416.0
79.90	375.0
80.90	1482.0
81.80	444.0
86.90	1801.0
88.00	1758.0
90.80	140.0
92.00	961.0
93.00	1712.0
94.00	4569.0
95.00	39120.0
96.00	2518.0
103.90	111.0
105.80	203.0
115.90	156.0
116.80	363.0
117.90	113.0
118.90	280.0
129.90	155.0
140.80	361.0
142.90	498.0
144.90	233.0
170.70	122.0
171.90	739.0
172.90	494.0
173.90	34928.0
174.90	2398.0
175.90	33736.0
176.90	2054.0
206.90	110.0