


Methylene Chloride

Response Ratio

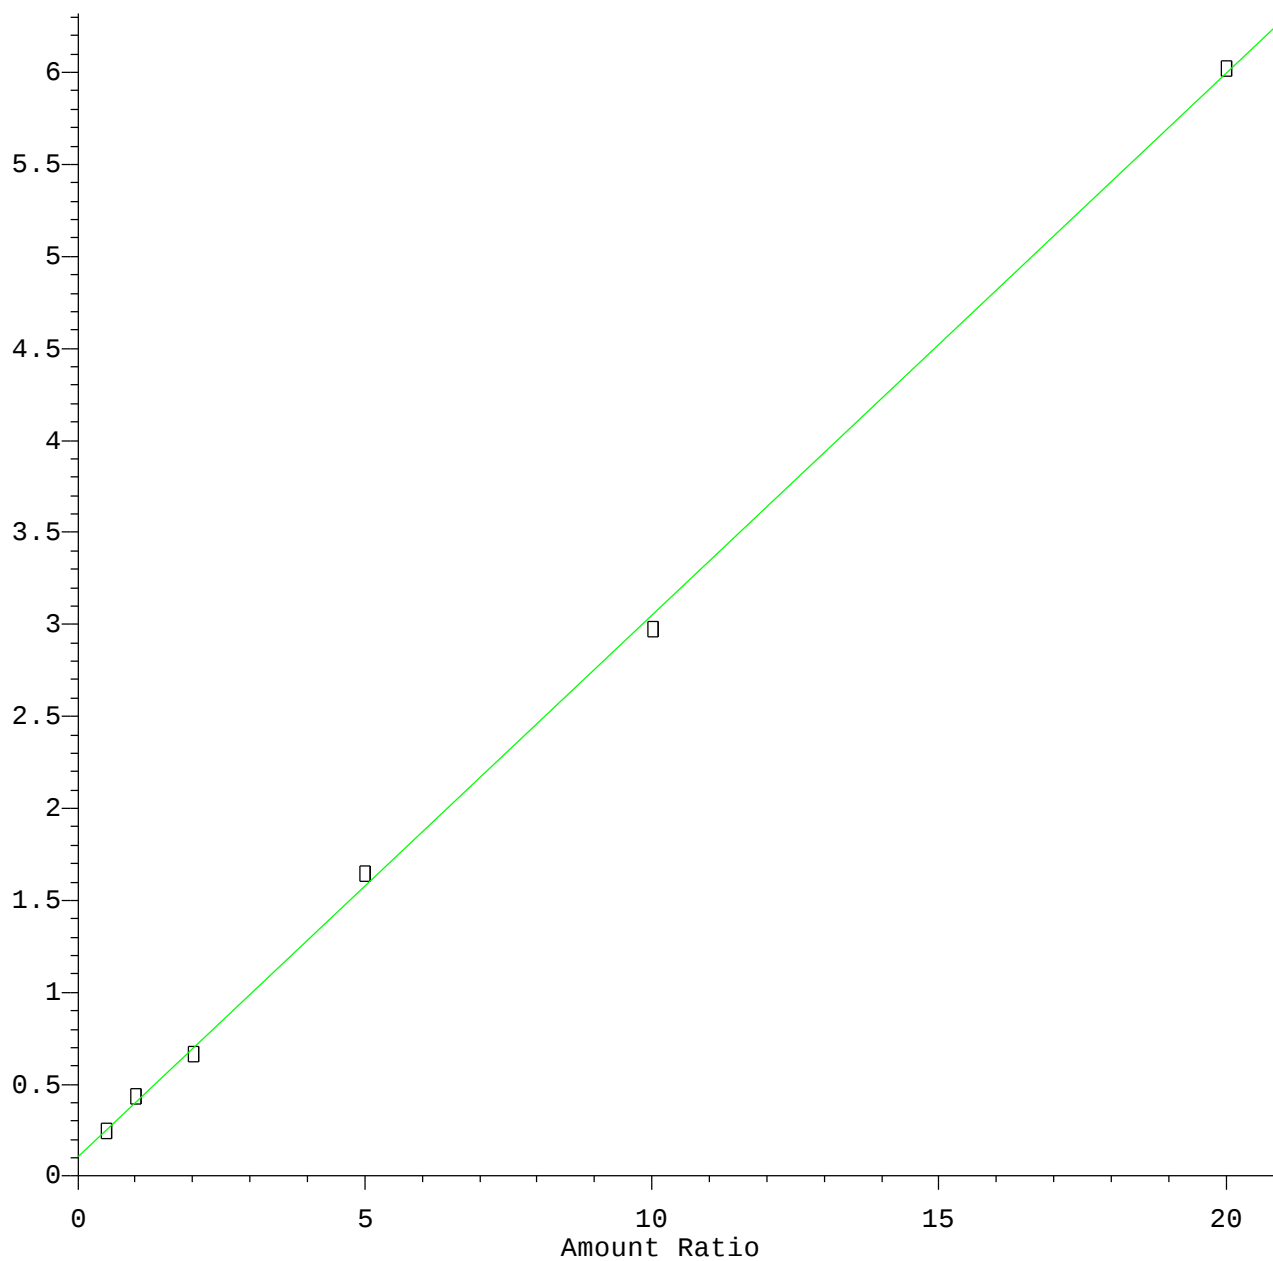


Resp Ratio = $2.94 \times 10^{-1} \times \text{Amt} + 1.05 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
Calibration Table Last Updated: Tue May 05 02:20:02 2020

Iodomethane

Response Ratio

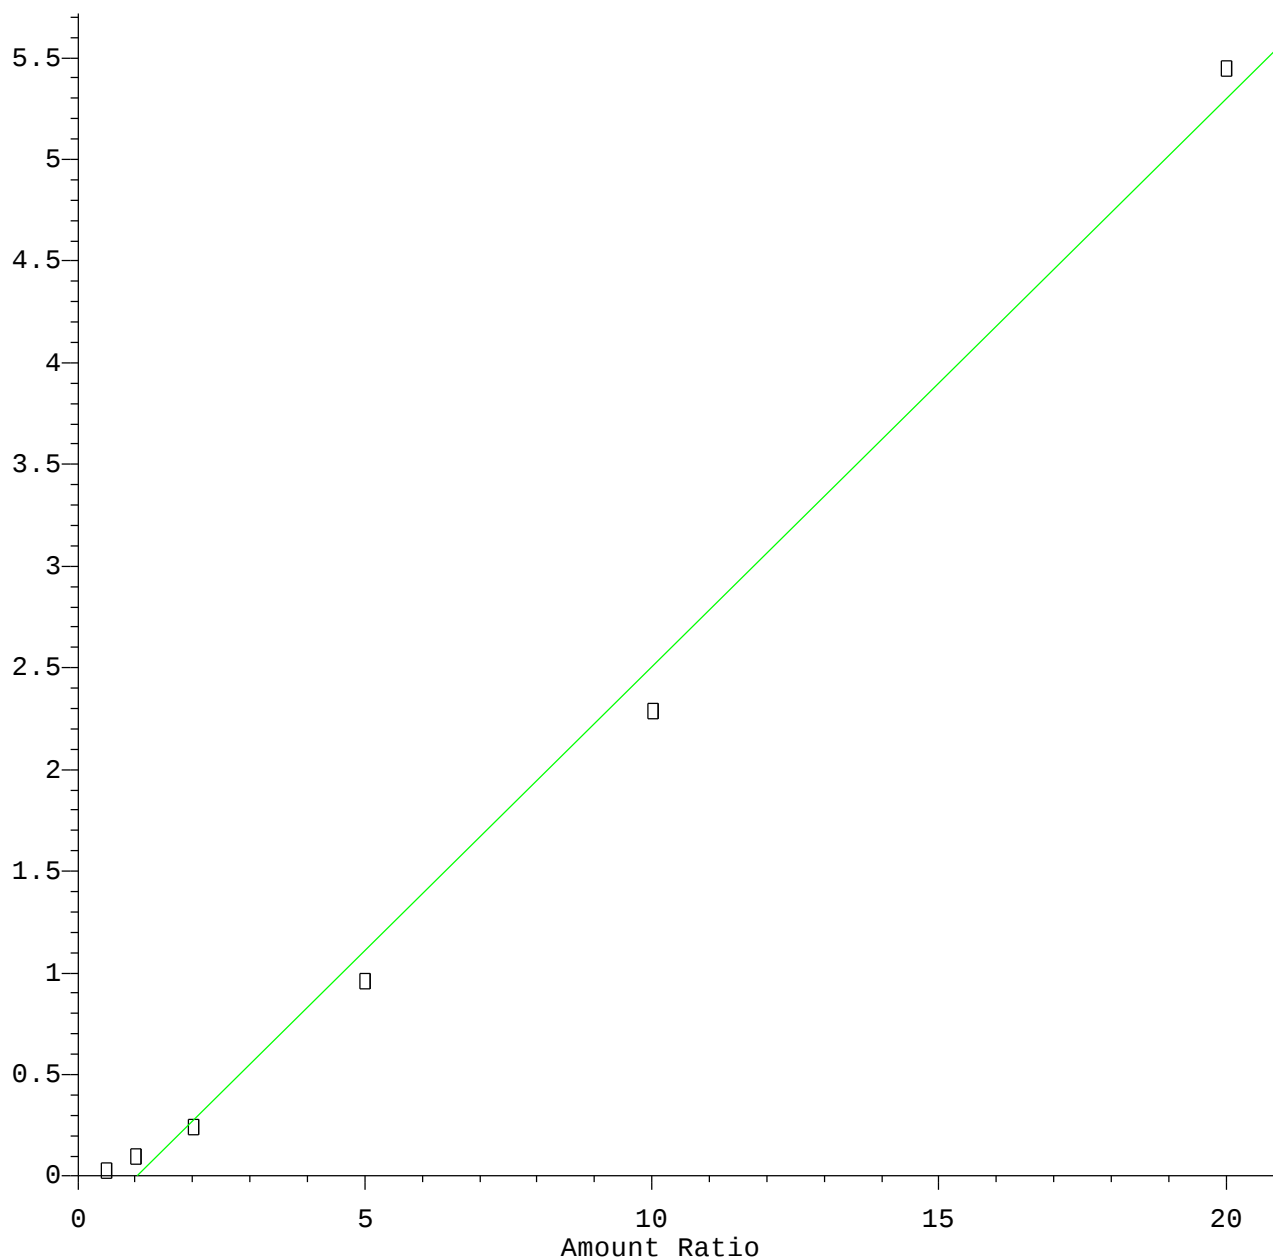


Resp Ratio = $2.79 \times 10^{-1} \times \text{Amt} - 2.84 \times 10^{-1}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
Calibration Table Last Updated: Tue May 05 02:20:02 2020

Iodomethane

Response Ratio

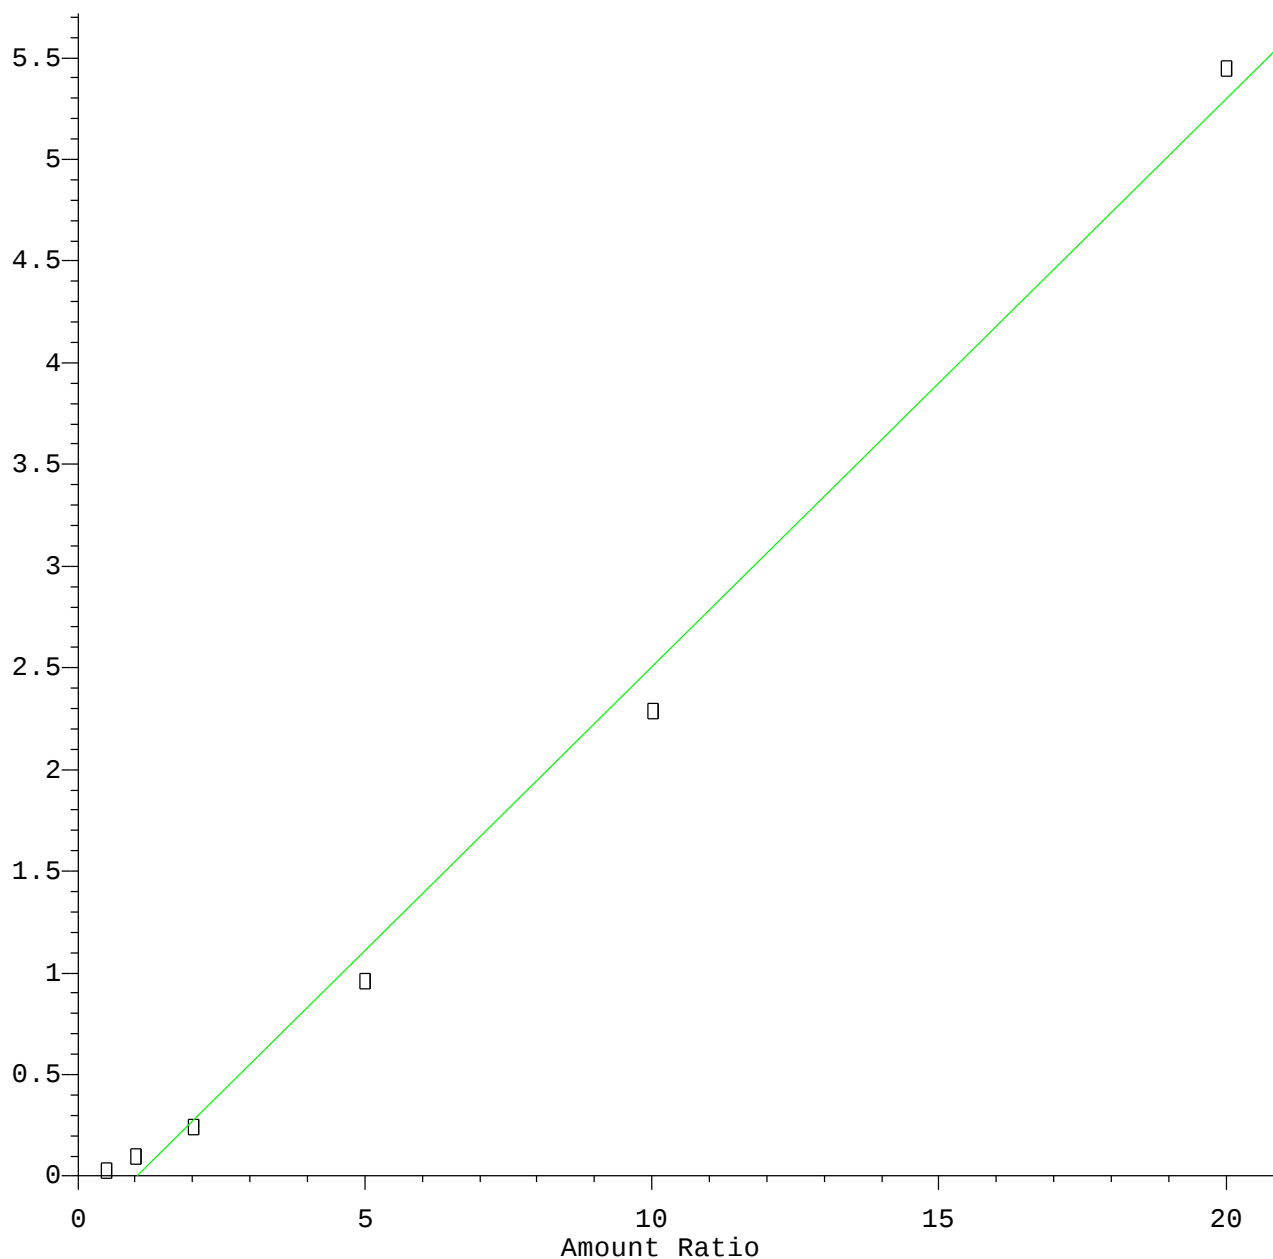

Resp Ratio = $2.79 \times 10^{-1} \times \text{Amt} - 2.84 \times 10^{-1}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
Calibration Table Last Updated: Tue May 05 02:20:02 2020