

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050420\
 Data File : VU038003.D
 Acq On : 04 May 2020 15:55
 Operator : JC/MD
 Sample : VU0504WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0504WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U050420DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.707	1031	1047	1065	rBV	14045	36066	17.88%	4.712%
2	5.118	1160	1175	1177	rBV4	2955	4850	2.40%	0.634%
3	5.420	1259	1269	1282	rVB6	2323	4135	2.05%	0.540%
4	6.147	1478	1495	1510	rBV	96918	192607	95.47%	25.162%
5	6.575	1617	1628	1635	rBV8	3501	6939	3.44%	0.907%
6	6.787	1685	1694	1702	rBV7	2086	3261	1.62%	0.426%
7	7.822	2004	2016	2027	rBV4	5662	11308	5.61%	1.477%
8	7.919	2038	2046	2055	rBV7	2009	3158	1.57%	0.413%
9	8.356	2175	2182	2192	rBV3	1677	2189	1.09%	0.286%
10	8.571	2243	2249	2258	rVB6	3696	5729	2.84%	0.748%
11	8.713	2285	2293	2304	rVB4	4372	8057	3.99%	1.053%
12	8.947	2360	2366	2381	rVB8	3180	5673	2.81%	0.741%
13	9.452	2508	2523	2525	rBV7	2194	4005	1.99%	0.523%
14	9.587	2556	2565	2572	rBV3	2534	3623	1.80%	0.473%
15	9.710	2593	2603	2614	rBV5	3884	6014	2.98%	0.786%
16	10.131	2722	2734	2741	rVB6	4076	6915	3.43%	0.903%
17	10.504	2842	2850	2855	rBV4	3534	4593	2.28%	0.600%
18	10.648	2885	2895	2907	rBV2	90346	142891	70.83%	18.667%
19	10.922	2974	2980	2991	rVB6	1976	3199	1.59%	0.418%
20	11.105	3028	3037	3046	rBV7	3382	6508	3.23%	0.850%
21	11.330	3096	3107	3119	rVB7	4369	7903	3.92%	1.032%
22	11.478	3146	3153	3154	rBV2	2816	2553	1.27%	0.334%
23	11.761	3232	3241	3248	rVB6	5106	7087	3.51%	0.926%
24	11.828	3248	3262	3265	rBV7	7146	12243	6.07%	1.599%
25	11.848	3265	3268	3277	rVB6	5549	7967	3.95%	1.041%
26	12.208	3368	3380	3393	rBV2	119562	201744	100.00%	26.356%
27	12.912	3594	3599	3609	rVB6	1616	2384	1.18%	0.311%
28	13.044	3630	3640	3653	rBV3	10851	16824	8.34%	2.198%
29	13.246	3696	3703	3712	rVB5	2625	3116	1.54%	0.407%
30	13.471	3767	3773	3781	rVB6	3385	4597	2.28%	0.601%
31	13.867	3888	3896	3906	rVB4	9170	14510	7.19%	1.896%
32	14.118	3965	3974	3983	rBV2	7518	10489	5.20%	1.370%
33	14.362	4042	4050	4060	rBV6	7626	12334	6.11%	1.611%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050420\
Data File : VU038003.D
Acq On : 04 May 2020 15:55
Operator : JC/MD
Sample : VU0504WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0504WBL01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER


Sum of corrected areas: 765471

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050420\
Data File : VU038003.D
Acq On : 04 May 2020 15:55
Operator : JC/MD
Sample : VU0504WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0504WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U050420DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

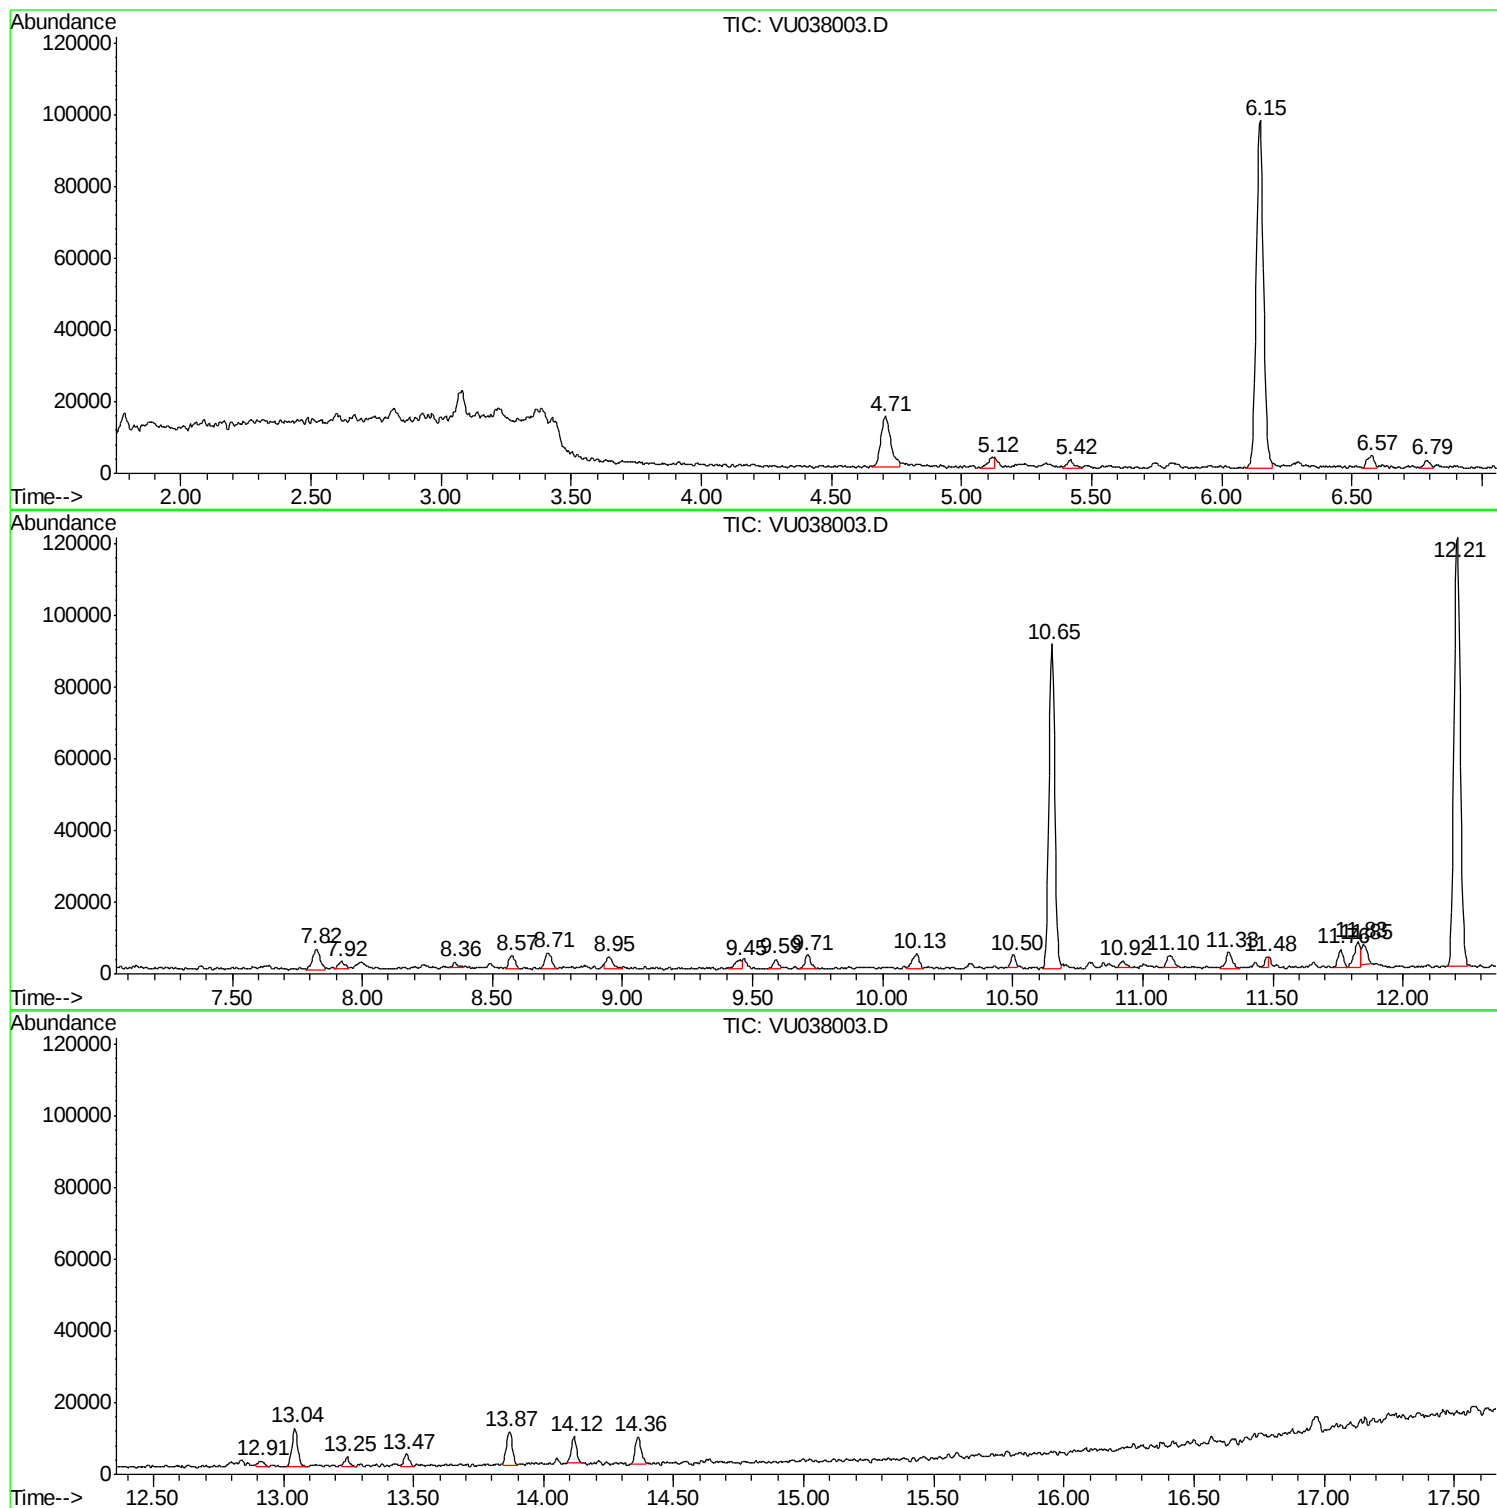

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050420\
Data File : VU038003.D
Acq On : 04 May 2020 15:55
Operator : JC/MD
Sample : VU0504WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0504WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050420\
Data File : VU038003.D
Acq On : 04 May 2020 15:55
Operator : JC/MD
Sample : VU0504WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0504WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc