


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU050420\
 Data File : VU037995.D
 Acq On : 04 May 2020 10:08
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Tue May 05 02:20:02 2020

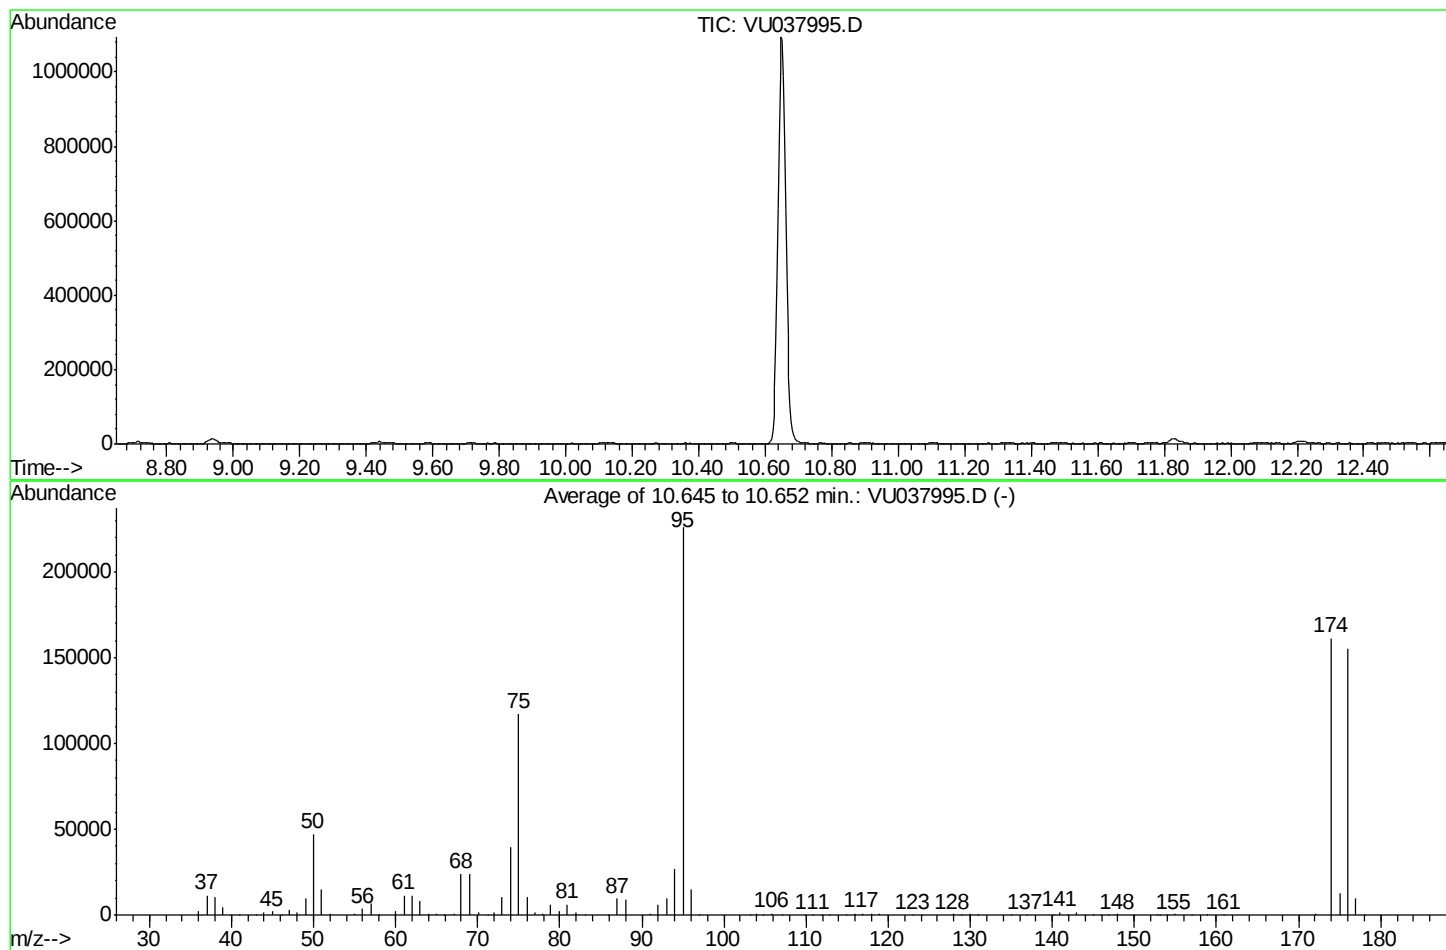

AutoFind: Scans 2894, 2895, 2896; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	47258	PASS
75	95	30	60	51.9	117368	PASS
95	95	100	100	100.0	225962	PASS
96	95	5	9	6.6	14914	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.4	161301	PASS
175	174	5	9	7.8	12618	PASS
176	174	95	101	96.2	155178	PASS
177	176	5	9	6.3	9844	PASS