


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043528.D
Acq On : 04 May 2021 18:34
Operator : SY/MD
Sample : M2195-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3J6

Manual Integrations
APPROVED

MMDadoda
5/6/2021 11:32:54 AM

Quant Time: May 05 08:13:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 05 08:11:40 2021
Response via : Initial Calibration

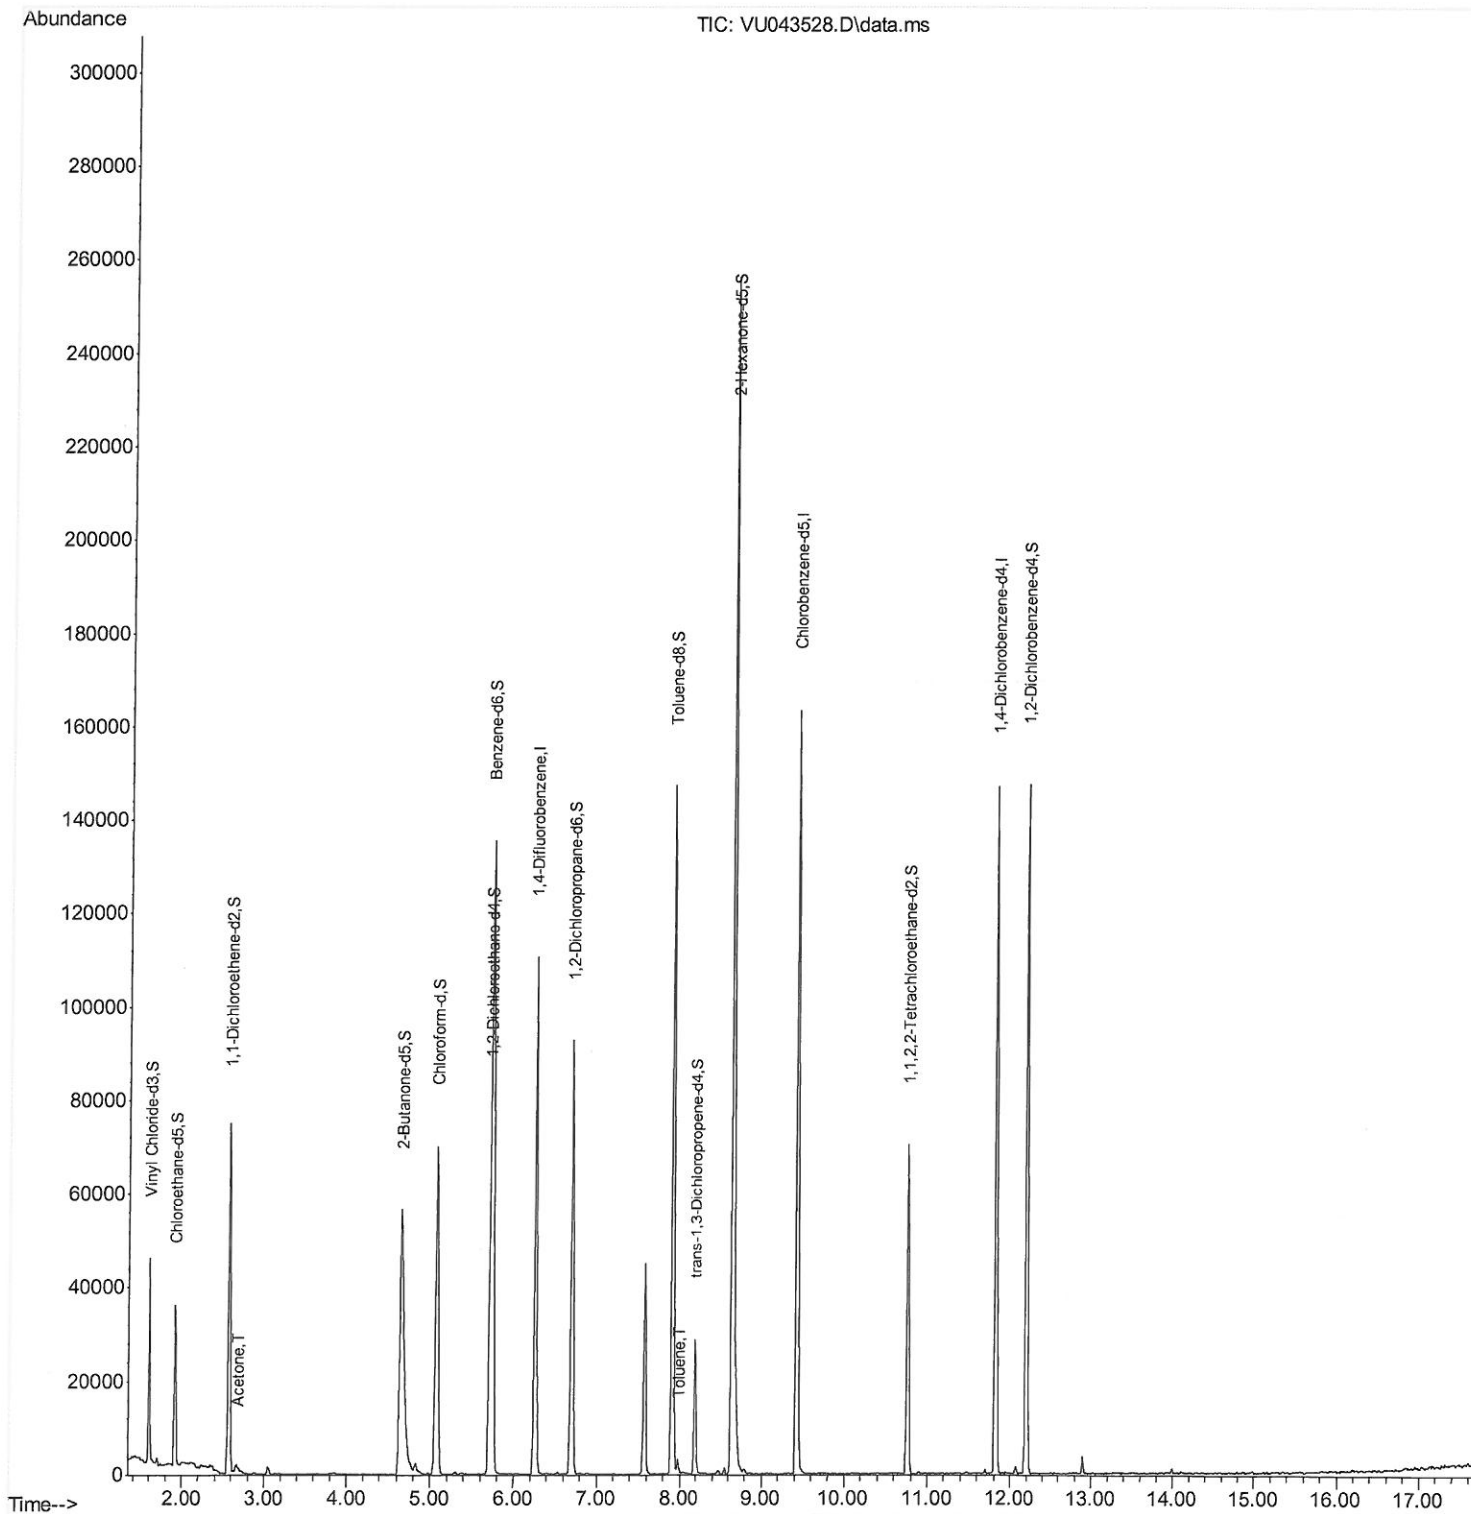

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
 Data File : VU043528.D
 Acq On : 04 May 2021 18:34
 Operator : SY/MD
 Sample : M2195-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB3J6

Manual Integrations
 APPROVED

MMDadoda
 5/6/2021 11:32:54 AM

Quant Time: May 05 08:13:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 05 08:11:40 2021
 Response via : Initial Calibration

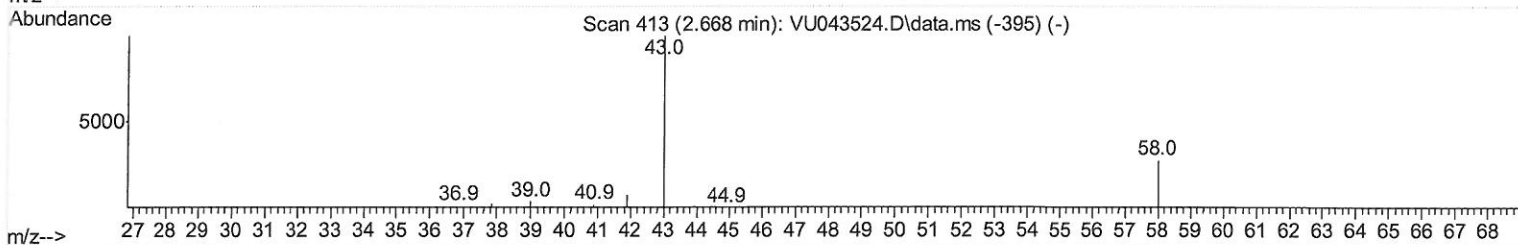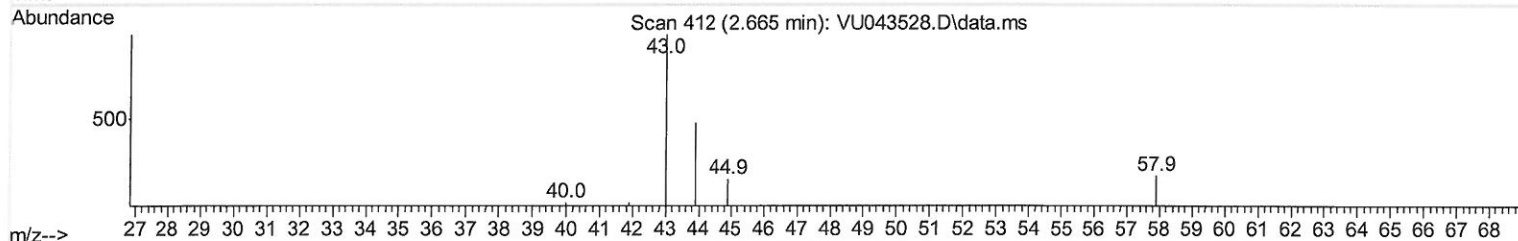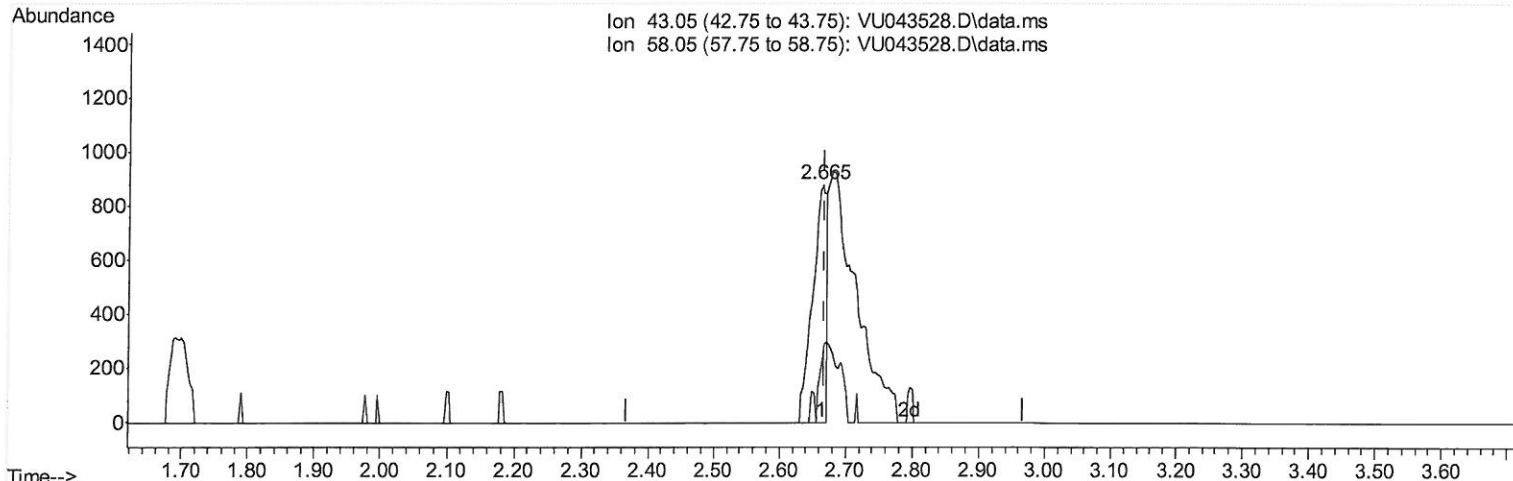

TIC: VU043528.D\data.ms

(13) Acetone (T)

2.665min (-0.003) 1.00 ug/L

response 1333

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.40	34.13
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043528.D
Acq On : 04 May 2021 18:34
Operator : SY/MD
Sample : M2195-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3J6

Manual Integrations
APPROVED

MMDadoda
5/6/2021 11:32:54 AM

Quant Time: May 05 08:13:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 05 08:11:40 2021
Response via : Initial Calibration

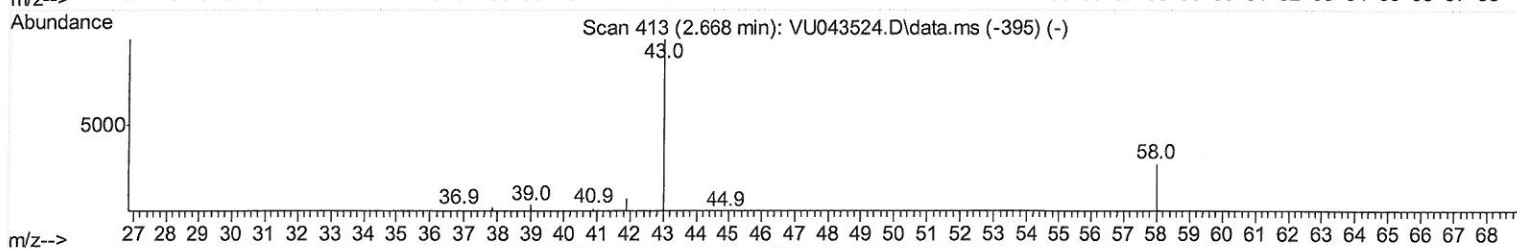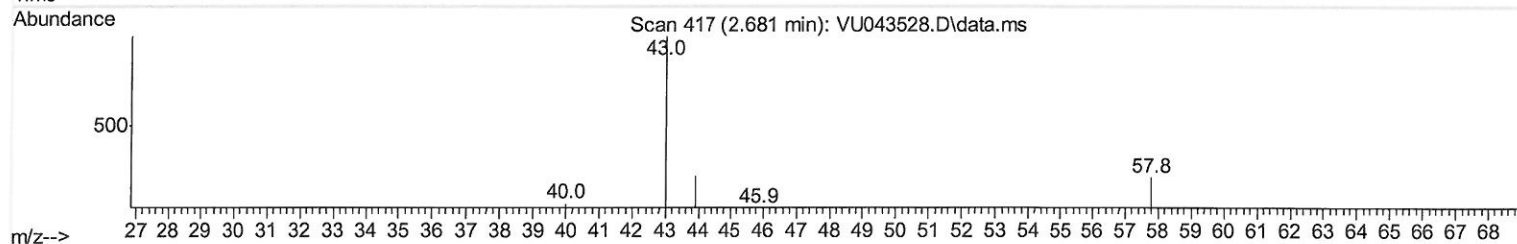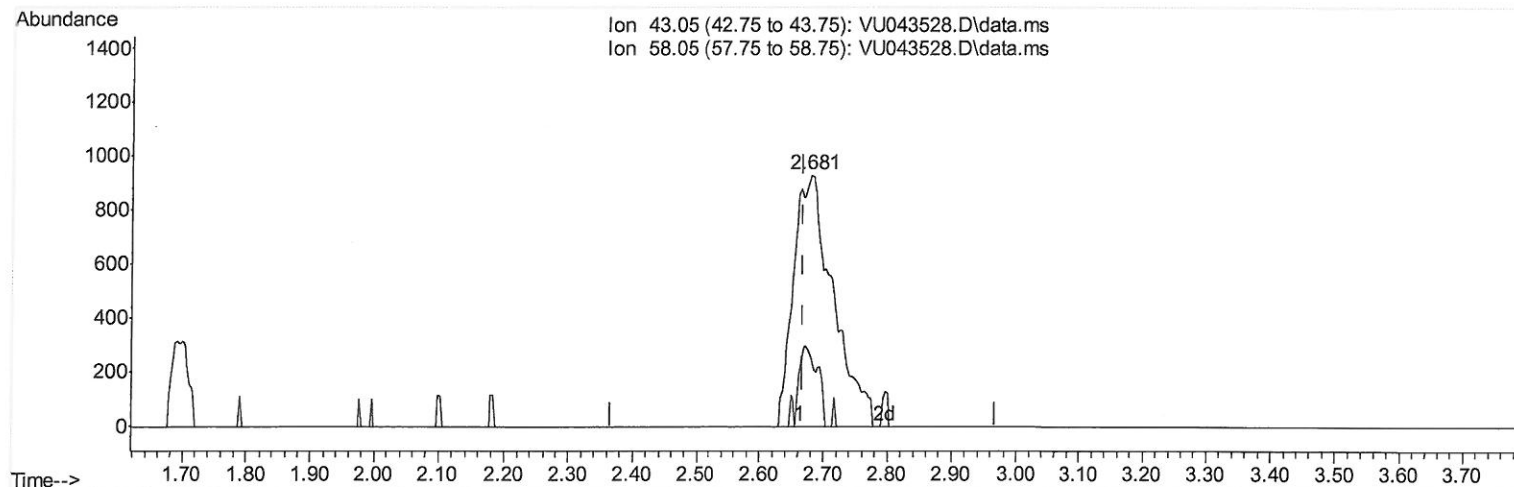

TIC: VU043528.D\data.ms

(13) Acetone (T)

2.681min (+ 0.013) 2.98 ug/L m

response 3962

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.40	11.48
0.00	0.00	0.00
0.00	0.00	0.00

MD
5/13/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
 Data File : VU043528.D
 Acq On : 04 May 2021 18:34
 Operator : SY/MD
 Sample : M2195-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB3J6

Manual Integrations
 APPROVED

MMDadoda
 5/6/2021 11:32:54 AM

Quant Time: May 05 08:13:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 05 08:11:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	79946	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.426	117	82051	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.822	152	36295	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	29046	4.52	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.40%	
7) Chloroethane-d5	1.916	69	23289	4.95	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.00%	
11) 1,1-Dichloroethene-d2	2.568	65	14570	4.62	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	92.40%	
20) 2-Butanone-d5	4.655	46	128317	64.29	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	128.58%	
24) Chloroform-d	5.073	84	61460	5.00	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.00%	
26) 1,2-Dichloroethane-d4	5.713	65	40694	5.49	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.80%	
32) Benzene-d6	5.735	84	110884	5.00	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.00%	
36) 1,2-Dichloropropane-d6	6.700	67	39512	5.07	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.40%	
41) Toluene-d8	7.906	98	90259	4.43	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.60%	
43) trans-1,3-Dichloroprop...	8.185	79	15109	4.81	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.20%	
46) 2-Hexanone-d5	8.645	63	78169	59.36	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	118.72%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	33818	5.42	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	108.40%	
66) 1,2-Dichlorobenzene-d4	12.201	152	34958	5.40	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.00%	
Target Compounds						
13) Acetone	2.681	43	3962m	2.98	ug/L	Qvalue
42) Toluene	7.980	91	2009	0.09	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed