

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
 Data File : VU043508.D
 Acq On : 04 May 2021 10:01
 Operator : SY/MD
 Sample : VU0504WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK145

Quant Time: May 05 04:51:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 05 04:50:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	88233	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	87910	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	39881	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	34545	4.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.40%
7) Chloroethane-d5	1.916	69	25865	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.572	65	16809	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.60%
20) 2-Butanone-d5	4.652	46	109700	49.80	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.60%
24) Chloroform-d	5.073	84	64679	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
26) 1,2-Dichloroethane-d4	5.713	65	41735	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.00%
32) Benzene-d6	5.739	84	123591	5.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.00%
36) 1,2-Dichloropropane-d6	6.700	67	44230	5.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.00%
41) Toluene-d8	7.906	98	105389	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
43) trans-1,3-Dichloroprop...	8.189	79	16151	4.80	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.00%
46) 2-Hexanone-d5	8.645	63	73222	51.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.78%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	34172	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.20%
66) 1,2-Dichlorobenzene-d4	12.201	152	38923	5.47	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.40%
Target Compounds						Qvalue
16) Methylene chloride	3.054	84	1907	0.24	ug/L	87
25) Chloroform	5.102	83	2589	0.20	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043508.D
Acq On : 04 May 2021 10:01
Operator : SY/MD
Sample : VU0504WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK145

Quant Time: May 05 04:51:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 05 04:50:58 2021
Response via : Initial Calibration




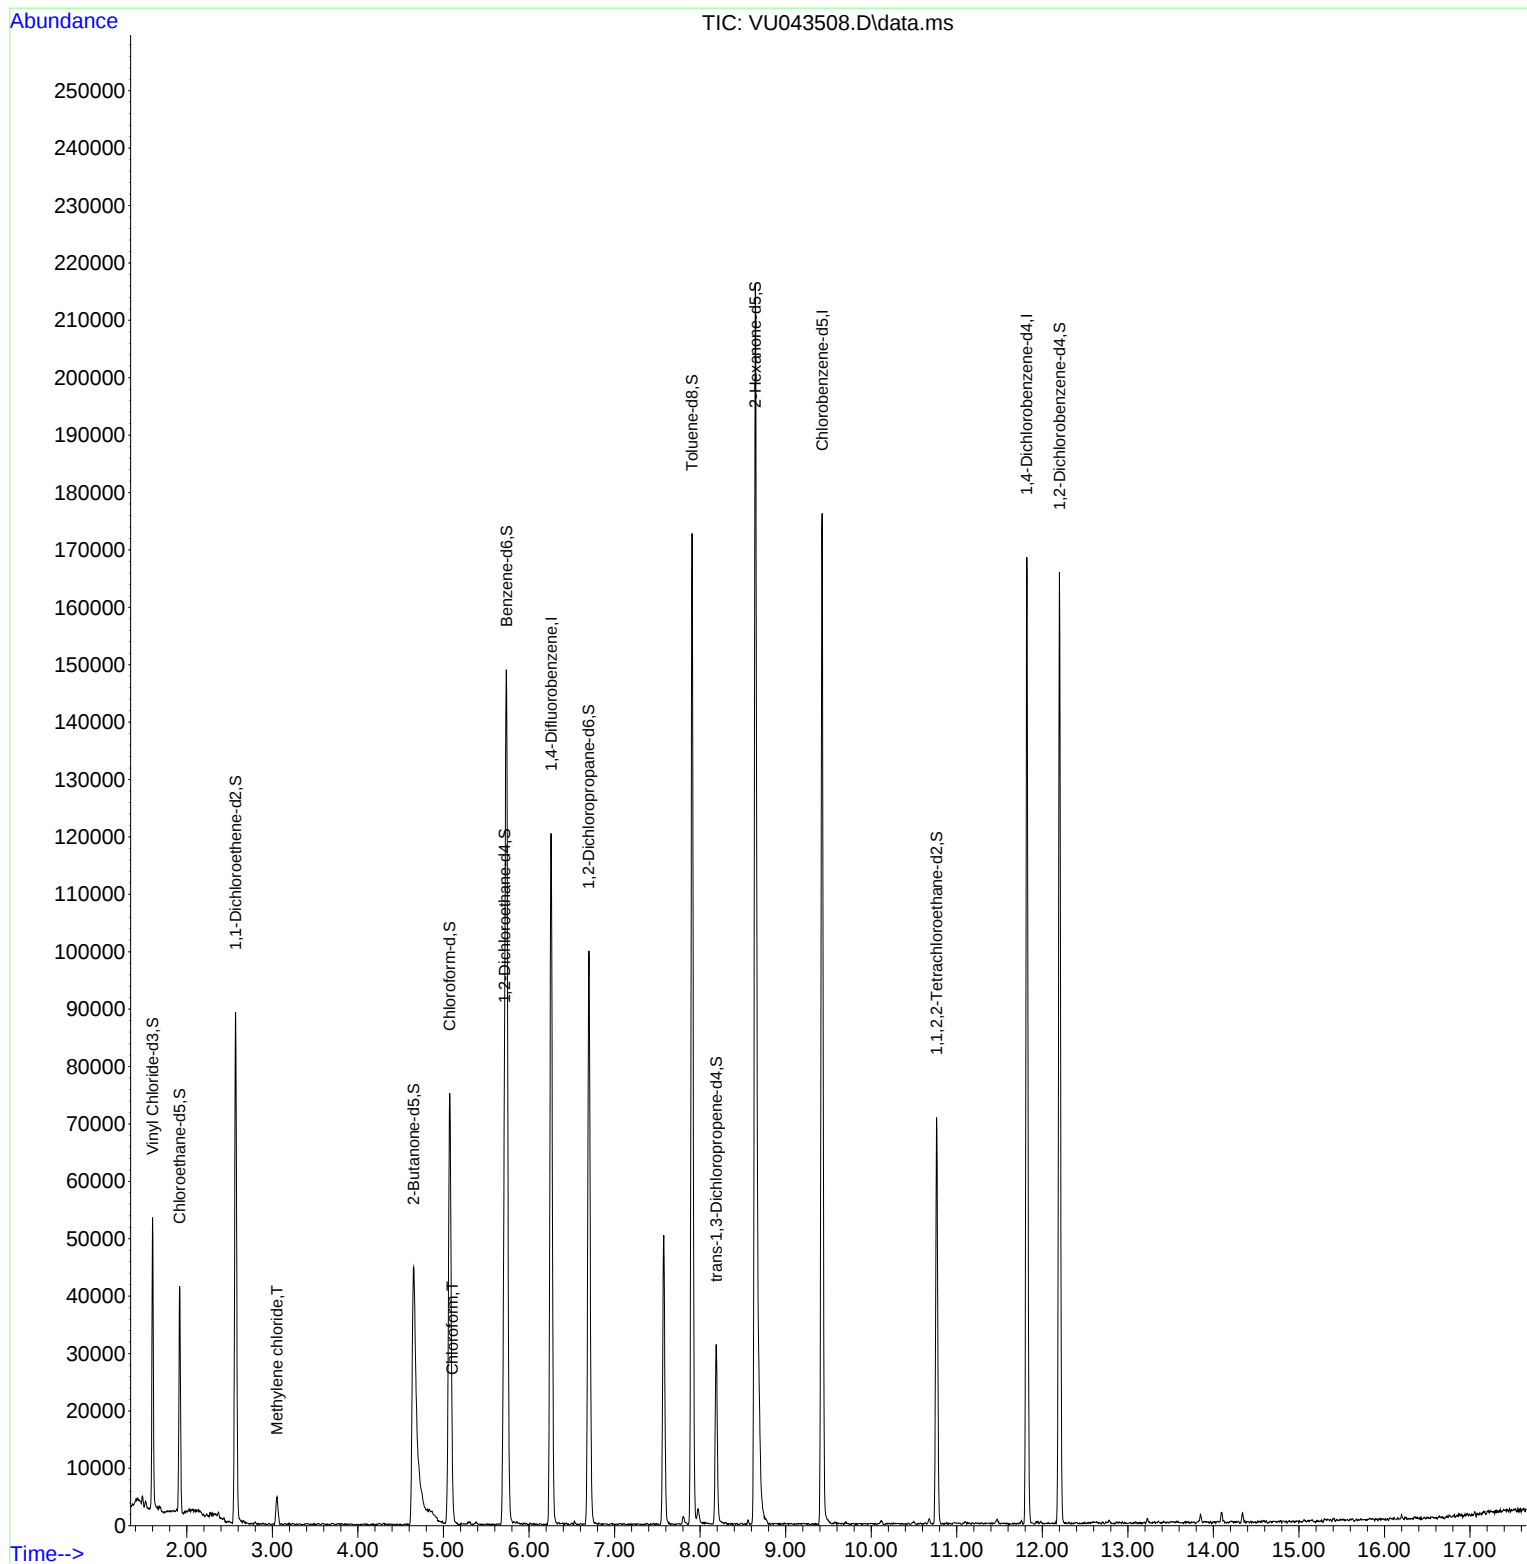


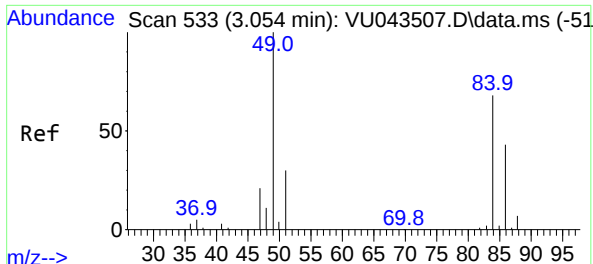

#16
Methylene chloride
Concen: 0.24 ug/L
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU043508.D
Acq: 04 May 2021 10:01

Instrument :
MSVOA_U
ClientSampleId :
VBLK145

Tgt Ion: 84 Resp: 1907
Ion Ratio Lower Upper
84 100
86 62.9 45.6 84.6
49 175.8 107.0 198.8

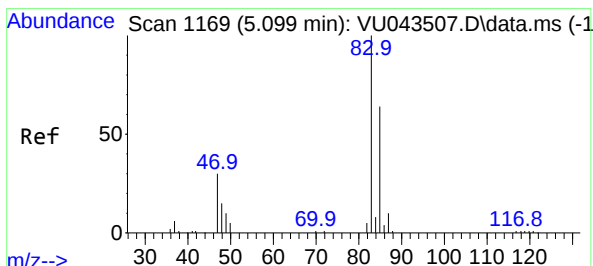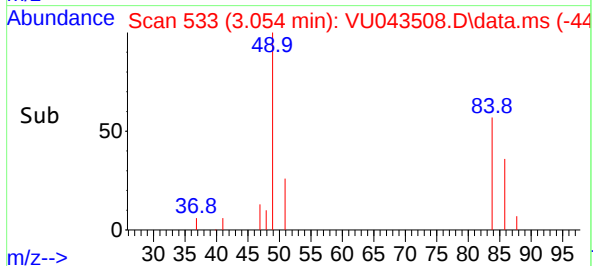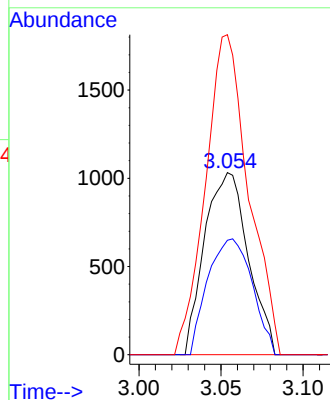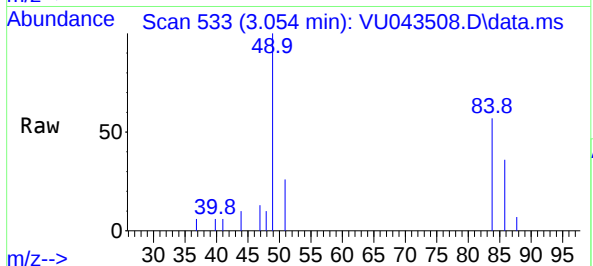

#25
Chloroform
Concen: 0.20 ug/L
RT: 5.102 min Scan# 1170
Delta R.T. 0.003 min
Lab File: VU043508.D
Acq: 04 May 2021 10:01

Tgt Ion: 83 Resp: 2589
Ion Ratio Lower Upper
83 100
85 60.0 45.1 83.9

