

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
 Data File : VU043534.D
 Acq On : 04 May 2021 21:00
 Operator : SY/MD
 Sample : M2195-08DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB3H6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	93	rBV	42732	48871	9.98%	1.417%
2	1.916	171	179	189	rVB	33979	43648	8.91%	1.265%
3	2.568	371	382	397	rBV	76120	122853	25.09%	3.561%
4	3.054	520	533	548	rVB3	9678	18348	3.75%	0.532%
5	3.192	563	576	590	rBV2	6481	13813	2.82%	0.400%
6	4.658	1015	1032	1076	rBV2	60387	233921	47.78%	6.781%
7	5.073	1141	1161	1181	rBV	69462	154380	31.53%	4.475%
8	5.735	1347	1367	1392	rVB2	133883	351587	71.81%	10.192%
9	6.256	1516	1529	1546	rBV	112663	211819	43.26%	6.140%
10	6.700	1651	1667	1688	rBV	90113	175892	35.92%	5.099%
11	7.575	1927	1939	1957	rBV2	43878	76410	15.61%	2.215%
12	7.906	2024	2042	2057	rBV	144112	248555	50.76%	7.205%
13	8.189	2117	2130	2150	rBV	28111	47862	9.78%	1.387%
14	8.562	2233	2246	2259	rBV	206670	352010	71.89%	10.204%
15	8.645	2259	2272	2306	rVV	254458	489620	100.00%	14.194%
16	8.925	2350	2359	2376	rVB4	5240	9494	1.94%	0.275%
17	9.423	2502	2514	2535	rBV	168404	277105	56.60%	8.033%
18	10.764	2919	2931	2946	rBV	70993	112580	22.99%	3.264%
19	11.819	3246	3259	3277	rBV	149802	233851	47.76%	6.779%
20	12.201	3363	3378	3396	rBV	142362	226982	46.36%	6.580%




Sum of corrected areas: 3449601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043534.D
Acq On : 04 May 2021 21:00
Operator : SY/MD
Sample : M2195-08DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3H6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

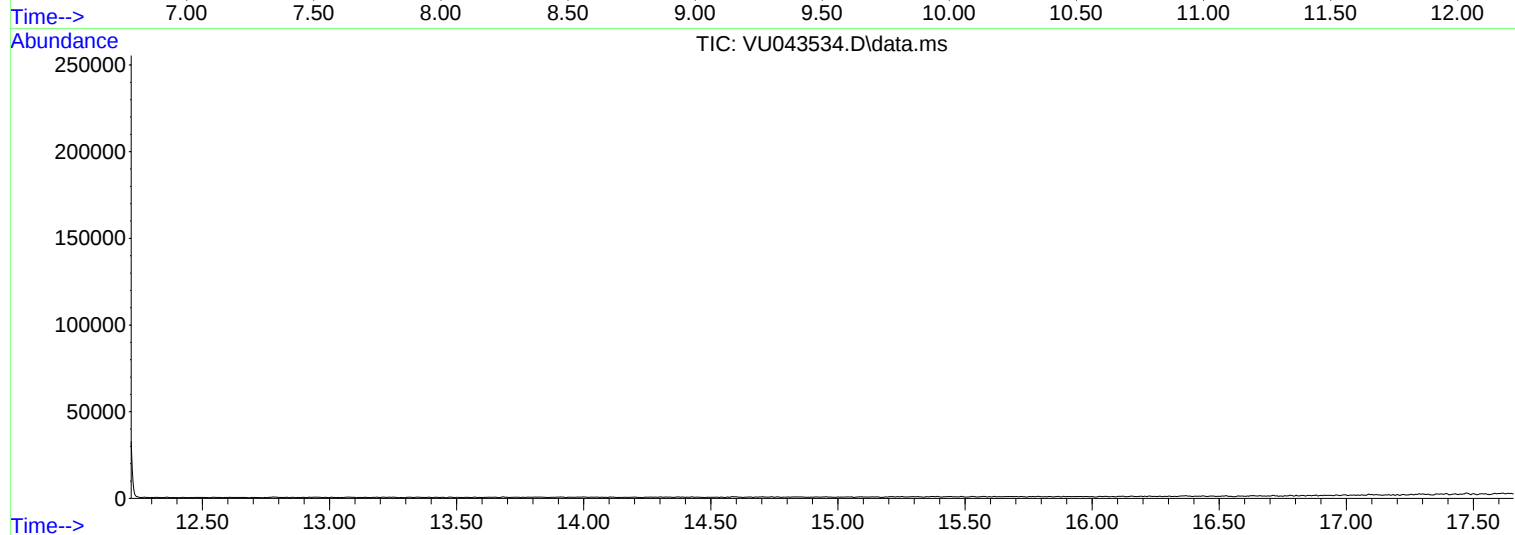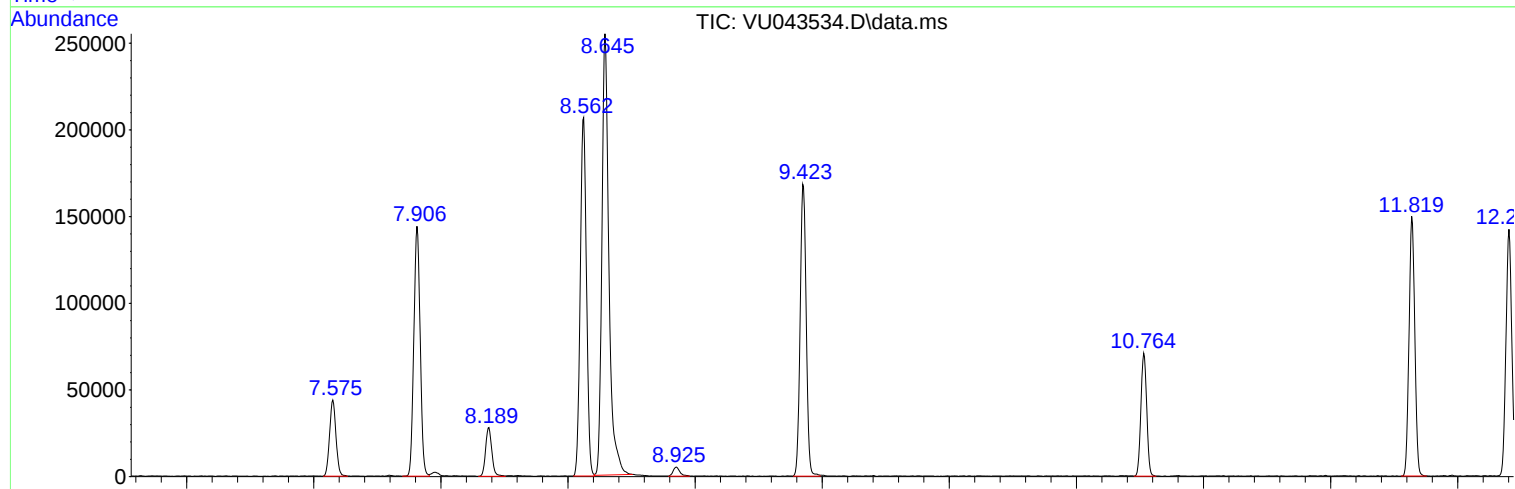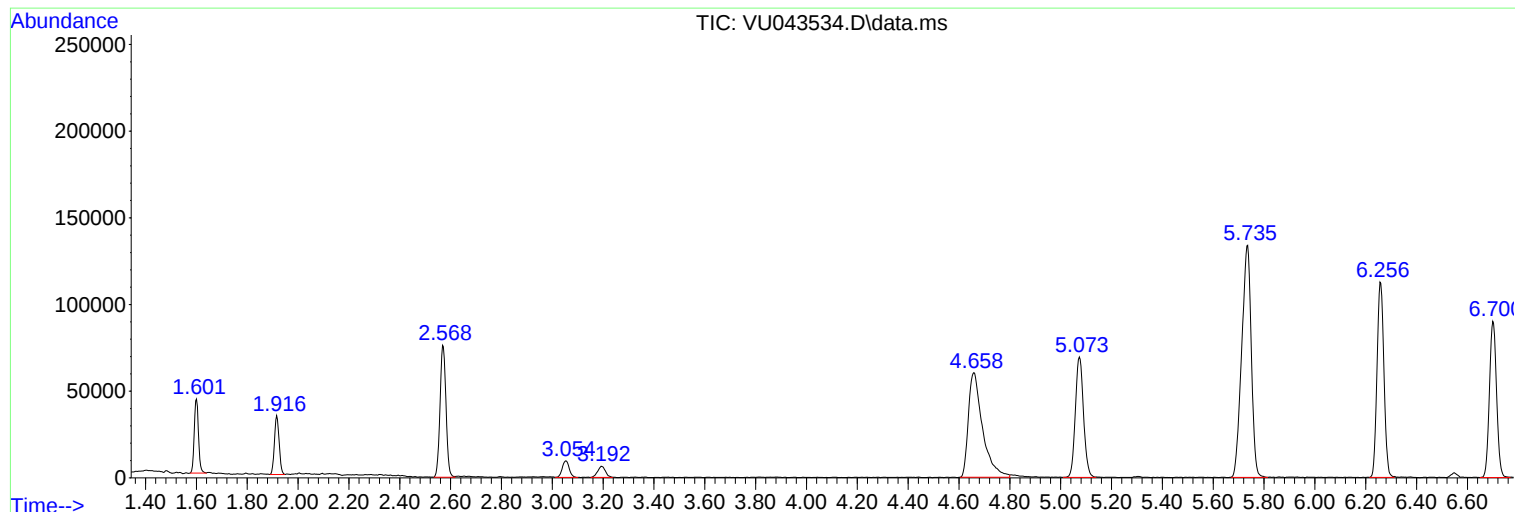

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043534.D
Acq On : 04 May 2021 21:00
Operator : SY/MD
Sample : M2195-08DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3H6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043534.D
Acq On : 04 May 2021 21:00
Operator : SY/MD
Sample : M2195-08DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3H6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
