

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
 Data File : VU043535.D
 Acq On : 04 May 2021 21:24
 Operator : SY/MD
 Sample : M2195-13DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB3J1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rBV	43085	49212	10.29%	1.560%
2	1.919	170	180	192	rVB	34748	44025	9.20%	1.395%
3	2.571	372	383	397	rBV	74490	119100	24.90%	3.775%
4	3.054	522	533	547	rBV2	8849	16455	3.44%	0.521%
5	3.195	565	577	596	rVB2	6020	13844	2.89%	0.439%
6	4.658	1015	1032	1083	rBV3	59897	248252	51.90%	7.868%
7	5.073	1147	1161	1182	rBV	68288	153339	32.06%	4.860%
8	5.735	1343	1367	1388	rBV2	131394	343164	71.75%	10.876%
9	6.259	1515	1530	1547	rBV	114807	214763	44.90%	6.806%
10	6.700	1654	1667	1686	rBV	88443	170516	35.65%	5.404%
11	7.574	1925	1939	1955	rBV3	42557	74548	15.59%	2.363%
12	7.906	2025	2042	2057	rBV	142530	242856	50.78%	7.697%
13	8.189	2120	2130	2150	rBV2	27528	46165	9.65%	1.463%
14	8.562	2235	2246	2259	rBV2	42167	70062	14.65%	2.220%
15	8.645	2259	2272	2303	rBV	242682	478292	100.00%	15.158%
16	8.925	2350	2359	2377	rVB3	7103	12317	2.58%	0.390%
17	9.426	2499	2515	2535	rBV	172364	285155	59.62%	9.037%
18	10.764	2919	2931	2944	rVB2	69390	109750	22.95%	3.478%
19	11.819	3248	3259	3275	rBV	154268	240605	50.31%	7.625%
20	12.201	3366	3378	3390	rBV	142165	222951	46.61%	7.066%




Sum of corrected areas: 3155371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043535.D
Acq On : 04 May 2021 21:24
Operator : SY/MD
Sample : M2195-13DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3J1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

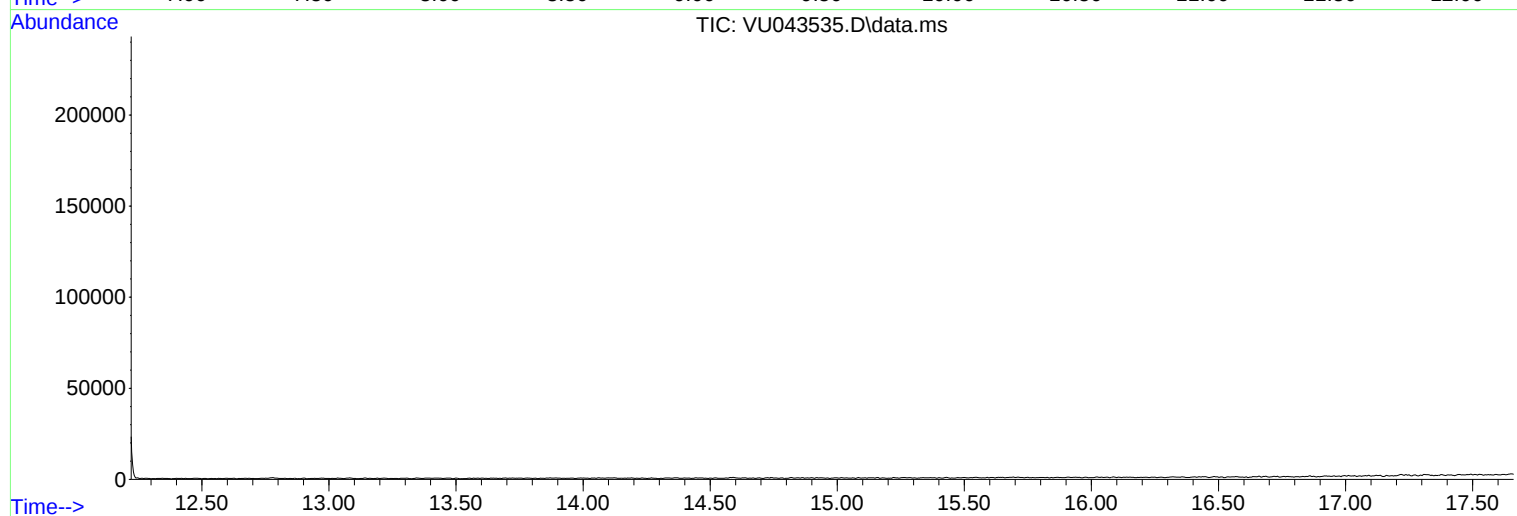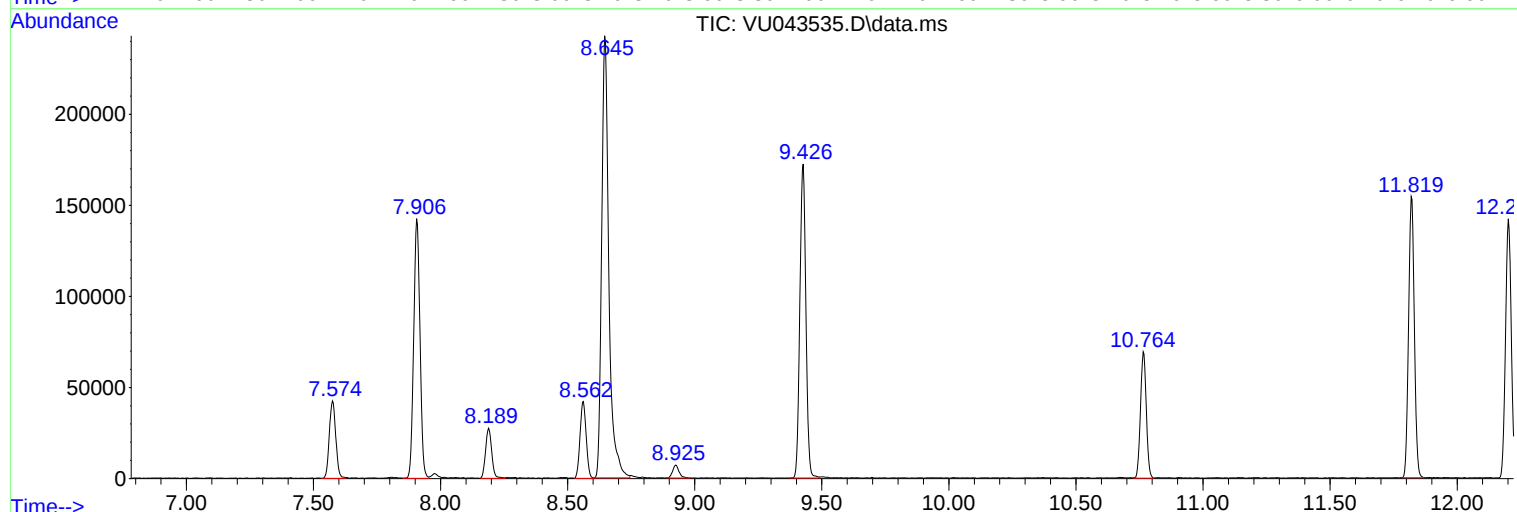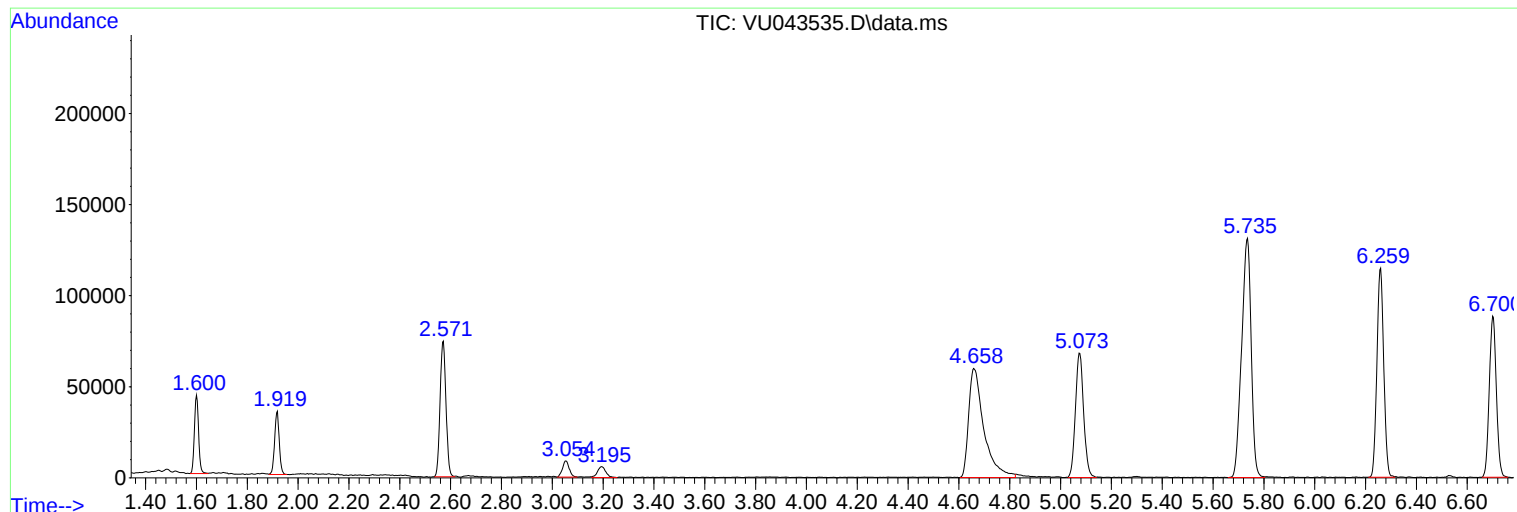

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043535.D
Acq On : 04 May 2021 21:24
Operator : SY/MD
Sample : M2195-13DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3J1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
Data File : VU043535.D
Acq On : 04 May 2021 21:24
Operator : SY/MD
Sample : M2195-13DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3J1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
