
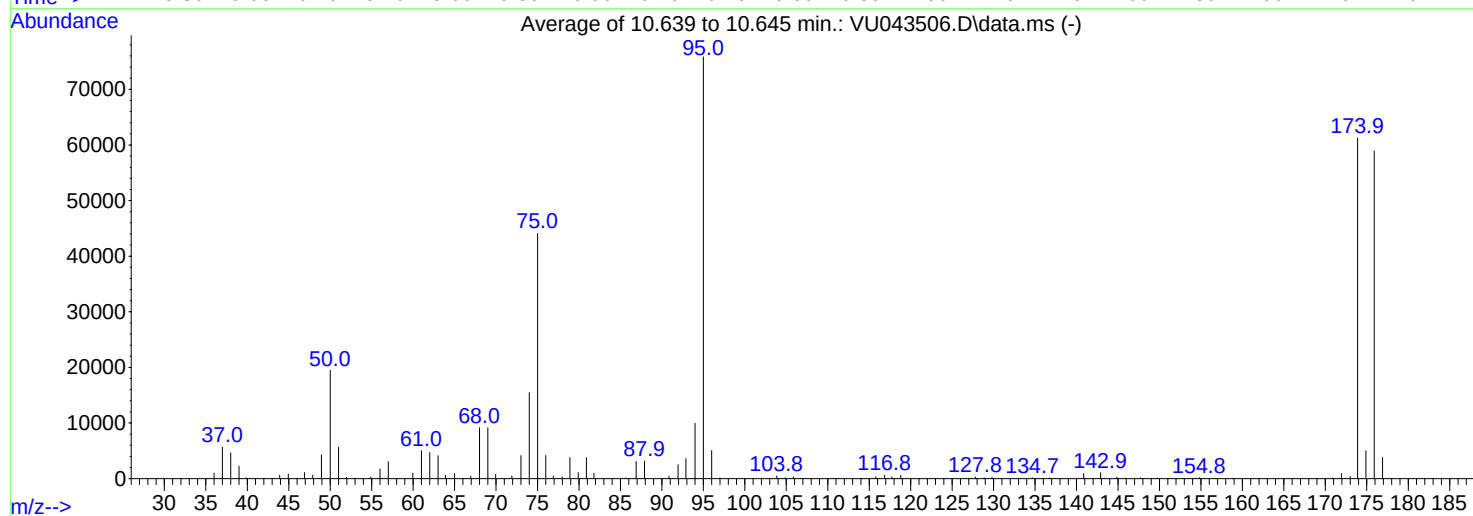


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050421\
 Data File : VU043506.D
 Acq On : 04 May 2021 08:59
 Operator : SY/MD
 Sample : BFB40
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB140

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 05 08:11:40 2021

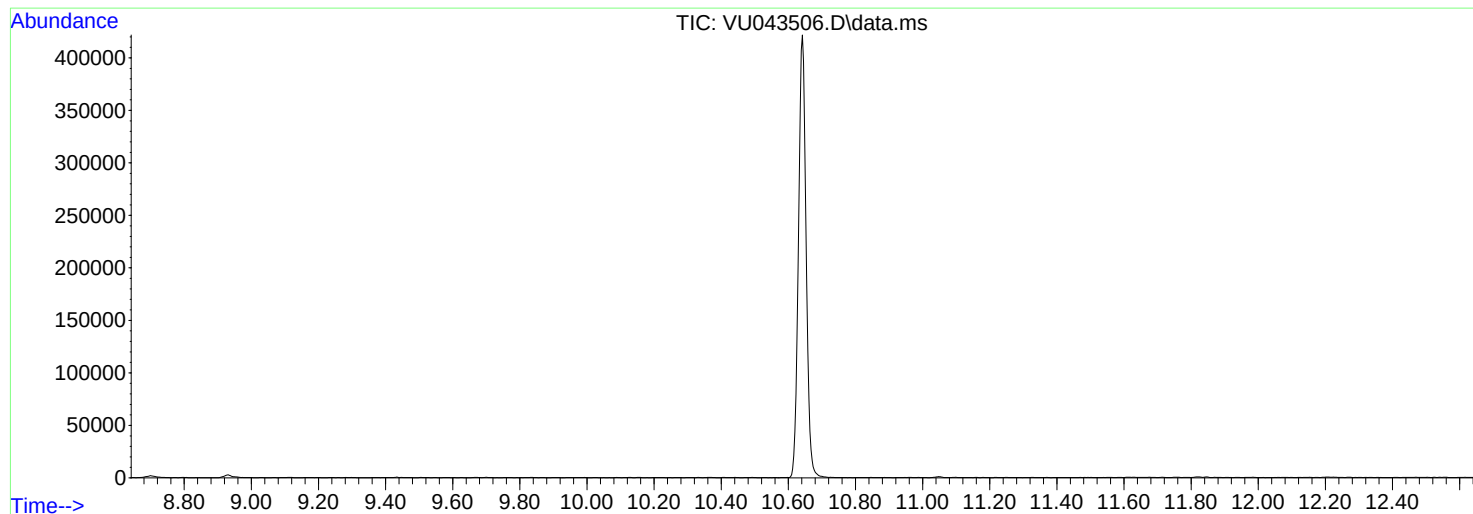

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.7	19469	PASS
75	95	30	80	58.2	44115	PASS
95	95	100	100	100.0	75845	PASS
96	95	5	9	6.6	5034	PASS
173	174	0.00	2	0.6	370	PASS
174	95	50	120	80.8	61261	PASS
175	174	5	9	8.2	4996	PASS
176	174	95	101	96.2	58931	PASS
177	176	5	9	6.5	3809	PASS

m/z	Abundance
36.00	1010.0
37.00	5227.0
38.00	4398.0
39.00	2131.0
40.00	244.0
43.90	926.0
44.90	780.0
46.90	1095.0
47.90	606.0
48.90	4132.0
50.00	18440.0
51.00	5339.0
51.90	216.0
52.90	125.0
54.90	315.0
56.00	1666.0
57.00	2717.0
57.90	113.0
59.90	1004.0
61.00	4781.0
62.00	4528.0
63.00	3821.0
63.90	526.0
65.00	836.0
67.00	419.0
68.00	8788.0
69.00	8846.0
69.90	772.0
71.90	498.0
73.00	4050.0
74.00	14712.0
75.00	42632.0
76.00	3987.0
76.90	493.0
78.00	315.0
78.90	3525.0
79.90	1030.0
80.90	3471.0
81.80	997.0
85.70	126.0
86.90	3030.0
87.90	3008.0
90.80	450.0
91.90	2347.0
92.90	3486.0
94.00	9765.0
95.00	73576.0
96.00	4702.0
97.00	147.0
103.90	463.0
104.90	150.0
105.90	306.0
115.80	342.0
116.80	539.0
117.70	297.0
118.80	523.0
127.90	323.0
128.90	139.0
129.80	269.0
130.90	113.0
134.70	168.0
136.70	177.0
140.80	888.0
142.90	1134.0
144.80	233.0
147.70	151.0
149.70	130.0
154.80	190.0
156.80	105.0
158.80	142.0
170.90	148.0
172.00	993.0
173.90	60840.0
174.90	4898.0
175.90	58824.0
176.90	3640.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

Scan 2879 (10.597 min): VU043506.D\data.ms
BFB40

m/z	Abundance
39.80	111.0
43.90	290.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

m/z	Abundance
36.00	997.0
37.00	5843.0
38.00	4748.0
39.00	2298.0
40.00	243.0
43.90	885.0
45.00	893.0
46.00	176.0
46.90	1046.0
47.90	706.0
49.00	4333.0
50.00	19840.0
51.00	5727.0
52.00	242.0
54.90	323.0
56.00	1722.0
57.00	3190.0
59.90	873.0
61.00	5090.0
62.00	4750.0
63.00	4290.0
63.90	635.0
65.00	866.0
66.90	392.0
68.00	9149.0
69.00	9212.0
70.00	761.0
71.90	515.0
73.00	4154.0
74.00	15794.0
75.00	44016.0
76.00	4178.0
76.90	520.0
77.90	333.0
78.90	3850.0
79.90	1105.0
80.90	3987.0
81.80	927.0
85.70	104.0
86.90	3128.0
87.90	3251.0
90.90	423.0
92.00	2599.0
92.90	3621.0
94.00	9825.0
95.00	75864.0
96.00	5132.0
97.00	140.0
103.80	465.0
104.80	156.0
105.80	353.0
115.80	336.0
116.90	672.0
117.80	322.0
118.80	580.0
127.70	233.0
128.80	128.0
129.80	256.0
134.70	108.0
136.80	169.0
140.90	938.0
142.90	1064.0
144.90	273.0
145.90	147.0
147.70	147.0
149.80	114.0
154.80	181.0
170.90	162.0
171.90	843.0
173.00	1110.0
173.90	59712.0
174.90	4902.0
175.90	57008.0
176.90	3839.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

m/z	Abundance
36.00	1039.0
37.00	5827.0
38.00	4726.0
39.00	2342.0
40.00	261.0
43.90	912.0
45.00	863.0
46.00	123.0
46.90	1117.0
47.90	659.0
49.00	4444.0
50.00	20128.0
51.00	5897.0
52.00	228.0
53.00	107.0
54.90	337.0
56.00	1785.0
57.00	3224.0
57.90	112.0
60.00	1028.0
61.00	5213.0
62.00	4838.0
63.00	4298.0
63.90	625.0
65.00	958.0
66.90	470.0
68.00	9481.0
69.00	9415.0
70.00	808.0
71.90	503.0
73.00	4265.0
74.00	15953.0
75.00	45696.0
76.00	4330.0
76.90	507.0
77.90	314.0
78.90	3905.0
79.90	1114.0
80.90	3893.0
81.80	1045.0
85.70	138.0
86.90	3181.0
87.90	3290.0
90.90	467.0
92.00	2577.0
92.90	3713.0
94.00	10241.0
95.00	78096.0
96.00	5268.0
97.00	169.0
103.90	509.0
104.80	156.0
105.80	337.0
106.70	106.0
110.70	101.0
115.80	386.0
116.90	640.0
117.70	331.0
118.80	612.0
127.80	275.0
128.80	136.0
129.80	278.0
134.70	148.0
136.80	189.0
140.80	940.0
142.90	1092.0
144.90	270.0
145.90	136.0
147.70	158.0
149.80	130.0
154.80	193.0
158.80	129.0
170.90	159.0
172.00	949.0
173.90	63232.0
174.90	5189.0
175.90	60960.0
176.90	3948.0
177.90	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140