

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048407.D
 Acq On : 04 May 2022 10:46
 Operator : SY/MD
 Sample : VU0504WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	52	rBV2	5584	7355	0.40%	0.053%
2	1.600	73	81	103	rBV	236725	309558	16.65%	2.231%
3	1.890	163	171	187	rVB	155530	231063	12.43%	1.665%
4	2.504	358	362	364	rBV2	292	202	0.01%	0.001%
5	2.562	367	380	399	rBV	400357	653707	35.17%	4.711%
6	2.732	427	433	435	rBV4	390	360	0.02%	0.003%
7	2.787	444	450	451	rBV2	858	774	0.04%	0.006%
8	2.825	458	462	465	rBV2	188	162	0.01%	0.001%
9	2.887	478	481	485	rVB3	282	213	0.01%	0.002%
10	2.941	489	498	499	rBV3	406	409	0.02%	0.003%
11	3.047	521	531	543	rVB4	1671	2925	0.16%	0.021%
12	3.099	543	547	550	rBV3	258	219	0.01%	0.002%
13	3.186	559	574	595	rVB	5803	14614	0.79%	0.105%
14	3.362	622	629	643	rVB5	829	1508	0.08%	0.011%
15	3.475	660	664	666	rVB	250	163	0.01%	0.001%
16	3.510	670	675	680	rBV2	151	175	0.01%	0.001%
17	3.870	783	787	790	rVB2	217	209	0.01%	0.002%
18	4.115	860	863	869	rBV2	189	217	0.01%	0.002%
19	4.182	875	884	887	rBV	333	380	0.02%	0.003%
20	4.620	1006	1020	1045	rBV	211079	510936	27.49%	3.682%
21	4.864	1091	1096	1100	rBV3	415	266	0.01%	0.002%
22	5.063	1141	1158	1184	rVV	329765	715072	38.47%	5.153%
23	5.247	1212	1215	1219	rVB3	326	261	0.01%	0.002%
24	5.279	1221	1225	1227	rBV3	532	414	0.02%	0.003%
25	5.308	1231	1234	1236	rBV3	366	205	0.01%	0.001%
26	5.324	1237	1239	1240	rBV2	453	200	0.01%	0.001%
27	5.382	1254	1257	1260	rBV3	337	261	0.01%	0.002%
28	5.523	1297	1301	1303	rBV2	315	266	0.01%	0.002%
29	5.591	1318	1322	1327	rBV2	220	202	0.01%	0.001%
30	5.722	1341	1363	1393	rBV2	683500	1858899	100.00%	13.395%
31	5.970	1432	1440	1441	rBV4	1091	1072	0.06%	0.008%
32	6.041	1459	1462	1465	rBV2	374	265	0.01%	0.002%
33	6.073	1470	1472	1475	rVB	371	191	0.01%	0.001%
34	6.160	1493	1499	1501	rBV2	276	283	0.02%	0.002%
35	6.250	1509	1527	1559	rBV	429854	818198	44.02%	5.896%
36	6.536	1605	1616	1629	rVV9	2677	5430	0.29%	0.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048407.D
 Acq On : 04 May 2022 10:46
 Operator : SY/MD
 Sample : VU0504WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.607	1636	1638	1640	rVB2	352	186	0.01%	0.001%
38	6.620	1640	1642	1645	rVB	392	171	0.01%	0.001%
39	6.690	1649	1664	1683	rBV	434887	836823	45.02%	6.030%
40	6.845	1710	1712	1717	rVB3	279	164	0.01%	0.001%
41	6.893	1724	1727	1733	rBV2	182	235	0.01%	0.002%
42	7.047	1770	1775	1780	rBV3	484	556	0.03%	0.004%
43	7.105	1789	1793	1797	rBV	517	335	0.02%	0.002%
44	7.137	1799	1803	1805	rVV3	289	259	0.01%	0.002%
45	7.182	1805	1817	1833	rVB4	4809	10652	0.57%	0.077%
46	7.256	1833	1840	1843	rBV3	365	378	0.02%	0.003%
47	7.494	1910	1914	1917	rBV2	232	180	0.01%	0.001%
48	7.565	1922	1936	1957	rBV	223489	395176	21.26%	2.848%
49	7.690	1967	1975	1989	rVB5	2401	4380	0.24%	0.032%
50	7.796	1998	2008	2015	rBV6	1864	3105	0.17%	0.022%
51	7.899	2025	2040	2055	rBV	845145	1462518	78.68%	10.539%
52	8.179	2115	2127	2148	rBV	158144	268553	14.45%	1.935%
53	8.375	2184	2188	2190	rBV3	356	273	0.01%	0.002%
54	8.404	2194	2197	2200	rVV4	325	248	0.01%	0.002%
55	8.549	2238	2242	2247	rVB3	769	684	0.04%	0.005%
56	8.636	2254	2269	2320	rBV2	637346	1208222	65.00%	8.706%
57	9.041	2392	2395	2397	rBV3	345	237	0.01%	0.002%
58	9.054	2397	2399	2403	rVV3	344	284	0.02%	0.002%
59	9.089	2408	2410	2412	rBV	293	173	0.01%	0.001%
60	9.150	2426	2429	2430	rBV	521	229	0.01%	0.002%
61	9.417	2499	2512	2534	rBV	640838	1069386	57.53%	7.706%
62	9.568	2553	2559	2560	rBV3	1228	929	0.05%	0.007%
63	9.658	2584	2587	2590	rVV2	398	233	0.01%	0.002%
64	9.697	2594	2599	2612	rVB4	1573	2476	0.13%	0.018%
65	9.832	2635	2641	2643	rBV2	144	179	0.01%	0.001%
66	9.928	2668	2671	2680	rVB	360	457	0.02%	0.003%
67	9.970	2680	2684	2686	rBV2	255	191	0.01%	0.001%
68	10.095	2719	2723	2725	rBV3	914	778	0.04%	0.006%
69	10.153	2737	2741	2744	rVB	319	247	0.01%	0.002%
70	10.365	2804	2807	2812	rBV	210	198	0.01%	0.001%
71	10.391	2812	2815	2821	rVB	435	357	0.02%	0.003%
72	10.423	2821	2825	2829	rBV	280	267	0.01%	0.002%
73	10.484	2840	2844	2851	rVB3	1144	1135	0.06%	0.008%
74	10.581	2871	2874	2880	rBV2	198	178	0.01%	0.001%
75	10.616	2881	2885	2886	rBV	268	190	0.01%	0.001%
76	10.668	2896	2901	2909	rVB4	2396	3114	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048407.D
 Acq On : 04 May 2022 10:46
 Operator : SY/MD
 Sample : VU0504WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.758	2916	2929	2947	rBV	716748	1152702	62.01%	8.306%
78	11.089	3028	3032	3037	rVB5	654	572	0.03%	0.004%
79	11.121	3039	3042	3047	rBV3	537	512	0.03%	0.004%
80	11.275	3084	3090	3092	rBV2	371	365	0.02%	0.003%
81	11.417	3130	3134	3137	rVB2	498	346	0.02%	0.002%
82	11.468	3141	3150	3156	rVV5	2118	3269	0.18%	0.024%
83	11.610	3187	3194	3197	rVB3	282	325	0.02%	0.002%
84	11.626	3197	3199	3203	rVB	336	201	0.01%	0.001%
85	11.648	3203	3206	3209	rBV	307	199	0.01%	0.001%
86	11.697	3219	3221	3230	rVB4	890	715	0.04%	0.005%
87	11.748	3230	3237	3243	rBV3	1368	1993	0.11%	0.014%
88	11.812	3244	3257	3281	rBV	612690	981160	52.78%	7.070%
89	11.973	3303	3307	3315	rVB7	1520	1623	0.09%	0.012%
90	12.131	3354	3356	3360	rBV2	253	174	0.01%	0.001%
91	12.195	3360	3376	3394	rBV	797944	1300772	69.98%	9.373%
92	12.462	3456	3459	3462	rVB	338	191	0.01%	0.001%
93	12.481	3462	3465	3469	rBV	300	261	0.01%	0.002%
94	12.635	3510	3513	3516	rBV3	415	349	0.02%	0.003%
95	12.719	3535	3539	3541	rBV3	305	248	0.01%	0.002%
96	13.063	3643	3646	3648	rBV	316	202	0.01%	0.001%
97	13.227	3693	3697	3708	rVB3	1472	1717	0.09%	0.012%
98	13.851	3883	3891	3903	rVB5	3168	4698	0.25%	0.034%
99	14.095	3960	3967	3978	rVB	5410	8040	0.43%	0.058%
100	14.336	4033	4042	4051	rBV5	3661	5798	0.31%	0.042%




Sum of corrected areas: 13877402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048407.D
Acq On : 04 May 2022 10:46
Operator : SY/MD
Sample : VU0504WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

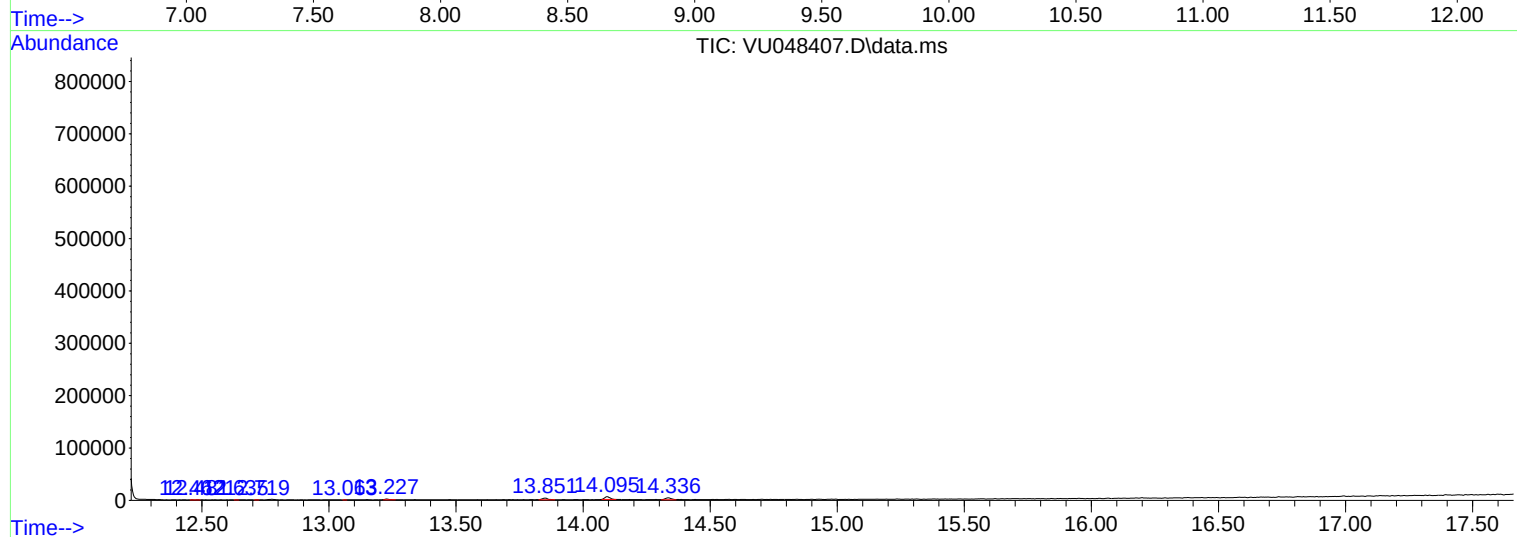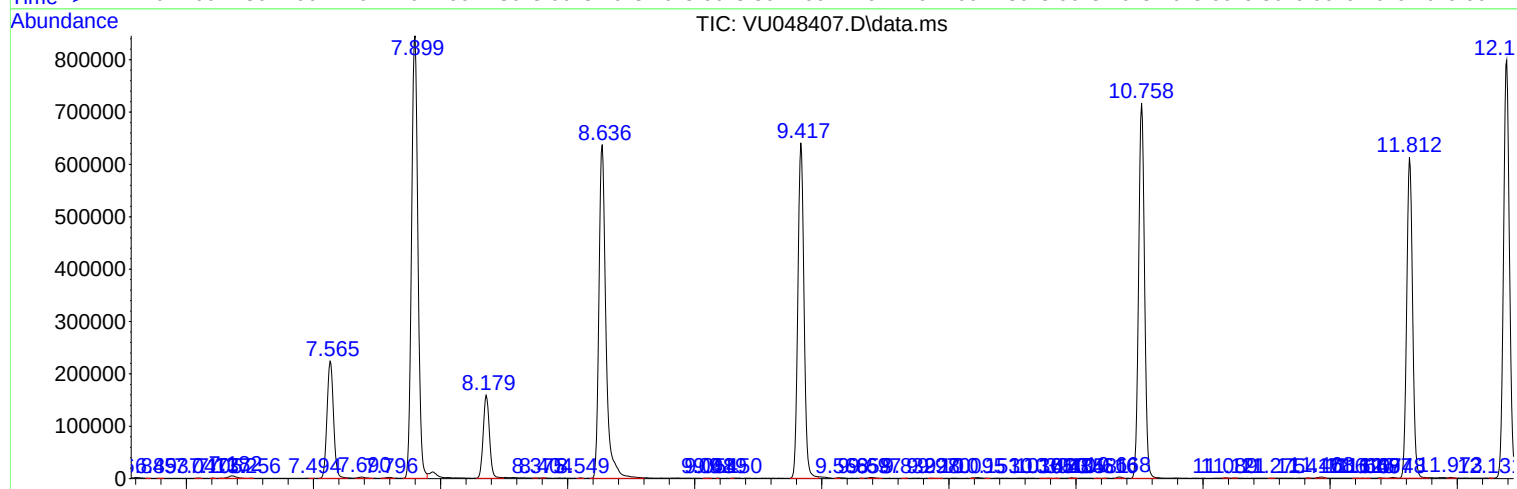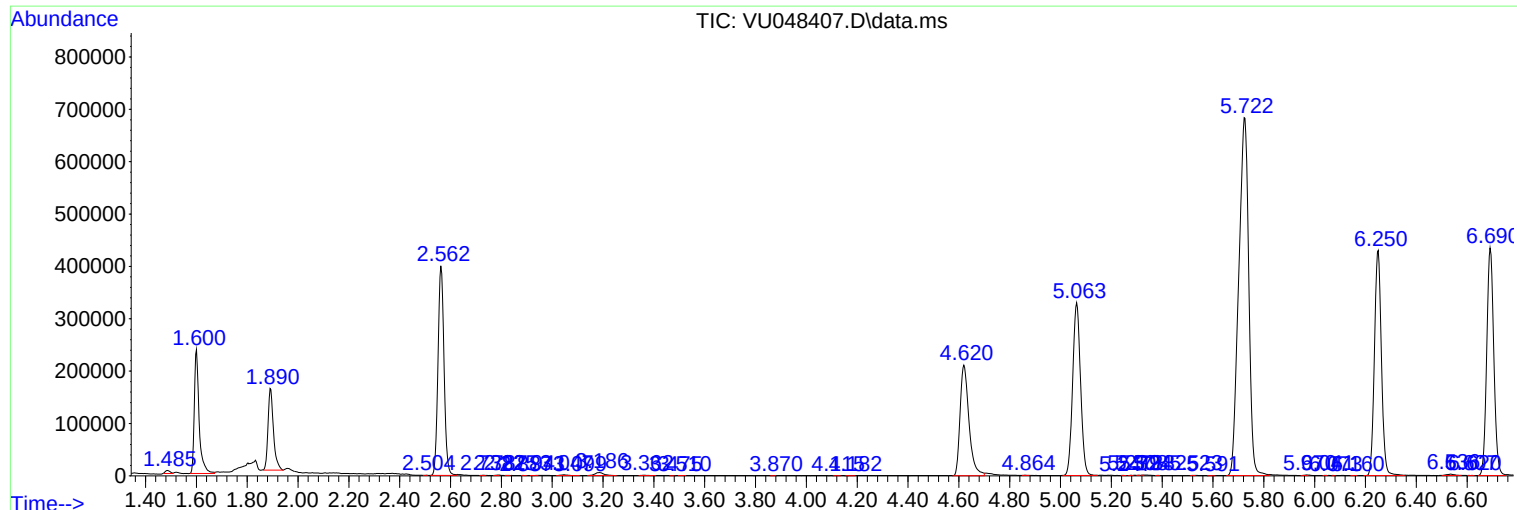

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048407.D
Acq On : 04 May 2022 10:46
Operator : SY/MD
Sample : VU0504WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048407.D
Acq On : 04 May 2022 10:46
Operator : SY/MD
Sample : VU0504WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc