

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048409.D
 Acq On : 04 May 2022 11:40
 Operator : SY/MD
 Sample : N2668-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	51	rBV2	3228	3214	0.16%	0.023%
2	1.601	73	81	105	rBV	244148	323957	16.45%	2.305%
3	1.903	167	175	204	rVB	181258	281375	14.29%	2.002%
4	2.495	358	359	364	rVB2	414	231	0.01%	0.002%
5	2.565	364	381	398	rBV	427001	699329	35.51%	4.976%
6	2.713	423	427	431	rBV3	380	289	0.01%	0.002%
7	2.765	437	443	446	rBV2	703	676	0.03%	0.005%
8	2.790	446	451	453	rBV3	792	897	0.05%	0.006%
9	2.900	480	485	486	rBV	290	214	0.01%	0.002%
10	2.980	507	510	512	rVB3	375	231	0.01%	0.002%
11	3.048	524	531	540	rVB4	814	1295	0.07%	0.009%
12	3.189	561	575	596	rBV2	5923	15726	0.80%	0.112%
13	3.305	608	611	613	rBV	329	240	0.01%	0.002%
14	3.459	654	659	664	rVB3	317	320	0.02%	0.002%
15	3.491	664	669	676	rBV3	361	418	0.02%	0.003%
16	3.523	676	679	681	rBV2	329	196	0.01%	0.001%
17	3.758	750	752	756	rVB2	349	204	0.01%	0.001%
18	3.784	756	760	765	rBV	251	198	0.01%	0.001%
19	3.813	765	769	773	rVB2	296	208	0.01%	0.001%
20	3.932	800	806	810	rBV2	144	208	0.01%	0.001%
21	4.077	847	851	855	rBV2	233	242	0.01%	0.002%
22	4.105	856	860	864	rVB2	273	229	0.01%	0.002%
23	4.125	864	866	872	rBV2	199	214	0.01%	0.002%
24	4.292	910	918	920	rBV2	226	273	0.01%	0.002%
25	4.575	1002	1006	1008	rBV2	314	218	0.01%	0.002%
26	4.626	1008	1022	1067	rBV	203106	525959	26.71%	3.742%
27	4.822	1077	1083	1095	rVB4	2410	4755	0.24%	0.034%
28	4.951	1121	1123	1130	rVB2	439	400	0.02%	0.003%
29	5.067	1142	1159	1186	rVV	344906	754359	38.31%	5.367%
30	5.279	1221	1225	1227	rBV2	514	352	0.02%	0.003%
31	5.292	1227	1229	1233	rVV3	309	236	0.01%	0.002%
32	5.504	1288	1295	1297	rBV2	227	216	0.01%	0.002%
33	5.726	1340	1364	1397	rBV2	736719	1969165	100.00%	14.010%
34	5.887	1412	1414	1417	rVB3	439	229	0.01%	0.002%
35	5.967	1436	1439	1441	rBV	475	303	0.02%	0.002%
36	6.118	1482	1486	1488	rBV2	530	366	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048409.D
 Acq On : 04 May 2022 11:40
 Operator : SY/MD
 Sample : N2668-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.173	1500	1503	1506	rBV2	314	249	0.01%	0.002%
38	6.250	1513	1527	1557	rBV	465212	887876	45.09%	6.317%
39	6.536	1602	1616	1619	rBV6	1981	3515	0.18%	0.025%
40	6.588	1630	1632	1636	rBV2	313	208	0.01%	0.001%
41	6.691	1650	1664	1685	rBV	447449	877472	44.56%	6.243%
42	6.809	1696	1701	1706	rBV3	841	844	0.04%	0.006%
43	6.861	1714	1717	1720	rVB3	434	260	0.01%	0.002%
44	6.890	1720	1726	1730	rBV	213	232	0.01%	0.002%
45	6.977	1747	1753	1756	rBV2	298	301	0.02%	0.002%
46	7.064	1778	1780	1785	rVB	313	220	0.01%	0.002%
47	7.186	1809	1818	1828	rBV5	4286	7824	0.40%	0.056%
48	7.295	1849	1852	1857	rVB3	319	284	0.01%	0.002%
49	7.337	1857	1865	1870	rVB3	311	386	0.02%	0.003%
50	7.498	1913	1915	1923	rVB2	261	334	0.02%	0.002%
51	7.565	1923	1936	1965	rBV	216217	385666	19.59%	2.744%
52	7.697	1969	1977	1986	rVB4	1978	3480	0.18%	0.025%
53	7.742	1989	1991	1995	rBV4	210	187	0.01%	0.001%
54	7.790	2003	2006	2009	rBV2	228	187	0.01%	0.001%
55	7.826	2013	2017	2021	rVB3	371	372	0.02%	0.003%
56	7.899	2021	2040	2056	rBV	874788	1518464	77.11%	10.804%
57	8.179	2116	2127	2142	rBV	148176	255346	12.97%	1.817%
58	8.321	2169	2171	2174	rBV3	367	193	0.01%	0.001%
59	8.462	2209	2215	2218	rBV3	761	806	0.04%	0.006%
60	8.555	2241	2244	2246	rVB2	498	209	0.01%	0.001%
61	8.636	2255	2269	2312	rBV2	625258	1152389	58.52%	8.199%
62	8.970	2369	2373	2374	rBV	448	255	0.01%	0.002%
63	9.118	2414	2419	2420	rBV2	449	299	0.02%	0.002%
64	9.150	2425	2429	2431	rBV3	349	295	0.01%	0.002%
65	9.166	2431	2434	2436	rVV	370	219	0.01%	0.002%
66	9.417	2499	2512	2550	rBV	650305	1094443	55.58%	7.787%
67	9.575	2555	2561	2569	rVB5	753	909	0.05%	0.006%
68	9.616	2569	2574	2577	rBV2	358	282	0.01%	0.002%
69	9.636	2577	2580	2583	rBV2	370	297	0.02%	0.002%
70	9.694	2592	2598	2609	rVB3	1040	1598	0.08%	0.011%
71	10.047	2702	2708	2713	rBV2	280	397	0.02%	0.003%
72	10.099	2719	2724	2729	rVB3	409	449	0.02%	0.003%
73	10.391	2811	2815	2820	rBV2	220	217	0.01%	0.002%
74	10.488	2841	2845	2847	rBV	234	194	0.01%	0.001%
75	10.539	2856	2861	2865	rBV2	203	214	0.01%	0.002%
76	10.671	2897	2902	2909	rVB3	1924	2314	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048409.D
 Acq On : 04 May 2022 11:40
 Operator : SY/MD
 Sample : N2668-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.758	2915	2929	2950	rBV	675555	1084075	55.05%	7.713%
78	10.896	2963	2972	2980	rVB4	2207	4053	0.21%	0.029%
79	10.960	2989	2992	2997	rVB2	295	220	0.01%	0.002%
80	11.050	3017	3020	3023	rBV2	266	190	0.01%	0.001%
81	11.096	3029	3034	3037	rBV3	353	367	0.02%	0.003%
82	11.115	3038	3040	3044	rBV3	407	297	0.02%	0.002%
83	11.234	3074	3077	3081	rVB	417	302	0.02%	0.002%
84	11.256	3081	3084	3087	rBV2	363	211	0.01%	0.002%
85	11.391	3122	3126	3128	rBV	240	186	0.01%	0.001%
86	11.417	3130	3134	3138	rVB2	660	542	0.03%	0.004%
87	11.459	3138	3147	3157	rBV7	1675	3166	0.16%	0.023%
88	11.700	3215	3222	3229	rVB3	950	1227	0.06%	0.009%
89	11.745	3231	3236	3244	rVB3	559	670	0.03%	0.005%
90	11.813	3244	3257	3277	rBV	586998	924688	46.96%	6.579%
91	12.192	3359	3375	3394	rBV	765415	1240997	63.02%	8.830%
92	12.407	3439	3442	3448	rVB3	349	331	0.02%	0.002%
93	12.719	3534	3539	3542	rBV3	514	499	0.03%	0.004%
94	12.761	3549	3552	3554	rBV2	703	497	0.03%	0.004%
95	12.851	3575	3580	3583	rBV2	355	383	0.02%	0.003%
96	13.050	3638	3642	3646	rBV2	288	372	0.02%	0.003%
97	13.851	3885	3891	3903	rVB5	1085	1805	0.09%	0.013%
98	14.099	3963	3968	3976	rVB2	1810	2119	0.11%	0.015%
99	14.337	4039	4042	4046	rVB2	939	653	0.03%	0.005%
100	15.221	4313	4317	4319	rBV3	791	622	0.03%	0.004%


Sum of corrected areas: 14055100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048409.D
Acq On : 04 May 2022 11:40
Operator : SY/MD
Sample : N2668-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

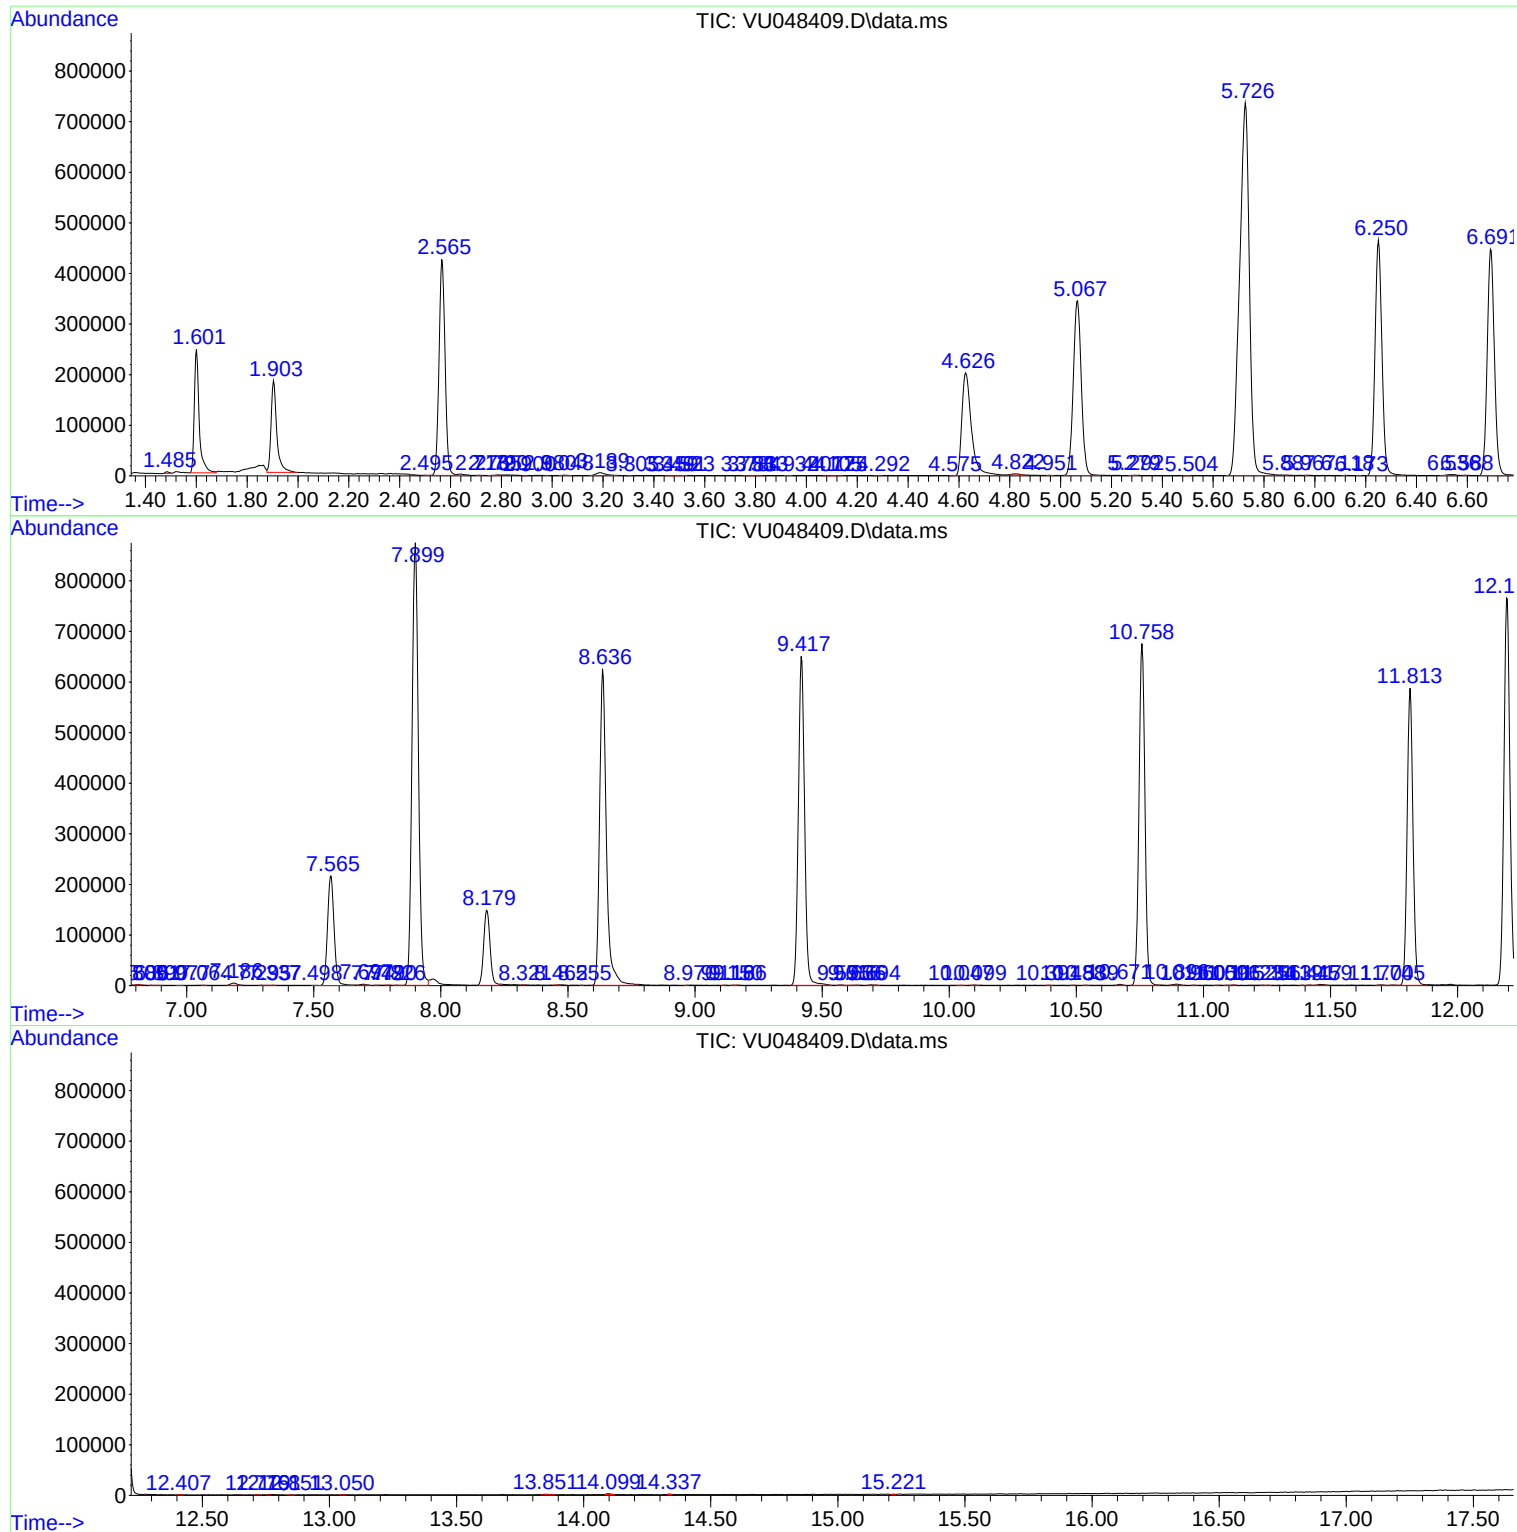

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048409.D
Acq On : 04 May 2022 11:40
Operator : SY/MD
Sample : N2668-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048409.D
Acq On : 04 May 2022 11:40
Operator : SY/MD
Sample : N2668-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------