

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048412.D
 Acq On : 04 May 2022 12:52
 Operator : SY/MD
 Sample : N2668-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	103	rBV	236360	314367	15.87%	1.970%
2	1.900	167	174	203	rVB	182574	279991	14.14%	1.755%
3	2.472	349	352	354	rBV2	521	304	0.02%	0.002%
4	2.565	368	381	398	rBV	421153	690602	34.86%	4.328%
5	2.739	429	435	438	rVB2	452	431	0.02%	0.003%
6	2.765	438	443	445	rBV2	524	516	0.03%	0.003%
7	2.793	449	452	458	rVB4	876	916	0.05%	0.006%
8	2.822	458	461	463	rBV2	436	344	0.02%	0.002%
9	2.855	468	471	476	rVV3	619	333	0.02%	0.002%
10	2.961	501	504	508	rVV2	294	216	0.01%	0.001%
11	3.051	524	532	541	rVB4	851	1432	0.07%	0.009%
12	3.102	541	548	553	rVB2	362	426	0.02%	0.003%
13	3.183	561	573	576	rBV4	1470	2298	0.12%	0.014%
14	3.260	589	597	604	rVB3	630	1036	0.05%	0.006%
15	3.295	604	608	610	rBV2	398	260	0.01%	0.002%
16	3.520	672	678	681	rBV2	284	300	0.02%	0.002%
17	3.633	709	713	716	rBV	306	192	0.01%	0.001%
18	3.935	802	807	811	rBV2	307	302	0.02%	0.002%
19	4.176	877	882	892	rBV2	212	338	0.02%	0.002%
20	4.224	893	897	902	rBV2	296	306	0.02%	0.002%
21	4.388	943	948	951	rBV2	247	222	0.01%	0.001%
22	4.629	1009	1023	1062	rBV	196392	523368	26.42%	3.280%
23	4.957	1120	1125	1131	rVB4	381	409	0.02%	0.003%
24	4.990	1133	1135	1141	rVB2	351	222	0.01%	0.001%
25	5.063	1141	1158	1179	rBV	346262	757074	38.22%	4.745%
26	5.298	1222	1231	1238	rVB4	700	1151	0.06%	0.007%
27	5.385	1256	1258	1265	rVB3	324	226	0.01%	0.001%
28	5.726	1340	1364	1405	rBV2	740565	1980824	100.00%	12.414%
29	5.964	1433	1438	1440	rBV3	886	722	0.04%	0.005%
30	6.034	1457	1460	1462	rBV2	344	252	0.01%	0.002%
31	6.067	1467	1470	1475	rVB2	391	306	0.02%	0.002%
32	6.115	1479	1485	1490	rVB2	471	602	0.03%	0.004%
33	6.153	1490	1497	1498	rBV2	277	221	0.01%	0.001%
34	6.250	1512	1527	1559	rBV	476433	912519	46.07%	5.719%
35	6.520	1606	1611	1612	rBV	1705	1067	0.05%	0.007%
36	6.620	1640	1642	1646	rVB2	506	269	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048412.D
 Acq On : 04 May 2022 12:52
 Operator : SY/MD
 Sample : N2668-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.690	1646	1664	1686	rBV	452575	882537	44.55%	5.531%
38	6.925	1732	1737	1741	rBV2	193	210	0.01%	0.001%
39	7.047	1770	1775	1780	rBV2	228	299	0.02%	0.002%
40	7.102	1787	1792	1796	rBV2	141	202	0.01%	0.001%
41	7.189	1808	1819	1830	rBV3	4777	9450	0.48%	0.059%
42	7.253	1836	1839	1842	rVB	322	204	0.01%	0.001%
43	7.475	1904	1908	1911	rBV	314	269	0.01%	0.002%
44	7.568	1920	1937	1960	rBV	214485	385734	19.47%	2.417%
45	7.690	1969	1975	1987	rVB7	1759	3332	0.17%	0.021%
46	7.764	1994	1998	2001	rVB3	336	274	0.01%	0.002%
47	7.793	2001	2007	2009	rBV4	272	281	0.01%	0.002%
48	7.809	2009	2012	2017	rVB3	473	384	0.02%	0.002%
49	7.899	2026	2040	2057	rBV	895726	1543653	77.93%	9.674%
50	8.179	2115	2127	2142	rBV	150769	256416	12.94%	1.607%
51	8.468	2209	2217	2230	rVB3	2944	5475	0.28%	0.034%
52	8.552	2230	2243	2258	rBV	985166	1684622	85.05%	10.558%
53	8.639	2259	2270	2315	rVB2	634827	1173781	59.26%	7.356%
54	8.841	2331	2333	2335	rBV	344	211	0.01%	0.001%
55	8.896	2345	2350	2356	rVB3	451	519	0.03%	0.003%
56	8.951	2361	2367	2372	rVB2	509	612	0.03%	0.004%
57	8.986	2376	2378	2382	rVB	366	213	0.01%	0.001%
58	9.166	2430	2434	2438	rBV3	382	359	0.02%	0.002%
59	9.208	2444	2447	2451	rVB2	312	266	0.01%	0.002%
60	9.231	2451	2454	2458	rBV2	340	237	0.01%	0.001%
61	9.301	2474	2476	2481	rVV2	238	229	0.01%	0.001%
62	9.417	2497	2512	2532	rBV	672821	1127888	56.94%	7.069%
63	9.568	2555	2559	2562	rBV3	422	300	0.02%	0.002%
64	9.636	2575	2580	2581	rBV2	536	369	0.02%	0.002%
65	9.674	2588	2592	2594	rBV2	269	210	0.01%	0.001%
66	9.700	2594	2600	2609	rVB3	948	1354	0.07%	0.008%
67	9.822	2633	2638	2640	rBV2	279	226	0.01%	0.001%
68	10.099	2717	2724	2728	rVB5	425	576	0.03%	0.004%
69	10.430	2822	2827	2831	rBV2	264	233	0.01%	0.001%
70	10.481	2839	2843	2849	rBV	310	331	0.02%	0.002%
71	10.533	2855	2859	2863	rBV	313	295	0.01%	0.002%
72	10.674	2896	2903	2910	rVB5	1552	2095	0.11%	0.013%
73	10.758	2916	2929	2950	rBV	687383	1104202	55.74%	6.920%
74	10.890	2959	2970	2986	rBV3	6510	11280	0.57%	0.071%
75	10.970	2992	2995	2998	rBV2	411	314	0.02%	0.002%
76	11.089	3029	3032	3035	rVB	280	196	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
 Data File : VU048412.D
 Acq On : 04 May 2022 12:52
 Operator : SY/MD
 Sample : N2668-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.115	3036	3040	3041	rBV	414	263	0.01%	0.002%
78	11.173	3055	3058	3062	rVV2	272	252	0.01%	0.002%
79	11.214	3069	3071	3077	rVB2	266	228	0.01%	0.001%
80	11.246	3078	3081	3085	rBV	354	200	0.01%	0.001%
81	11.330	3104	3107	3110	rVB	403	232	0.01%	0.001%
82	11.462	3142	3148	3159	rVB4	1232	2119	0.11%	0.013%
83	11.655	3204	3208	3214	rBV2	430	553	0.03%	0.003%
84	11.697	3215	3221	3225	rVB4	576	727	0.04%	0.005%
85	11.812	3244	3257	3279	rBV	622775	983151	49.63%	6.162%
86	11.938	3294	3296	3302	rVV2	714	568	0.03%	0.004%
87	11.973	3302	3307	3315	rVB7	1334	1737	0.09%	0.011%
88	12.066	3326	3336	3349	rBV3	3604	7392	0.37%	0.046%
89	12.195	3361	3376	3396	rBV	786576	1277159	64.48%	8.004%
90	12.365	3427	3429	3432	rVB2	561	302	0.02%	0.002%
91	12.385	3432	3435	3437	rBV2	302	194	0.01%	0.001%
92	12.443	3450	3453	3456	rBV2	311	291	0.01%	0.002%
93	12.478	3461	3464	3467	rVB2	467	238	0.01%	0.001%
94	12.510	3467	3474	3477	rBV3	371	472	0.02%	0.003%
95	12.771	3548	3555	3567	rVB2	2544	3939	0.20%	0.025%
96	12.867	3582	3585	3589	rBV2	378	301	0.02%	0.002%
97	12.941	3605	3608	3611	rBV3	387	372	0.02%	0.002%
98	14.098	3965	3968	3974	rBV3	896	725	0.04%	0.005%
99	14.796	4181	4185	4187	rBV2	466	364	0.02%	0.002%
100	15.082	4271	4274	4277	rBV3	570	514	0.03%	0.003%




Sum of corrected areas: 15956295

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048412.D
Acq On : 04 May 2022 12:52
Operator : SY/MD
Sample : N2668-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

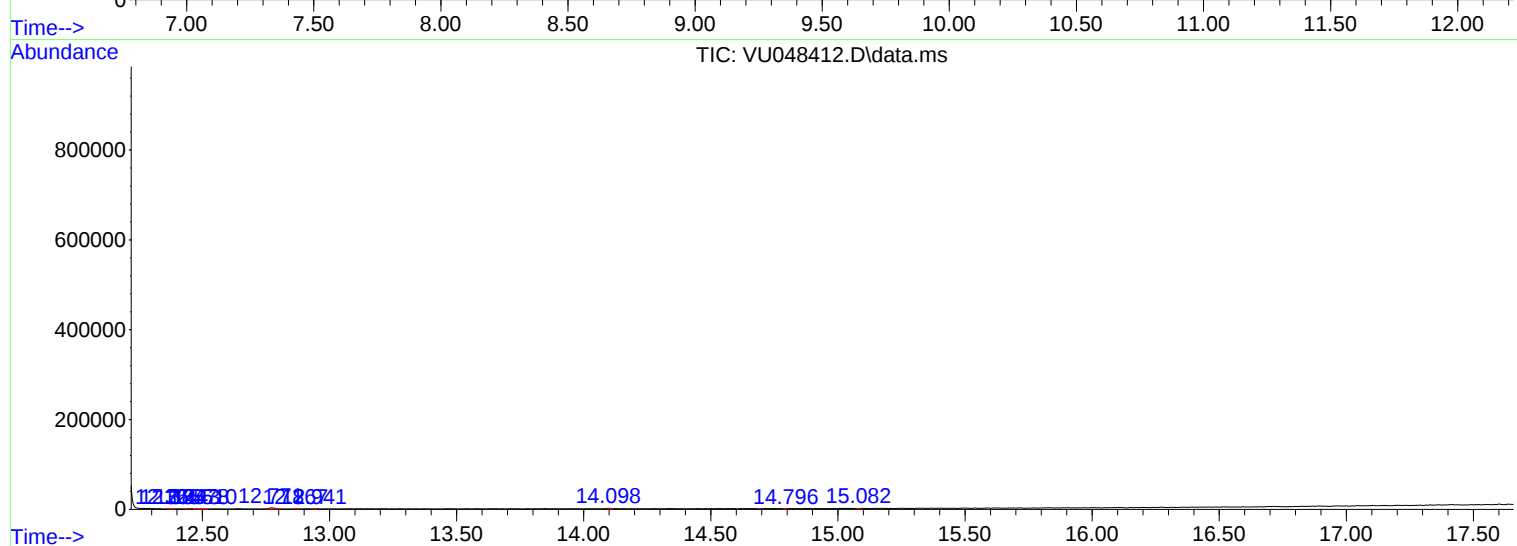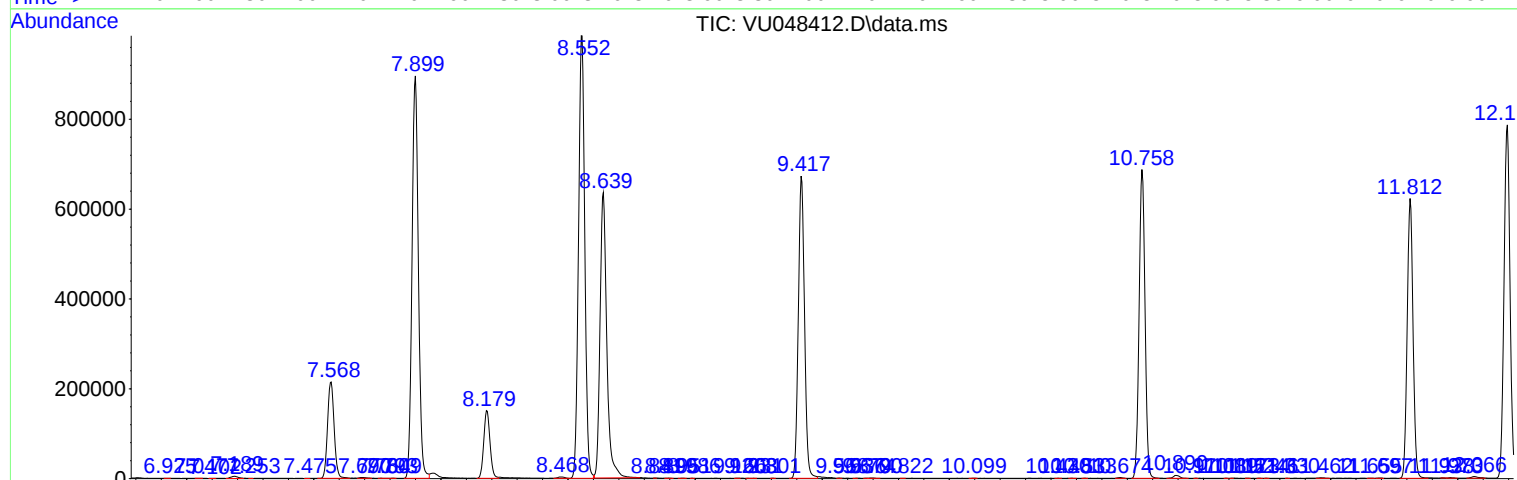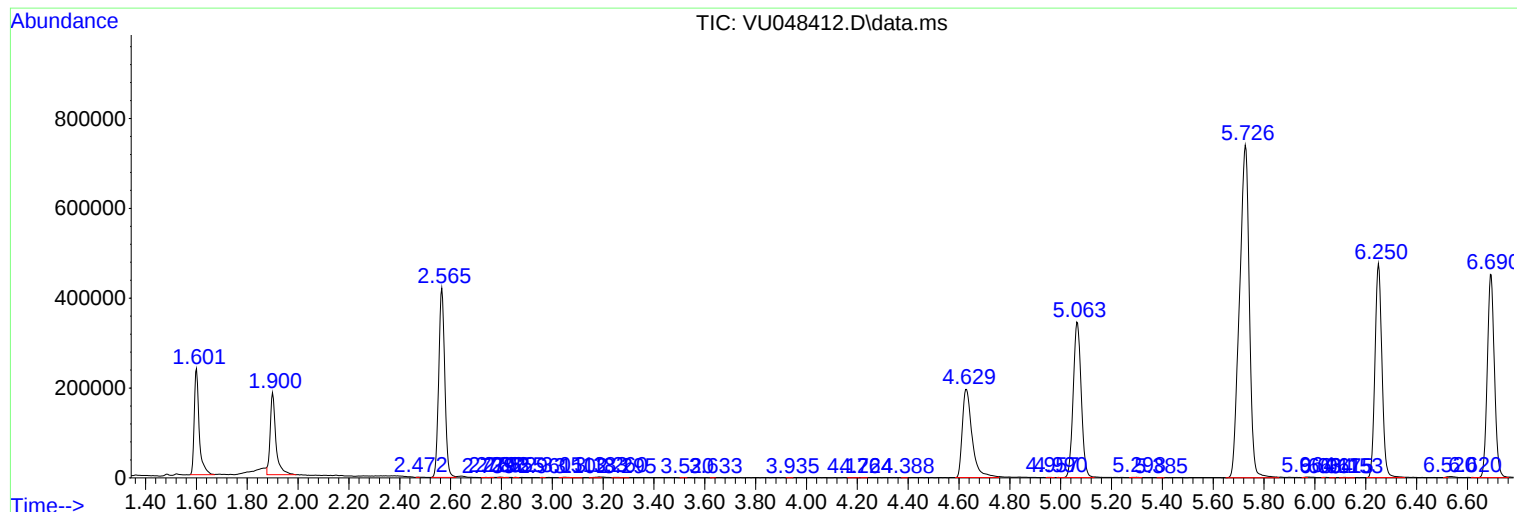

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048412.D
Acq On : 04 May 2022 12:52
Operator : SY/MD
Sample : N2668-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048412.D
Acq On : 04 May 2022 12:52
Operator : SY/MD
Sample : N2668-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------