


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050422\
Data File : VU048404.D
Acq On : 04 May 2022 08:59
Operator : SY/MD
Sample : BFB079
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB079

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Title : VOC Analysis
Last Update : Fri May 06 05:30:23 2022

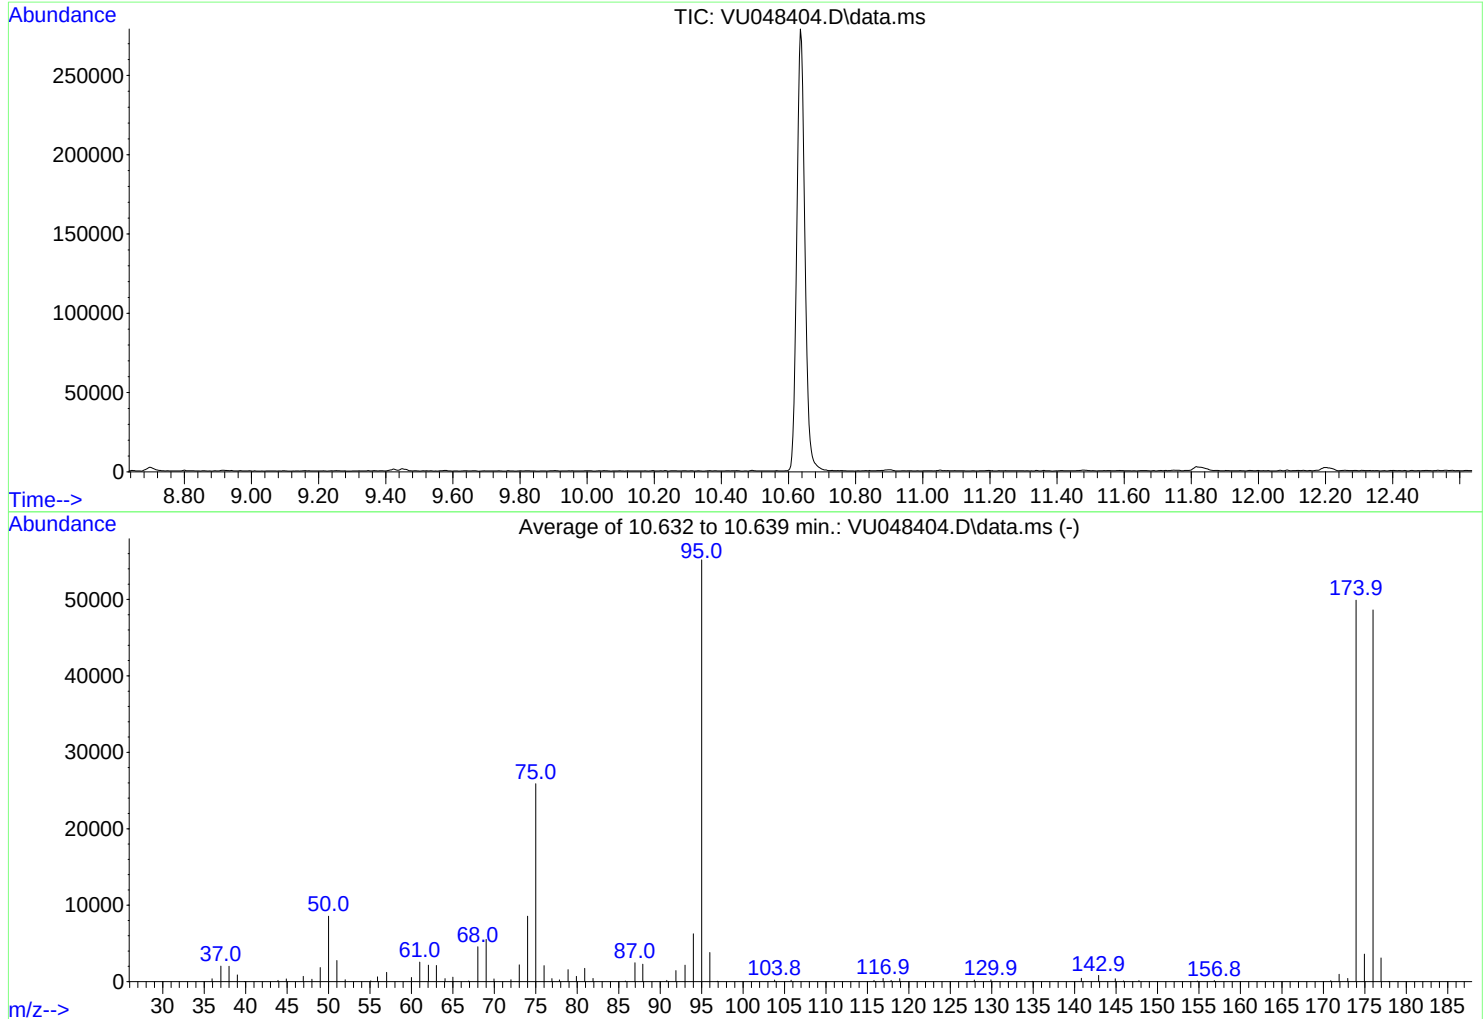

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	8563	PASS
75	95	30	80	46.9	25885	PASS
95	95	100	100	100.0	55179	PASS
96	95	5	9	6.9	3818	PASS
173	174	0.00	2	0.8	421	PASS
174	95	50	120	90.4	49899	PASS
175	174	5	9	7.2	3592	PASS
176	174	95	101	97.4	48624	PASS
177	176	5	9	6.4	3095	PASS

Scan 2878 (10.594 min): VU048404.D\data.ms
BFB079

m/z	Abundance
39.80	243.0
43.90	485.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	374.0
37.00	1951.0
38.00	2058.0
39.00	882.0
40.00	295.0
44.00	656.0
44.90	347.0
46.90	644.0
48.00	314.0
49.00	1774.0
50.00	8429.0
51.00	2749.0
52.00	233.0
55.90	576.0
57.00	1105.0
60.00	484.0
61.00	2319.0
62.10	2197.0
63.00	2054.0
64.10	359.0
65.00	554.0
66.90	156.0
68.00	4678.0
69.00	5433.0
70.00	384.0
72.00	203.0
73.00	2188.0
74.00	8222.0
75.00	25112.0
76.00	2025.0
77.00	406.0
77.90	243.0
78.90	1547.0
79.90	665.0
80.90	1648.0
81.90	401.0
85.80	139.0
87.00	2531.0
87.90	2354.0
90.80	179.0
91.90	1376.0
93.00	2143.0
94.00	6223.0
95.00	53520.0
96.00	3838.0
96.90	106.0
103.80	179.0
105.80	169.0
115.80	193.0
116.90	413.0
117.90	156.0
118.90	353.0
127.90	225.0
129.90	200.0
140.80	369.0
142.90	765.0
144.90	377.0
147.80	150.0
154.80	140.0
156.80	122.0
170.90	128.0
171.90	912.0
172.90	604.0
174.00	47608.0
174.90	3455.0
176.00	45888.0
177.00	2993.0
177.90	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
36.00	396.0
37.00	2069.0
38.00	2102.0
39.00	919.0
40.00	259.0
43.90	637.0
44.90	386.0
46.90	731.0
48.00	343.0
49.00	1890.0
50.00	8799.0
51.00	2855.0
52.00	269.0
55.10	134.0
55.90	638.0
57.00	1261.0
60.00	575.0
61.00	2649.0
62.00	2208.0
63.00	2201.0
64.00	393.0
65.00	617.0
66.90	123.0
68.00	4711.0
69.00	5720.0
70.00	369.0
72.00	272.0
73.00	2255.0
74.00	8846.0
75.00	26712.0
76.00	2143.0
76.90	406.0
77.80	231.0
78.90	1607.0
79.90	727.0
80.90	1776.0
81.90	414.0
85.80	126.0
87.00	2545.0
87.90	2330.0
90.80	163.0
91.90	1477.0
93.00	2223.0
94.00	6500.0
95.00	56840.0
96.00	3903.0
96.90	100.0
103.80	223.0
105.80	200.0
115.80	173.0
116.90	428.0
117.80	170.0
118.90	406.0
127.90	231.0
129.90	231.0
140.80	449.0
142.90	849.0
144.90	405.0
145.90	129.0
147.80	158.0
154.80	116.0
156.80	146.0
170.90	139.0
171.90	994.0
173.00	658.0
174.00	51224.0
175.00	3631.0
176.00	50304.0
176.90	3156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
36.00	375.0
37.00	2063.0
38.00	1886.0
39.00	858.0
39.90	248.0
43.90	644.0
44.90	369.0
47.00	716.0
48.00	319.0
49.00	1840.0
50.00	8462.0
51.00	2710.0
52.00	235.0
55.10	155.0
55.90	684.0
57.00	1261.0
60.00	560.0
61.00	2666.0
62.00	2052.0
63.00	2090.0
64.00	440.0
65.00	608.0
68.00	4319.0
69.00	5436.0
69.90	346.0
72.00	280.0
73.00	2134.0
74.00	8603.0
75.00	25832.0
76.00	2109.0
76.90	360.0
77.80	205.0
78.90	1546.0
79.90	710.0
80.90	1766.0
81.90	456.0
86.90	2327.0
87.90	2144.0
90.80	146.0
91.90	1489.0
93.00	2089.0
94.00	6060.0
95.00	55176.0
96.00	3712.0
103.80	262.0
105.80	194.0
115.80	124.0
116.90	411.0
117.80	178.0
118.90	416.0
127.90	198.0
129.90	238.0
134.90	110.0
140.80	489.0
142.90	835.0
144.90	376.0
145.90	165.0
147.70	138.0
156.90	162.0
170.90	132.0
171.90	956.0
173.90	50864.0
175.00	3689.0
176.00	49680.0
176.90	3137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079