

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054062.D
 Acq On : 04 May 2023 15:18
 Operator : JC/MD
 Sample : 02574-14ME
 Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP7ME

Quant Time: May 05 04:36:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 05 04:34:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	262373	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	244176	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	122665	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	63982	32.243	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	64.480%	
7) Chloroethane-d5	1.906	69	41797	32.088	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	64.180%#	
11) 1,1-Dichloroethene-d2	2.546	63	103193	29.320	ug/L	-0.02
Spiked Amount	50.000	Range 60 - 125	Recovery	=	58.640%#	
21) 2-Butanone-d5	4.632	46	99373	87.805	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	87.800%	
24) Chloroform-d	5.057	84	140539	38.562	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	77.120%	
26) 1,2-Dichloroethane-d4	5.694	65	103194	44.100	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.200%	
32) Benzene-d6	5.719	84	301188	41.905	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.820%	
36) 1,2-Dichloropropane-d6	6.684	67	98463	43.395	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	86.800%	
41) Toluene-d8	7.893	98	268407	41.364	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	82.720%	
43) trans-1,3-Dichloroprop...	8.176	79	47923	42.679	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.360%	
47) 2-Hexanone-d5	8.658	63	69898	86.009	ug/L	0.03
Spiked Amount	100.000	Range 45 - 130	Recovery	=	86.010%	
56) 1,1,2,2-Tetrachloroeth...	10.761	84	130276	43.589	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	87.180%	
66) 1,2-Dichlorobenzene-d4	12.192	152	108149	45.132	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	90.260%	
Target Compounds					Qvalue	
13) Acetone	2.642	43	27236	24.518	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054062.D
Acq On : 04 May 2023 15:18
Operator : JC/MD
Sample : 02574-14ME
Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP7ME

Quant Time: May 05 04:36:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 05 04:34:01 2023
Response via : Initial Calibration

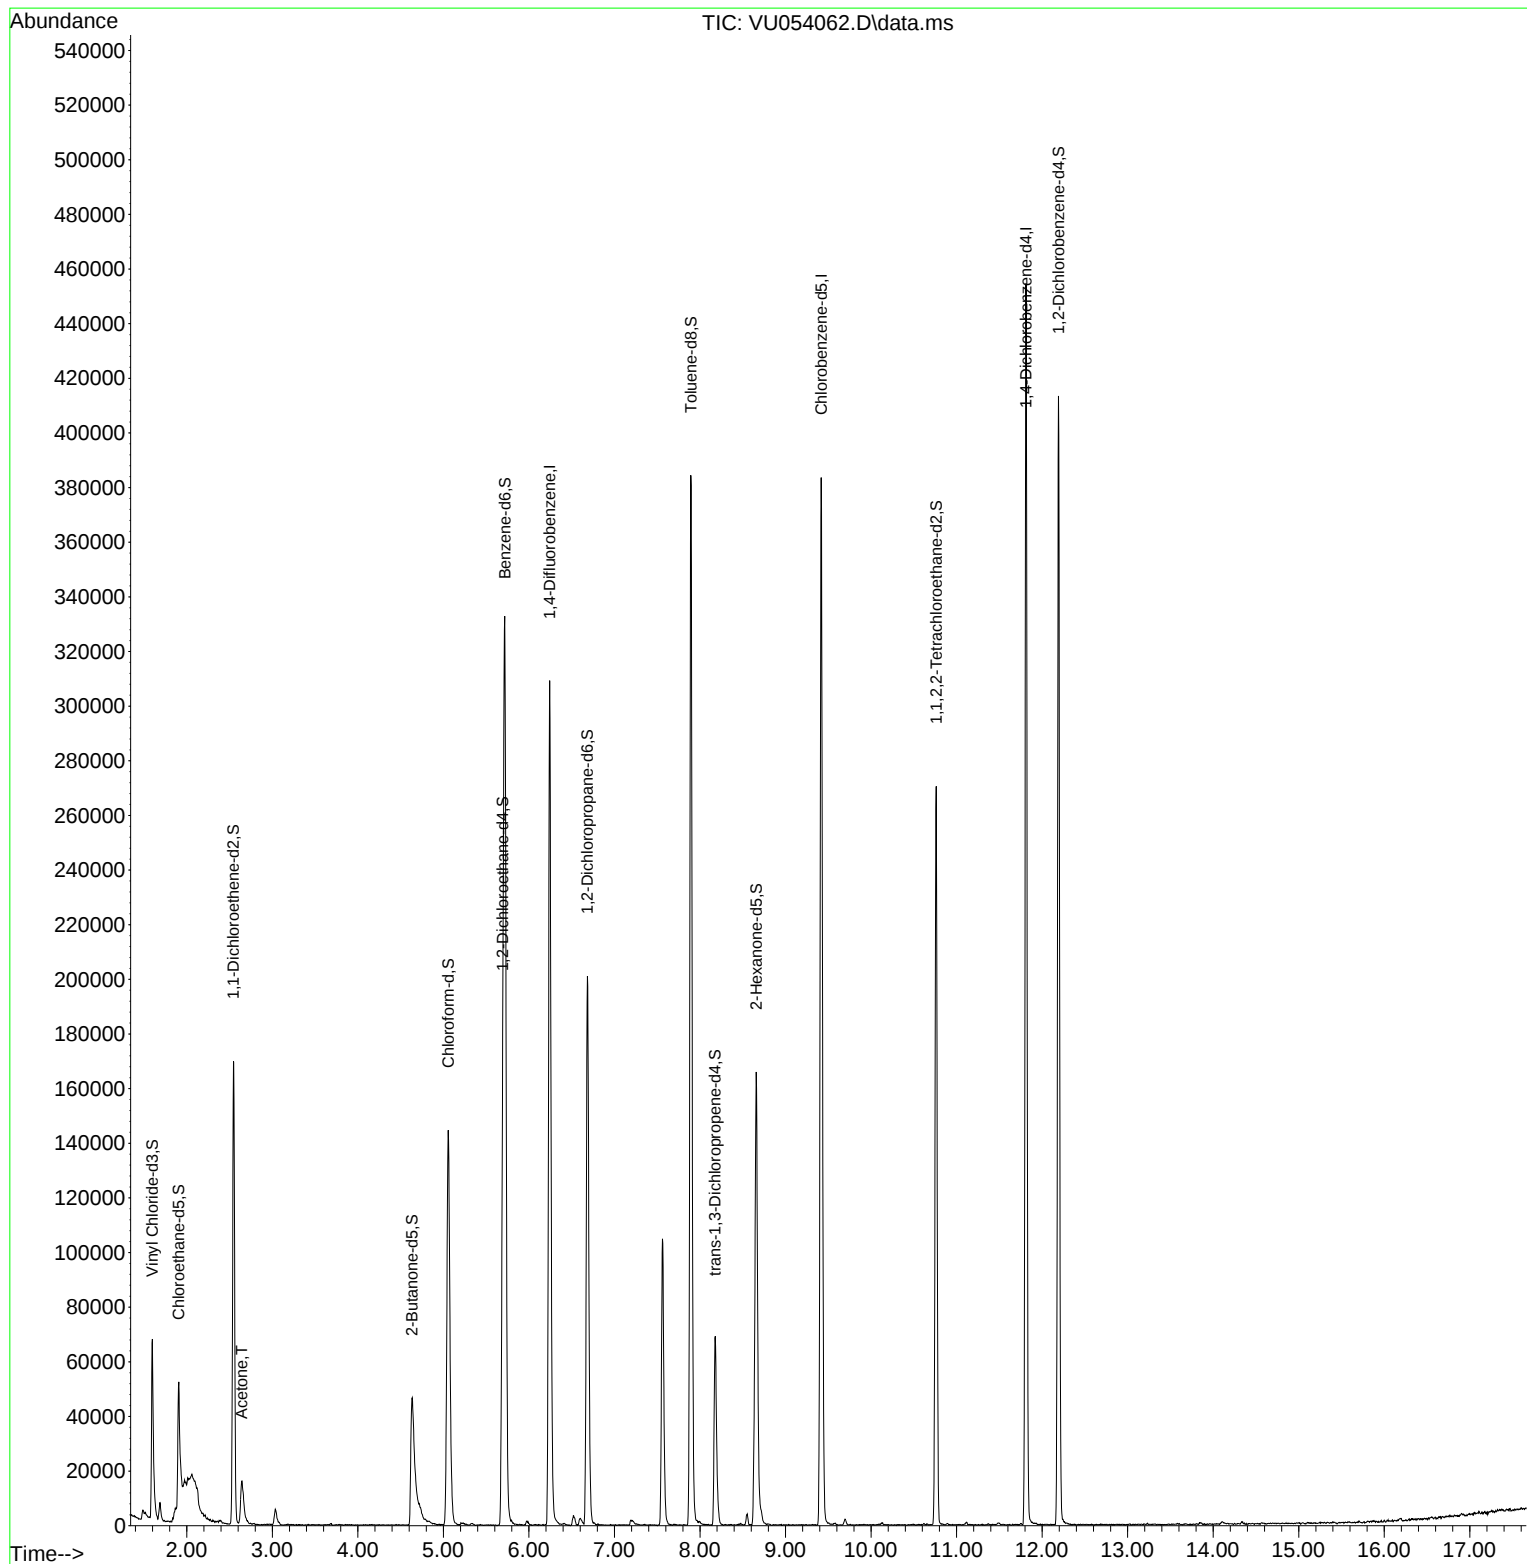

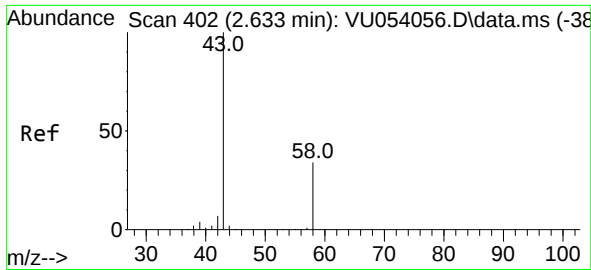

#13

Acetone

Concen: 24.518 ug/L

RT: 2.642 min Scan# 40

Delta R.T. 0.010 min

Lab File: VU054062.D


Acq: 04 May 2023 15:18

Instrument :

MSVOA_U

ClientSampleId :

DCCP7ME

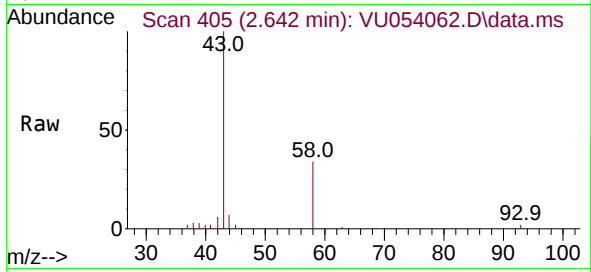

Tgt Ion: 43 Resp: 27236

Ion Ratio Lower Upper

43 100

58 32.5 0.0 67.4

