

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054058.D
 Acq On : 04 May 2023 12:49
 Operator : JC/MD
 Sample : VU0504WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK088

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU054058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	87504	105374	13.50%	1.689%
2	1.825	148	151	156	rBV5	831	707	0.09%	0.011%
3	1.858	158	161	162	rBV3	834	486	0.06%	0.008%
4	1.909	169	177	194	rVB	66619	91309	11.70%	1.464%
5	2.266	284	288	291	rVB3	370	296	0.04%	0.005%
6	2.282	291	293	295	rBV	495	248	0.03%	0.004%
7	2.375	318	322	331	rBV5	481	651	0.08%	0.010%
8	2.565	368	381	398	rBV	158469	261029	33.44%	4.184%
9	2.632	398	402	410	rVV4	800	1172	0.15%	0.019%
10	2.787	445	450	456	rBV2	649	770	0.10%	0.012%
11	3.047	520	531	546	rVB2	6151	11909	1.53%	0.191%
12	3.186	568	574	575	rBV2	233	231	0.03%	0.004%
13	3.285	602	605	609	rVB	252	223	0.03%	0.004%
14	3.350	618	625	638	rVB4	1177	2343	0.30%	0.038%
15	3.401	638	641	645	rBV2	201	227	0.03%	0.004%
16	3.604	698	704	707	rBV2	209	252	0.03%	0.004%
17	3.713	735	738	742	rBV2	209	242	0.03%	0.004%
18	3.822	768	772	774	rBV	294	241	0.03%	0.004%
19	3.912	797	800	804	rBV	399	472	0.06%	0.008%
20	3.999	825	827	835	rBV	139	216	0.03%	0.003%
21	4.237	897	901	906	rVB2	309	295	0.04%	0.005%
22	4.465	966	972	977	rBV2	224	311	0.04%	0.005%
23	4.623	1009	1021	1052	rBV2	62177	160975	20.62%	2.580%
24	4.919	1110	1113	1120	rBV2	519	551	0.07%	0.009%
25	4.976	1129	1131	1135	rVB2	384	230	0.03%	0.004%
26	5.057	1139	1156	1179	rBV	146580	321996	41.25%	5.161%
27	5.173	1190	1192	1196	rVB	389	229	0.03%	0.004%
28	5.205	1200	1202	1207	rVB2	318	244	0.03%	0.004%
29	5.372	1251	1254	1256	rBV3	402	226	0.03%	0.004%
30	5.520	1296	1300	1305	rVV	645	846	0.11%	0.014%
31	5.546	1305	1308	1313	rVB2	316	319	0.04%	0.005%
32	5.719	1339	1362	1379	rBV2	284269	780656	100.00%	12.513%
33	5.845	1398	1401	1407	rVB2	482	510	0.07%	0.008%
34	6.243	1511	1525	1546	rBV	278478	531841	68.13%	8.525%
35	6.369	1560	1564	1567	rBV3	478	385	0.05%	0.006%
36	6.529	1605	1614	1624	rVB6	3186	5717	0.73%	0.092%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054058.D
 Acq On : 04 May 2023 12:49
 Operator : JC/MD
 Sample : VU0504WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK088

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.574	1624	1628	1631	rBV	250	236	0.03%	0.004%
38	6.684	1649	1662	1680	rBV	183102	360343	46.16%	5.776%
39	6.912	1729	1733	1736	rBV2	190	218	0.03%	0.003%
40	7.099	1788	1791	1793	rVV	422	302	0.04%	0.005%
41	7.111	1793	1795	1801	rVB3	329	256	0.03%	0.004%
42	7.185	1814	1818	1828	rBV3	316	389	0.05%	0.006%
43	7.378	1873	1878	1884	rVB2	260	381	0.05%	0.006%
44	7.459	1898	1903	1906	rVB2	237	222	0.03%	0.004%
45	7.562	1920	1935	1952	rBV	99904	178204	22.83%	2.856%
46	7.693	1973	1976	1979	rBV	494	408	0.05%	0.007%
47	7.787	2002	2005	2012	rBV4	664	824	0.11%	0.013%
48	7.893	2024	2038	2057	rBV	352694	611907	78.38%	9.808%
49	8.176	2115	2126	2144	rBV2	71493	122827	15.73%	1.969%
50	8.295	2160	2163	2168	rBV2	348	333	0.04%	0.005%
51	8.320	2168	2171	2174	rVV2	387	224	0.03%	0.004%
52	8.398	2192	2195	2203	rVB3	749	605	0.08%	0.010%
53	8.552	2236	2243	2249	rBV3	1392	1771	0.23%	0.028%
54	8.629	2256	2267	2298	rBV2	181188	355047	45.48%	5.691%
55	8.867	2335	2341	2344	rBV2	238	285	0.04%	0.005%
56	8.925	2352	2359	2362	rBV3	530	570	0.07%	0.009%
57	9.037	2391	2394	2400	rVB2	285	225	0.03%	0.004%
58	9.095	2406	2412	2415	rVB2	303	311	0.04%	0.005%
59	9.121	2415	2420	2423	rBV2	234	283	0.04%	0.005%
60	9.240	2453	2457	2463	rVB2	438	634	0.08%	0.010%
61	9.279	2464	2469	2474	rBV2	380	578	0.07%	0.009%
62	9.414	2498	2511	2538	rBV	377373	635330	81.38%	10.183%
63	9.655	2583	2586	2590	rBV2	236	275	0.04%	0.004%
64	9.697	2591	2599	2608	rVB3	1063	2070	0.27%	0.033%
65	9.735	2608	2611	2618	rVB	292	346	0.04%	0.006%
66	9.793	2622	2629	2630	rBV	225	280	0.04%	0.004%
67	10.108	2718	2727	2742	rVB4	1582	3317	0.42%	0.053%
68	10.404	2816	2819	2824	rVB2	360	261	0.03%	0.004%
69	10.484	2837	2844	2851	rBV2	1100	1705	0.22%	0.027%
70	10.642	2886	2893	2899	rVB5	975	1381	0.18%	0.022%
71	10.751	2914	2927	2943	rBV2	255750	410325	52.56%	6.577%
72	10.822	2946	2949	2953	rVV3	771	580	0.07%	0.009%
73	11.092	3023	3033	3040	rBV4	1017	1695	0.22%	0.027%
74	11.176	3054	3059	3060	rBV2	285	238	0.03%	0.004%
75	11.243	3076	3080	3084	rBV2	239	245	0.03%	0.004%
76	11.471	3143	3151	3165	rBV3	1217	2036	0.26%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054058.D
 Acq On : 04 May 2023 12:49
 Operator : JC/MD
 Sample : VU0504WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK088

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.677	3211	3215	3219	rBV2	223	230	0.03%	0.004%
78	11.745	3229	3236	3243	rVV3	1792	2288	0.29%	0.037%
79	11.806	3243	3255	3284	rBV	394480	631957	80.95%	10.129%
80	11.947	3297	3299	3303	rBV2	485	300	0.04%	0.005%
81	12.069	3333	3337	3340	rBV2	254	232	0.03%	0.004%
82	12.188	3361	3374	3403	rBV	363963	598125	76.62%	9.587%
83	12.320	3411	3415	3418	rVB2	410	299	0.04%	0.005%
84	12.552	3483	3487	3490	rBV2	272	283	0.04%	0.005%
85	12.725	3535	3541	3545	rVB2	248	347	0.04%	0.006%
86	12.748	3545	3548	3552	rBV	250	268	0.03%	0.004%
87	13.220	3689	3695	3708	rVB5	1726	2739	0.35%	0.044%
88	13.452	3761	3767	3774	rVB3	483	571	0.07%	0.009%
89	13.491	3774	3779	3784	rBV	324	319	0.04%	0.005%
90	13.841	3881	3888	3897	rBV4	3110	4843	0.62%	0.078%
91	13.976	3926	3930	3932	rBV	432	266	0.03%	0.004%
92	14.092	3957	3966	3973	rBV2	4298	7188	0.92%	0.115%
93	14.298	4026	4030	4032	rBV2	297	259	0.03%	0.004%
94	14.330	4033	4040	4048	rVV5	3162	4561	0.58%	0.073%
95	14.564	4109	4113	4119	rBV2	668	781	0.10%	0.013%
96	14.632	4130	4134	4138	rBV2	403	378	0.05%	0.006%
97	15.050	4261	4264	4266	rBV2	368	262	0.03%	0.004%
98	15.146	4290	4294	4298	rBV	570	563	0.07%	0.009%
99	15.828	4503	4506	4508	rBV2	560	340	0.04%	0.005%
100	15.976	4549	4552	4554	rBV3	450	308	0.04%	0.005%




Sum of corrected areas: 6238903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054058.D
Acq On : 04 May 2023 12:49
Operator : JC/MD
Sample : VU0504WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK088

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

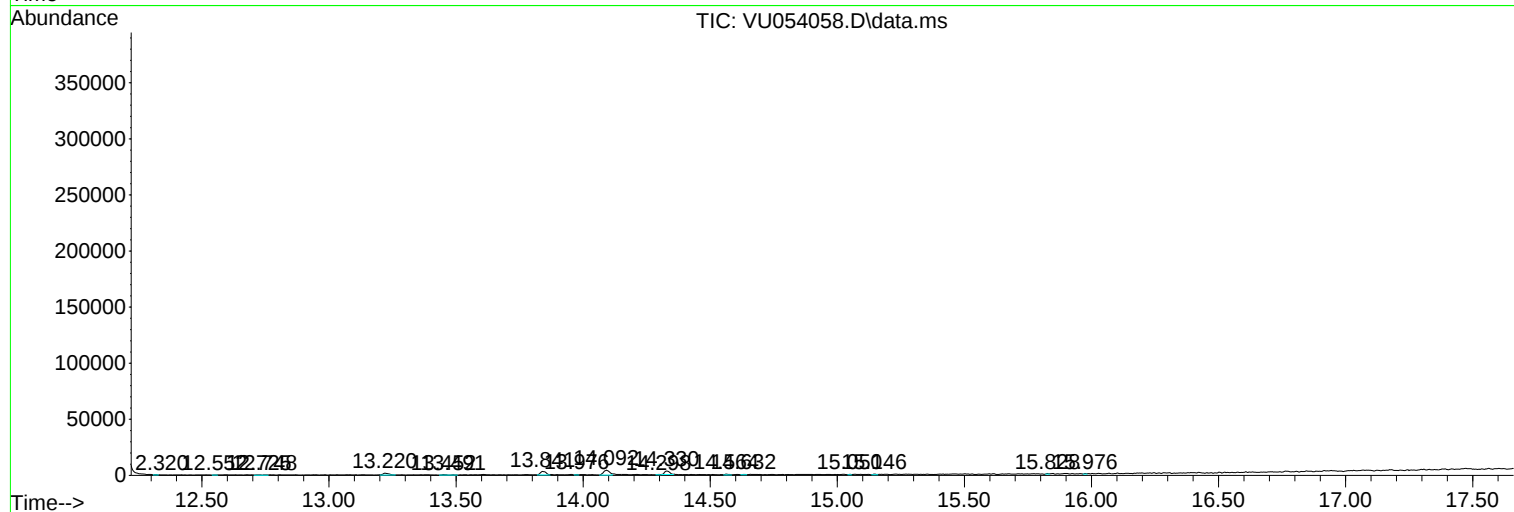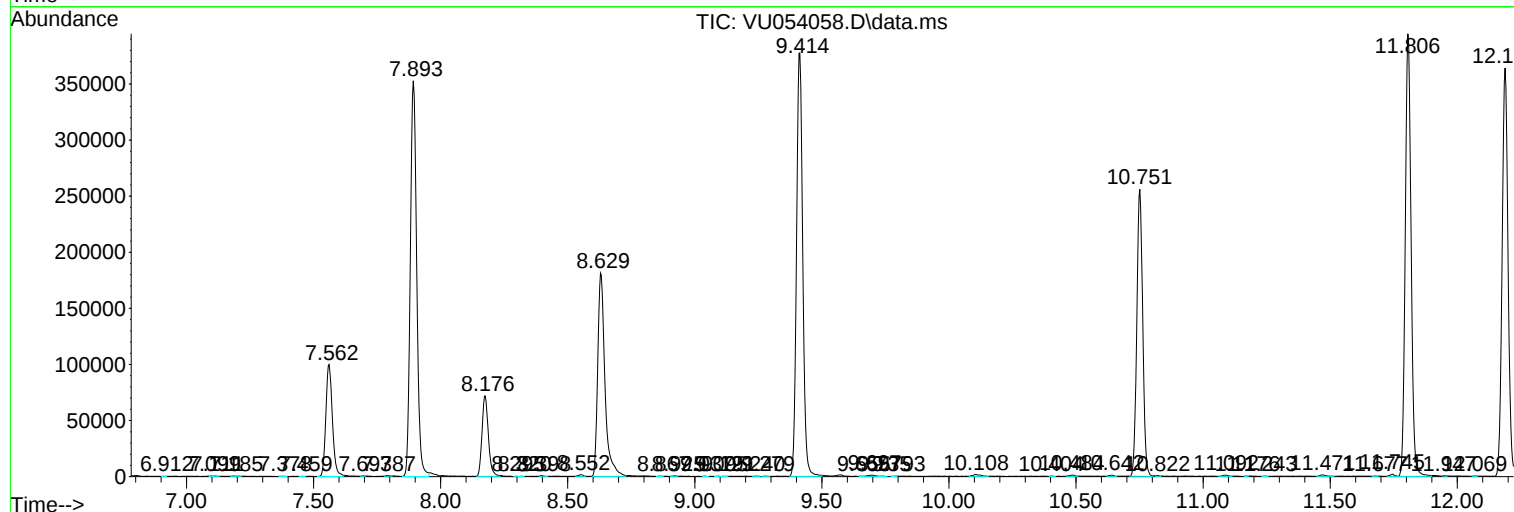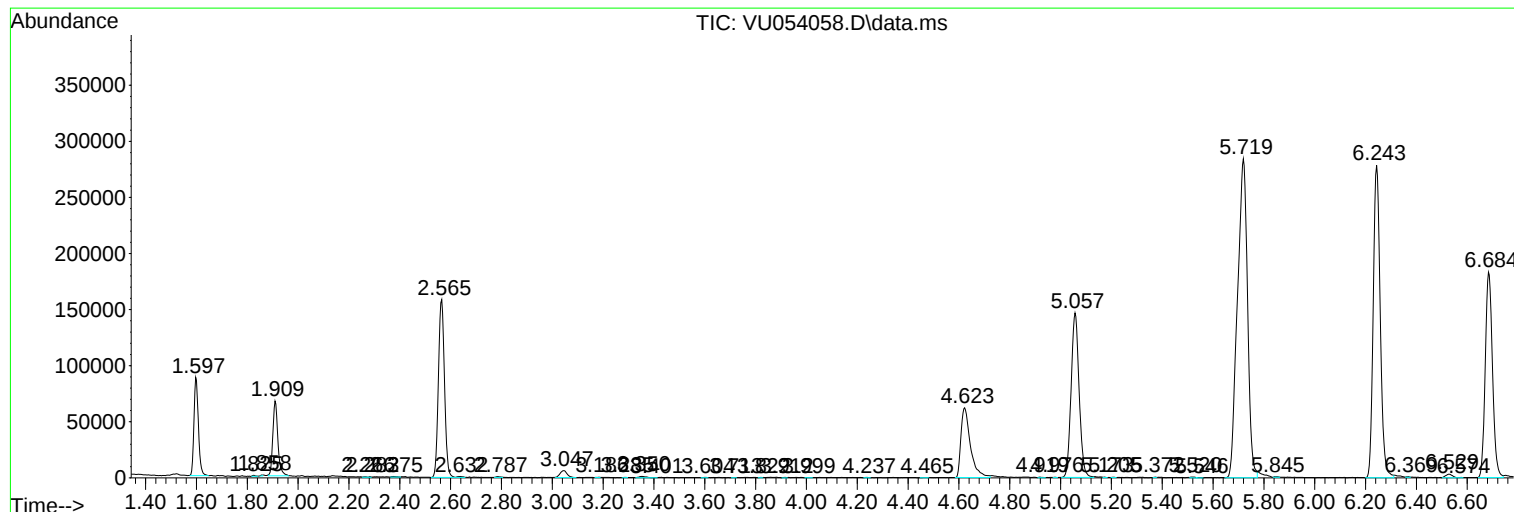

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054058.D
Acq On : 04 May 2023 12:49
Operator : JC/MD
Sample : VU0504WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK088

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054058.D
Acq On : 04 May 2023 12:49
Operator : JC/MD
Sample : VU0504WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK088

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc