

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054062.D
 Acq On : 04 May 2023 15:18
 Operator : JC/MD
 Sample : 02574-14ME
 Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU054062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	40	46	51	rBV6	3268	4941	0.56%	0.071%
2	1.597	72	80	100	rVV	66049	100711	11.43%	1.453%
3	1.687	100	108	120	rVB	6821	10889	1.24%	0.157%
4	1.871	150	165	166	rBV6	5122	8584	0.97%	0.124%
5	1.906	168	176	189	rBV	46219	83367	9.46%	1.203%
6	2.379	320	323	325	rBV3	800	530	0.06%	0.008%
7	2.546	363	375	393	rBV	169212	275254	31.25%	3.972%
8	2.645	394	406	425	rBV	15403	38984	4.43%	0.563%
9	2.906	480	487	489	rBV	339	394	0.04%	0.006%
10	2.935	493	496	500	rVV	235	206	0.02%	0.003%
11	3.034	517	527	538	rBV4	5700	11474	1.30%	0.166%
12	3.276	596	602	603	rBV	299	289	0.03%	0.004%
13	3.308	607	612	613	rBV2	276	226	0.03%	0.003%
14	3.346	622	624	631	rVB2	243	256	0.03%	0.004%
15	3.385	632	636	643	rBV	161	217	0.02%	0.003%
16	3.514	671	676	679	rBV	173	234	0.03%	0.003%
17	3.684	724	729	730	rBV2	488	425	0.05%	0.006%
18	3.970	815	818	823	rBV2	249	277	0.03%	0.004%
19	4.253	902	906	911	rVB2	295	316	0.04%	0.005%
20	4.285	911	916	919	rBV	257	311	0.04%	0.004%
21	4.481	974	977	985	rVB2	259	327	0.04%	0.005%
22	4.520	985	989	992	rBV2	196	210	0.02%	0.003%
23	4.636	1013	1025	1049	rBV	46501	152666	17.33%	2.203%
24	4.951	1118	1123	1126	rVB3	331	326	0.04%	0.005%
25	4.976	1128	1131	1138	rVV2	230	296	0.03%	0.004%
26	5.057	1139	1156	1190	rVV2	144480	357354	40.57%	5.157%
27	5.205	1199	1202	1205	rBV4	675	500	0.06%	0.007%
28	5.324	1234	1239	1240	rBV2	458	326	0.04%	0.005%
29	5.411	1261	1266	1269	rBV2	217	254	0.03%	0.004%
30	5.552	1305	1310	1313	rBV2	247	252	0.03%	0.004%
31	5.716	1340	1361	1384	rVV2	332708	880924	100.00%	12.713%
32	5.976	1436	1442	1446	rBV5	1406	1851	0.21%	0.027%
33	6.115	1482	1485	1488	rBV2	358	289	0.03%	0.004%
34	6.160	1494	1499	1500	rBV	238	211	0.02%	0.003%
35	6.192	1504	1509	1511	rBV2	370	307	0.03%	0.004%
36	6.243	1511	1525	1556	rBV	308967	607211	68.93%	8.763%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054062.D
 Acq On : 04 May 2023 15:18
 Operator : JC/MD
 Sample : 02574-14ME
 Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.520	1599	1611	1623	rBV5	3732	7748	0.88%	0.112%
38	6.600	1625	1636	1649	rBV5	2565	6279	0.71%	0.091%
39	6.684	1649	1662	1683	rBV	200582	401975	45.63%	5.801%
40	6.806	1697	1700	1704	rVB2	585	476	0.05%	0.007%
41	6.832	1704	1708	1710	rBV	300	259	0.03%	0.004%
42	6.954	1744	1746	1750	rVB2	299	217	0.02%	0.003%
43	7.076	1781	1784	1788	rBV2	232	222	0.03%	0.003%
44	7.192	1814	1820	1823	rBV3	1818	2106	0.24%	0.030%
45	7.417	1884	1890	1892	rBV2	266	271	0.03%	0.004%
46	7.517	1917	1921	1923	rBV2	351	328	0.04%	0.005%
47	7.562	1923	1935	1958	rVV	104791	199968	22.70%	2.886%
48	7.690	1971	1975	1977	rBV2	365	307	0.03%	0.004%
49	7.893	2024	2038	2059	rBV	384287	699325	79.39%	10.092%
50	8.127	2107	2111	2115	rVB2	219	218	0.02%	0.003%
51	8.179	2115	2127	2151	rBV	69213	137139	15.57%	1.979%
52	8.295	2157	2163	2166	rBV2	356	405	0.05%	0.006%
53	8.356	2178	2182	2184	rBV2	342	294	0.03%	0.004%
54	8.552	2234	2243	2251	rVB4	4077	6021	0.68%	0.087%
55	8.658	2259	2276	2304	rBV	165921	369285	41.92%	5.329%
56	9.417	2496	2512	2537	rBV	383528	717430	81.44%	10.354%
57	9.568	2556	2559	2561	rBV	386	273	0.03%	0.004%
58	9.600	2567	2569	2574	rVB3	316	262	0.03%	0.004%
59	9.697	2588	2599	2610	rBV3	2189	3880	0.44%	0.056%
60	9.754	2615	2617	2624	rVB2	359	340	0.04%	0.005%
61	9.787	2624	2627	2632	rBV2	188	225	0.03%	0.003%
62	9.828	2636	2640	2647	rBV	286	421	0.05%	0.006%
63	9.883	2653	2657	2660	rBV2	239	238	0.03%	0.003%
64	9.989	2685	2690	2693	rBV2	237	290	0.03%	0.004%
65	10.124	2729	2732	2734	rBV4	493	349	0.04%	0.005%
66	10.279	2776	2780	2786	rBV	273	294	0.03%	0.004%
67	10.311	2786	2790	2793	rBV2	242	276	0.03%	0.004%
68	10.619	2883	2886	2890	rVB2	444	359	0.04%	0.005%
69	10.652	2894	2896	2898	rBV2	359	208	0.02%	0.003%
70	10.761	2917	2930	2948	rBV	270128	435239	49.41%	6.281%
71	10.893	2964	2971	2976	rVB3	508	684	0.08%	0.010%
72	11.092	3028	3033	3035	rBV2	385	324	0.04%	0.005%
73	11.217	3068	3072	3076	rBV2	330	317	0.04%	0.005%
74	11.487	3148	3156	3159	rBV3	655	910	0.10%	0.013%
75	11.655	3203	3208	3211	rBV2	414	352	0.04%	0.005%
76	11.677	3211	3215	3217	rBV2	286	216	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054062.D
 Acq On : 04 May 2023 15:18
 Operator : JC/MD
 Sample : 02574-14ME
 Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.751	3233	3238	3239	rBV2	505	391	0.04%	0.006%
78	11.812	3245	3257	3278	rBV	454418	717778	81.48%	10.359%
79	12.192	3363	3375	3395	rBV	413104	666335	75.64%	9.616%
80	12.635	3505	3513	3519	rBV2	314	604	0.07%	0.009%
81	12.857	3578	3582	3585	rBV2	254	293	0.03%	0.004%
82	12.986	3618	3622	3624	rBV2	232	213	0.02%	0.003%
83	13.057	3641	3644	3646	rBV2	292	206	0.02%	0.003%
84	13.089	3650	3654	3656	rBV	296	221	0.03%	0.003%
85	13.230	3695	3698	3701	rVB3	517	342	0.04%	0.005%
86	13.352	3732	3736	3741	rBV2	227	320	0.04%	0.005%
87	13.407	3750	3753	3757	rBV2	229	230	0.03%	0.003%
88	13.581	3804	3807	3811	rVV3	332	249	0.03%	0.004%
89	13.651	3826	3829	3832	rBV2	261	212	0.02%	0.003%
90	13.732	3851	3854	3856	rVB	392	242	0.03%	0.003%
91	13.803	3873	3876	3880	rBV2	296	235	0.03%	0.003%
92	13.841	3884	3888	3890	rBV2	715	516	0.06%	0.007%
93	13.896	3902	3905	3909	rVB2	469	344	0.04%	0.005%
94	14.085	3961	3964	3965	rBV2	435	282	0.03%	0.004%
95	14.249	4012	4015	4019	rVB3	357	272	0.03%	0.004%
96	14.336	4036	4042	4044	rBV3	907	899	0.10%	0.013%
97	14.362	4048	4050	4055	rVB2	429	226	0.03%	0.003%
98	14.571	4108	4115	4118	rBV4	602	842	0.10%	0.012%
99	15.703	4465	4467	4476	rVB3	649	535	0.06%	0.008%
100	16.002	4556	4560	4564	rVB3	759	622	0.07%	0.009%




Sum of corrected areas: 6929328

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054062.D
Acq On : 04 May 2023 15:18
Operator : JC/MD
Sample : 02574-14ME
Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

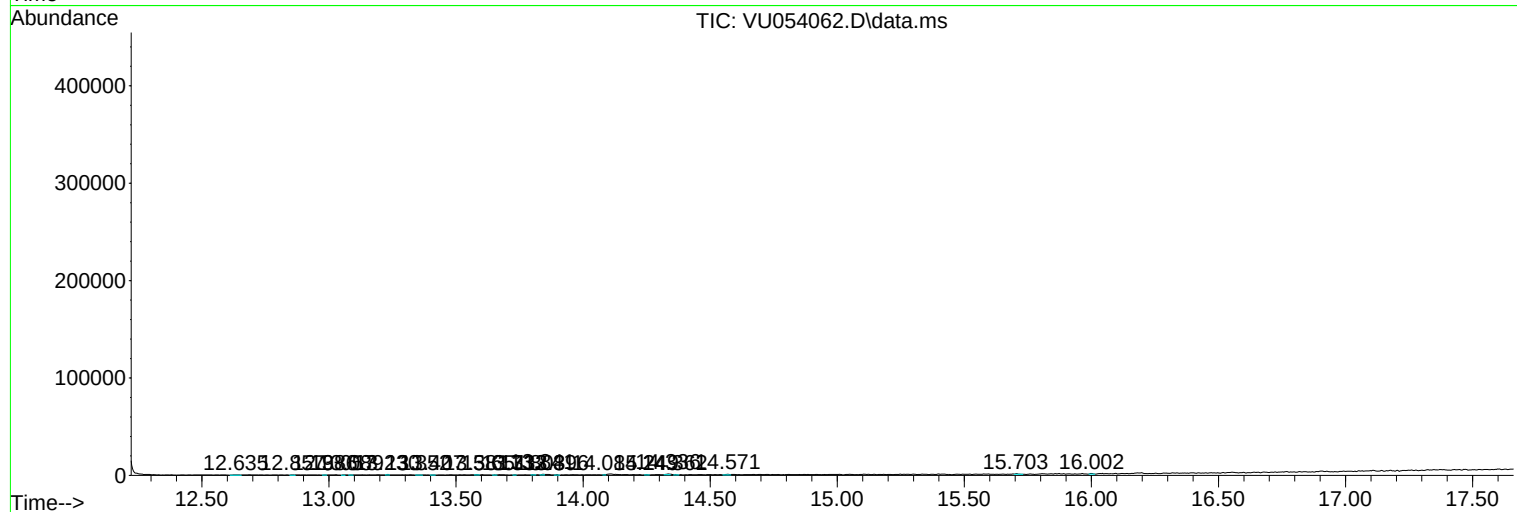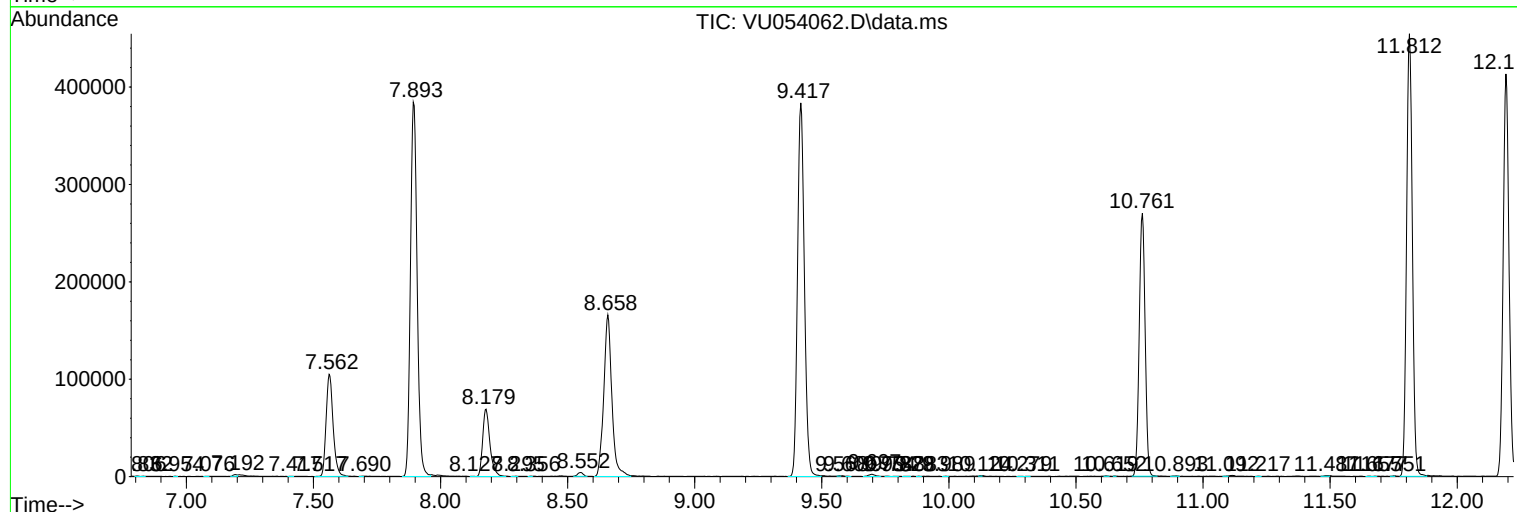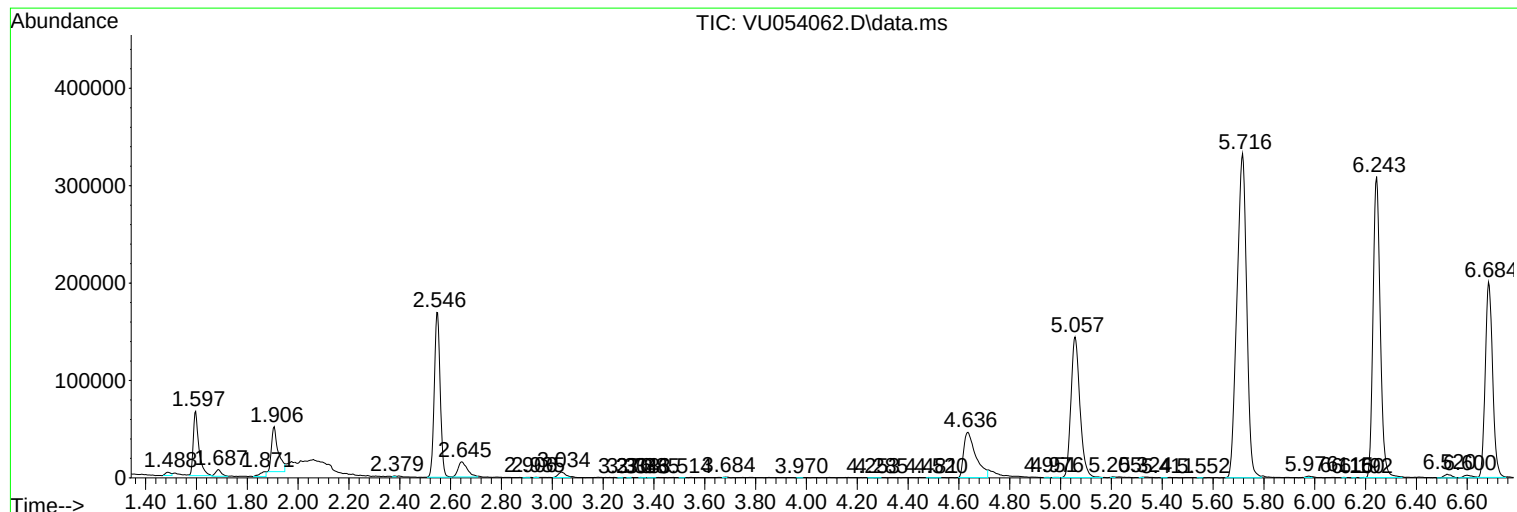

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054062.D
Acq On : 04 May 2023 15:18
Operator : JC/MD
Sample : 02574-14ME
Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054062.D
Acq On : 04 May 2023 15:18
Operator : JC/MD
Sample : 02574-14ME
Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc