

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054064.D
 Acq On : 04 May 2023 16:04
 Operator : JC/MD
 Sample : 02574-09ME
 Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	53	rBV3	1827	2670	0.31%	0.039%
2	1.594	72	79	103	rVB	64711	101086	11.62%	1.473%
3	1.867	155	164	166	rBV7	3694	5513	0.63%	0.080%
4	1.903	168	175	191	rBV	42209	84520	9.72%	1.232%
5	2.305	297	300	304	rVB5	679	449	0.05%	0.007%
6	2.395	323	328	330	rBV4	796	720	0.08%	0.010%
7	2.546	362	375	391	rVB	164446	267851	30.79%	3.903%
8	2.774	440	446	453	rBV3	501	844	0.10%	0.012%
9	2.819	457	460	464	rVB2	289	213	0.02%	0.003%
10	2.880	477	479	485	rBV3	313	255	0.03%	0.004%
11	2.980	507	510	513	rBV2	378	245	0.03%	0.004%
12	3.038	517	528	553	rVB2	7479	17606	2.02%	0.257%
13	3.166	564	568	572	rBV2	376	339	0.04%	0.005%
14	3.687	722	730	733	rVV3	434	627	0.07%	0.009%
15	3.941	805	809	815	rVB2	308	363	0.04%	0.005%
16	3.977	815	820	823	rBV2	244	238	0.03%	0.003%
17	4.012	826	831	836	rVB2	322	314	0.04%	0.005%
18	4.086	851	854	857	rVB2	316	197	0.02%	0.003%
19	4.141	864	871	872	rBV	308	361	0.04%	0.005%
20	4.253	902	906	909	rBV	234	231	0.03%	0.003%
21	4.359	933	939	945	rBV2	347	448	0.05%	0.007%
22	4.591	1005	1011	1012	rBV	227	233	0.03%	0.003%
23	4.632	1012	1024	1064	rBV	48537	172394	19.82%	2.512%
24	5.054	1139	1155	1181	rBV	148337	354569	40.76%	5.167%
25	5.208	1195	1203	1208	rBV3	1084	1309	0.15%	0.019%
26	5.250	1213	1216	1221	rVB3	542	491	0.06%	0.007%
27	5.279	1221	1225	1228	rBV	241	256	0.03%	0.004%
28	5.414	1261	1267	1270	rBV	358	486	0.06%	0.007%
29	5.494	1288	1292	1300	rBV2	255	454	0.05%	0.007%
30	5.713	1340	1360	1391	rBV2	326356	869806	100.00%	12.675%
31	5.825	1393	1395	1402	rVB3	518	554	0.06%	0.008%
32	5.980	1434	1443	1448	rBV4	1422	2387	0.27%	0.035%
33	6.240	1511	1524	1546	rBV	300679	602129	69.23%	8.775%
34	6.391	1568	1571	1574	rBV	438	280	0.03%	0.004%
35	6.523	1603	1612	1622	rVB5	3351	6252	0.72%	0.091%
36	6.600	1624	1636	1648	rBV5	2489	5570	0.64%	0.081%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054064.D
 Acq On : 04 May 2023 16:04
 Operator : JC/MD
 Sample : 02574-09ME
 Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.684	1648	1662	1690	rVV	197707	403088	46.34%	5.874%
38	6.780	1690	1692	1695	rVV2	326	196	0.02%	0.003%
39	6.803	1695	1699	1707	rVB4	417	473	0.05%	0.007%
40	6.980	1748	1754	1755	rBV2	247	221	0.03%	0.003%
41	7.025	1765	1768	1774	rBV2	275	307	0.04%	0.004%
42	7.195	1813	1821	1823	rBV3	1836	2132	0.25%	0.031%
43	7.272	1842	1845	1848	rVB2	388	255	0.03%	0.004%
44	7.320	1856	1860	1863	rVB	415	331	0.04%	0.005%
45	7.340	1863	1866	1869	rBV	270	229	0.03%	0.003%
46	7.562	1923	1935	1957	rVV2	106157	198808	22.86%	2.897%
47	7.690	1971	1975	1976	rBV2	269	189	0.02%	0.003%
48	7.761	1990	1997	1998	rBV2	188	220	0.03%	0.003%
49	7.816	2009	2014	2017	rVB2	244	227	0.03%	0.003%
50	7.893	2022	2038	2057	rBV	379349	686173	78.89%	9.999%
51	8.176	2113	2126	2154	rVB2	66495	134370	15.45%	1.958%
52	8.298	2160	2164	2169	rBV2	183	206	0.02%	0.003%
53	8.391	2189	2193	2198	rVB2	252	274	0.03%	0.004%
54	8.423	2198	2203	2208	rBV	196	283	0.03%	0.004%
55	8.462	2209	2215	2219	rBV3	436	596	0.07%	0.009%
56	8.552	2237	2243	2248	rVB3	1357	1507	0.17%	0.022%
57	8.658	2258	2276	2306	rBV	172470	379342	43.61%	5.528%
58	8.806	2320	2322	2325	rVB3	420	196	0.02%	0.003%
59	9.041	2389	2395	2398	rBV2	293	322	0.04%	0.005%
60	9.417	2498	2512	2540	rBV	373536	721175	82.91%	10.509%
61	9.565	2549	2558	2560	rBV3	848	1001	0.12%	0.015%
62	9.607	2569	2571	2575	rVB2	439	245	0.03%	0.004%
63	9.693	2590	2598	2610	rBV2	2006	3259	0.37%	0.047%
64	10.095	2720	2723	2728	rBV2	330	327	0.04%	0.005%
65	10.118	2728	2730	2732	rBV	390	206	0.02%	0.003%
66	10.169	2742	2746	2749	rBV2	265	254	0.03%	0.004%
67	10.214	2755	2760	2770	rVB2	443	789	0.09%	0.011%
68	10.259	2770	2774	2775	rBV	309	214	0.02%	0.003%
69	10.648	2891	2895	2897	rBV3	457	318	0.04%	0.005%
70	10.758	2916	2929	2948	rBV	270327	442474	50.87%	6.448%
71	10.835	2949	2953	2956	rVB3	529	382	0.04%	0.006%
72	10.918	2976	2979	2983	rBV2	232	220	0.03%	0.003%
73	11.115	3035	3040	3051	rVB6	883	1389	0.16%	0.020%
74	11.304	3095	3099	3100	rBV2	295	189	0.02%	0.003%
75	11.359	3114	3116	3118	rBV	440	260	0.03%	0.004%
76	11.703	3220	3223	3232	rVB2	319	407	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054064.D
 Acq On : 04 May 2023 16:04
 Operator : JC/MD
 Sample : 02574-09ME
 Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.751	3232	3238	3241	rBV2	655	714	0.08%	0.010%
78	11.809	3244	3256	3272	rBV	450312	704675	81.02%	10.269%
79	12.066	3333	3336	3345	rVB2	432	611	0.07%	0.009%
80	12.105	3345	3348	3350	rBV2	228	195	0.02%	0.003%
81	12.192	3362	3375	3403	rVV	420271	664273	76.37%	9.680%
82	12.378	3427	3433	3436	rBV2	276	253	0.03%	0.004%
83	12.549	3483	3486	3492	rBV2	276	302	0.03%	0.004%
84	12.639	3511	3514	3519	rVB2	300	272	0.03%	0.004%
85	12.664	3519	3522	3527	rBV	258	252	0.03%	0.004%
86	12.809	3564	3567	3570	rBV2	302	246	0.03%	0.004%
87	13.089	3650	3654	3657	rBV2	323	295	0.03%	0.004%
88	13.317	3722	3725	3730	rBV	256	216	0.02%	0.003%
89	13.391	3746	3748	3750	rBV	320	196	0.02%	0.003%
90	13.639	3821	3825	3828	rBV	334	349	0.04%	0.005%
91	13.844	3885	3889	3891	rBV2	540	441	0.05%	0.006%
92	13.918	3908	3912	3915	rBV	444	455	0.05%	0.007%
93	14.095	3964	3967	3968	rBV	500	273	0.03%	0.004%
94	14.336	4036	4042	4047	rVB4	825	1064	0.12%	0.016%
95	14.362	4047	4050	4054	rBV2	311	294	0.03%	0.004%
96	14.532	4097	4103	4110	rBV2	371	635	0.07%	0.009%
97	14.565	4110	4113	4114	rBV	395	231	0.03%	0.003%
98	14.674	4144	4147	4149	rBV2	342	224	0.03%	0.003%
99	14.770	4174	4177	4179	rBV	380	252	0.03%	0.004%
100	15.262	4328	4330	4332	rBV	387	218	0.03%	0.003%




Sum of corrected areas: 6862250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054064.D
Acq On : 04 May 2023 16:04
Operator : JC/MD
Sample : 02574-09ME
Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

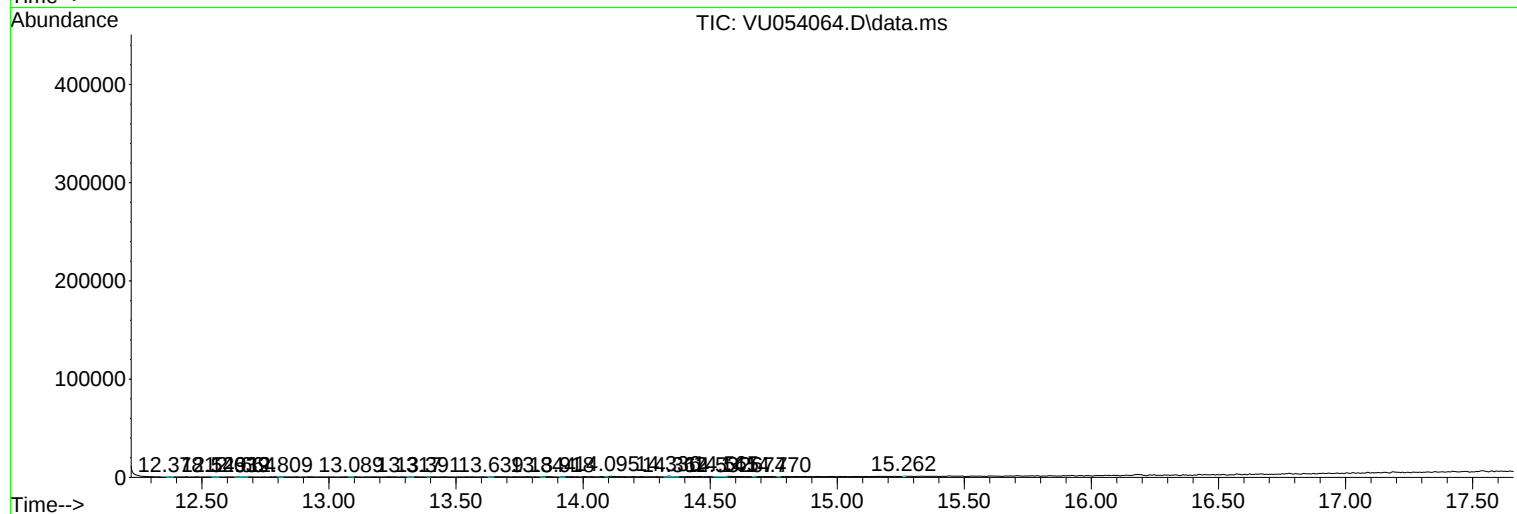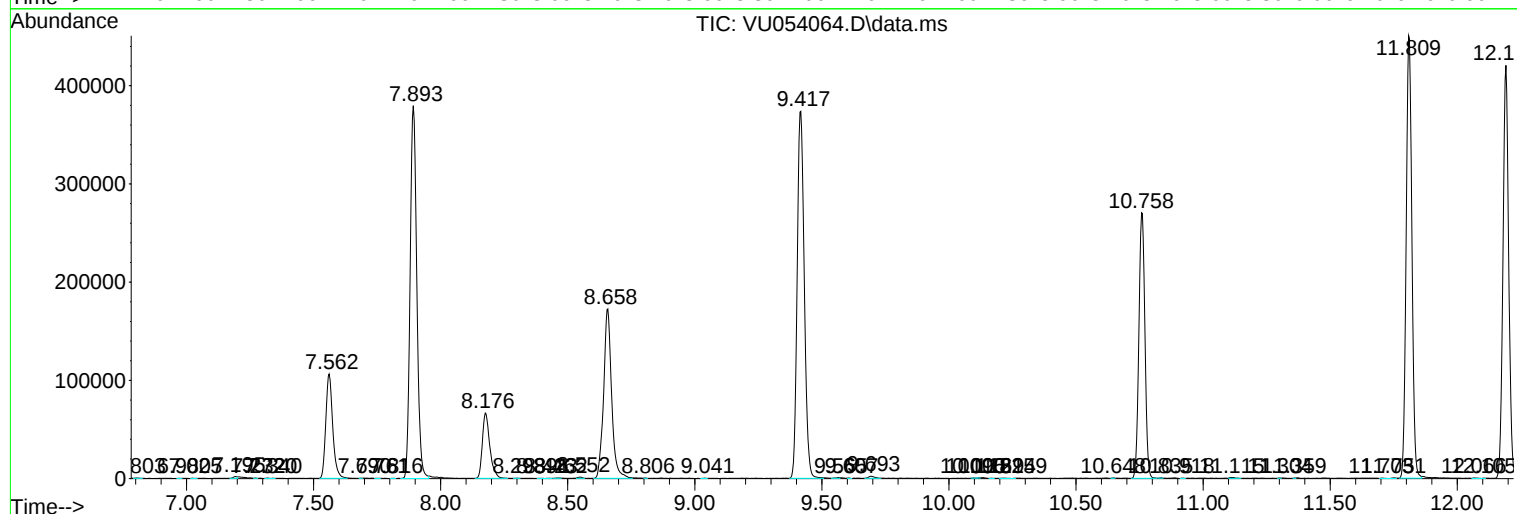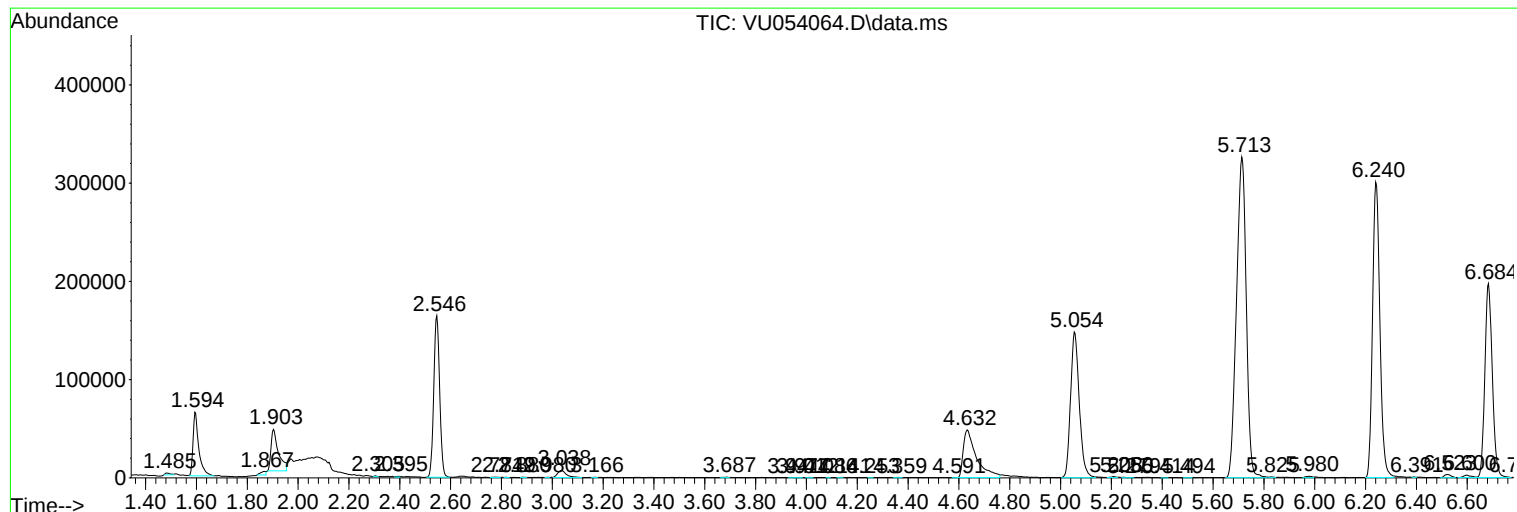

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054064.D
Acq On : 04 May 2023 16:04
Operator : JC/MD
Sample : 02574-09ME
Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054064.D
Acq On : 04 May 2023 16:04
Operator : JC/MD
Sample : 02574-09ME
Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------