

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054065.D
 Acq On : 04 May 2023 16:27
 Operator : JC/MD
 Sample : 02574-10ME
 Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU054065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	106	rVB	62423	98635	11.64%	1.519%
2	1.903	169	175	189	rBV	37622	67060	7.91%	1.033%
3	2.546	363	375	390	rBV	159414	259003	30.56%	3.990%
4	3.035	516	527	545	rBV2	7280	16391	1.93%	0.253%
5	3.147	560	562	564	rBV	122	63	0.01%	0.001%
6	3.166	565	568	572	rBV2	225	211	0.02%	0.003%
7	3.301	601	610	615	rBV2	384	557	0.07%	0.009%
8	3.359	625	628	633	rBV2	246	234	0.03%	0.004%
9	3.395	633	639	640	rBV	190	206	0.02%	0.003%
10	3.723	736	741	744	rBV	294	290	0.03%	0.004%
11	3.748	744	749	752	rBV2	244	291	0.03%	0.004%
12	3.809	765	768	770	rBV	238	172	0.02%	0.003%
13	3.957	809	814	817	rBV2	201	216	0.03%	0.003%
14	4.057	843	845	847	rBV2	221	127	0.01%	0.002%
15	4.070	847	849	853	rVB2	182	127	0.01%	0.002%
16	4.092	853	856	858	rBV	196	141	0.02%	0.002%
17	4.137	868	870	871	rBV	155	82	0.01%	0.001%
18	4.202	886	890	893	rBV2	218	213	0.03%	0.003%
19	4.350	932	936	938	rBV	196	147	0.02%	0.002%
20	4.459	964	970	973	rBV2	231	291	0.03%	0.004%
21	4.475	973	975	978	rVB2	282	141	0.02%	0.002%
22	4.497	978	982	988	rBV2	231	297	0.04%	0.005%
23	4.629	1012	1023	1068	rBV2	46328	171178	20.20%	2.637%
24	5.057	1139	1156	1184	rBV	141004	343114	40.48%	5.286%
25	5.208	1196	1203	1206	rBV3	925	1175	0.14%	0.018%
26	5.247	1213	1215	1218	rBV2	184	83	0.01%	0.001%
27	5.317	1235	1237	1240	rBV2	164	64	0.01%	0.001%
28	5.388	1255	1259	1260	rBV	179	140	0.02%	0.002%
29	5.562	1311	1313	1318	rVB2	169	151	0.02%	0.002%
30	5.604	1321	1326	1329	rBV2	217	233	0.03%	0.004%
31	5.713	1338	1360	1382	rBV2	318027	847567	100.00%	13.057%
32	5.909	1419	1421	1422	rBV	193	84	0.01%	0.001%
33	5.967	1434	1439	1440	rBV3	1280	896	0.11%	0.014%
34	6.018	1453	1455	1456	rBV3	197	66	0.01%	0.001%
35	6.079	1468	1474	1478	rBV2	231	303	0.04%	0.005%
36	6.118	1483	1486	1488	rBV2	195	145	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054065.D
 Acq On : 04 May 2023 16:27
 Operator : JC/MD
 Sample : 02574-10ME
 Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.166	1498	1501	1503	rBV	198	123	0.01%	0.002%
38	6.240	1509	1524	1548	rBV	272238	547197	64.56%	8.430%
39	6.430	1581	1583	1586	rBV	325	236	0.03%	0.004%
40	6.488	1598	1601	1604	rBV2	125	88	0.01%	0.001%
41	6.520	1604	1611	1621	rVV4	3320	6191	0.73%	0.095%
42	6.607	1626	1638	1645	rVV5	2451	5574	0.66%	0.086%
43	6.684	1648	1662	1691	rVB	191743	390798	46.11%	6.020%
44	6.845	1709	1712	1714	rBV2	166	131	0.02%	0.002%
45	6.880	1720	1723	1726	rVB	202	117	0.01%	0.002%
46	6.899	1726	1729	1732	rBV2	139	113	0.01%	0.002%
47	7.009	1757	1763	1768	rBV	196	323	0.04%	0.005%
48	7.047	1773	1775	1777	rBV2	176	67	0.01%	0.001%
49	7.198	1813	1822	1827	rBV7	1953	3514	0.41%	0.054%
50	7.256	1837	1840	1842	rVB	225	147	0.02%	0.002%
51	7.362	1871	1873	1877	rBV	171	123	0.01%	0.002%
52	7.423	1889	1892	1893	rBV	107	74	0.01%	0.001%
53	7.501	1914	1916	1919	rBV2	111	78	0.01%	0.001%
54	7.562	1922	1935	1953	rBV	98280	190262	22.45%	2.931%
55	7.661	1964	1966	1967	rBV	258	85	0.01%	0.001%
56	7.800	2007	2009	2012	rBV2	164	116	0.01%	0.002%
57	7.893	2025	2038	2063	rBV	371498	667668	78.77%	10.285%
58	8.057	2086	2089	2092	rBV2	202	154	0.02%	0.002%
59	8.079	2092	2096	2100	rBV3	306	324	0.04%	0.005%
60	8.176	2114	2126	2150	rBV	64473	131090	15.47%	2.019%
61	8.320	2170	2171	2172	rBV	198	67	0.01%	0.001%
62	8.465	2210	2216	2224	rVB3	414	736	0.09%	0.011%
63	8.546	2237	2241	2247	rVB5	1090	1084	0.13%	0.017%
64	8.658	2259	2276	2303	rBV2	160284	365113	43.08%	5.625%
65	8.825	2326	2328	2331	rBV	211	129	0.02%	0.002%
66	8.899	2349	2351	2354	rVB2	179	65	0.01%	0.001%
67	9.131	2418	2423	2426	rBV	184	159	0.02%	0.002%
68	9.169	2426	2435	2440	rBV2	335	585	0.07%	0.009%
69	9.308	2476	2478	2482	rVB2	216	130	0.02%	0.002%
70	9.333	2482	2486	2487	rBV	242	203	0.02%	0.003%
71	9.417	2498	2512	2538	rBV	340727	655452	77.33%	10.097%
72	9.661	2585	2588	2591	rBV2	234	211	0.02%	0.003%
73	9.690	2592	2597	2598	rBV2	1494	1123	0.13%	0.017%
74	9.809	2629	2634	2636	rBV2	233	238	0.03%	0.004%
75	9.861	2647	2650	2652	rBV	231	146	0.02%	0.002%
76	9.899	2659	2662	2664	rBV2	287	198	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054065.D
 Acq On : 04 May 2023 16:27
 Operator : JC/MD
 Sample : 02574-10ME
 Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCP5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	10.099	2720	2724	2727	rBV2	542	549	0.06%	0.008%
78	10.189	2746	2752	2754	rBV2	233	254	0.03%	0.004%
79	10.218	2758	2761	2762	rBV	176	104	0.01%	0.002%
80	10.436	2823	2829	2833	rBV2	293	397	0.05%	0.006%
81	10.484	2841	2844	2846	rBV2	333	178	0.02%	0.003%
82	10.520	2851	2855	2859	rBV	257	312	0.04%	0.005%
83	10.616	2882	2885	2891	rVB3	641	672	0.08%	0.010%
84	10.645	2891	2894	2895	rBV	517	355	0.04%	0.005%
85	10.693	2906	2909	2911	rBV	222	152	0.02%	0.002%
86	10.758	2917	2929	2946	rBV	261098	424782	50.12%	6.544%
87	11.111	3034	3039	3043	rBV4	874	995	0.12%	0.015%
88	11.237	3075	3078	3081	rBV2	192	130	0.02%	0.002%
89	11.308	3094	3100	3104	rBV3	685	704	0.08%	0.011%
90	11.362	3113	3117	3118	rBV	480	289	0.03%	0.004%
91	11.809	3240	3256	3280	rBV	405171	644810	76.08%	9.933%
92	12.192	3362	3375	3391	rBV	396460	634271	74.83%	9.771%
93	12.359	3424	3427	3430	rBV	214	130	0.02%	0.002%
94	12.780	3555	3558	3560	rBV2	225	120	0.01%	0.002%
95	12.796	3560	3563	3564	rBV	236	133	0.02%	0.002%
96	13.044	3637	3640	3642	rBV	228	135	0.02%	0.002%
97	13.118	3659	3663	3667	rBV2	355	424	0.05%	0.007%
98	13.349	3731	3735	3742	rBV2	405	406	0.05%	0.006%
99	13.407	3748	3753	3757	rBV2	374	424	0.05%	0.007%
100	14.253	4013	4016	4020	rBV2	377	376	0.04%	0.006%




Sum of corrected areas: 6491428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054065.D
Acq On : 04 May 2023 16:27
Operator : JC/MD
Sample : 02574-10ME
Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

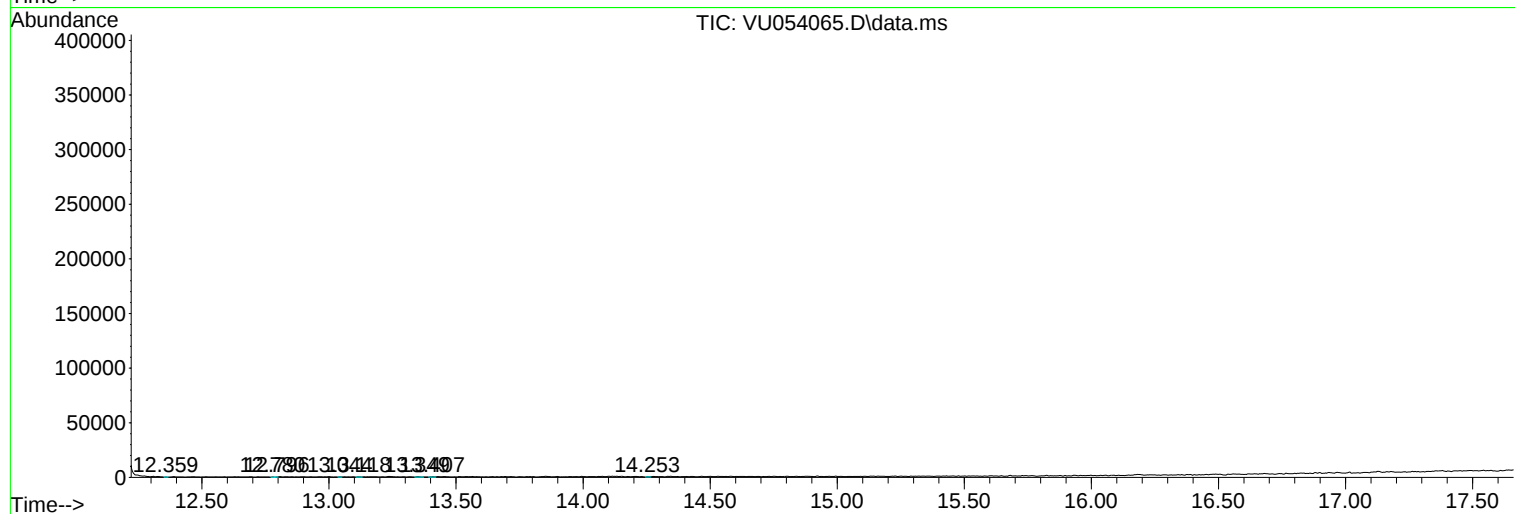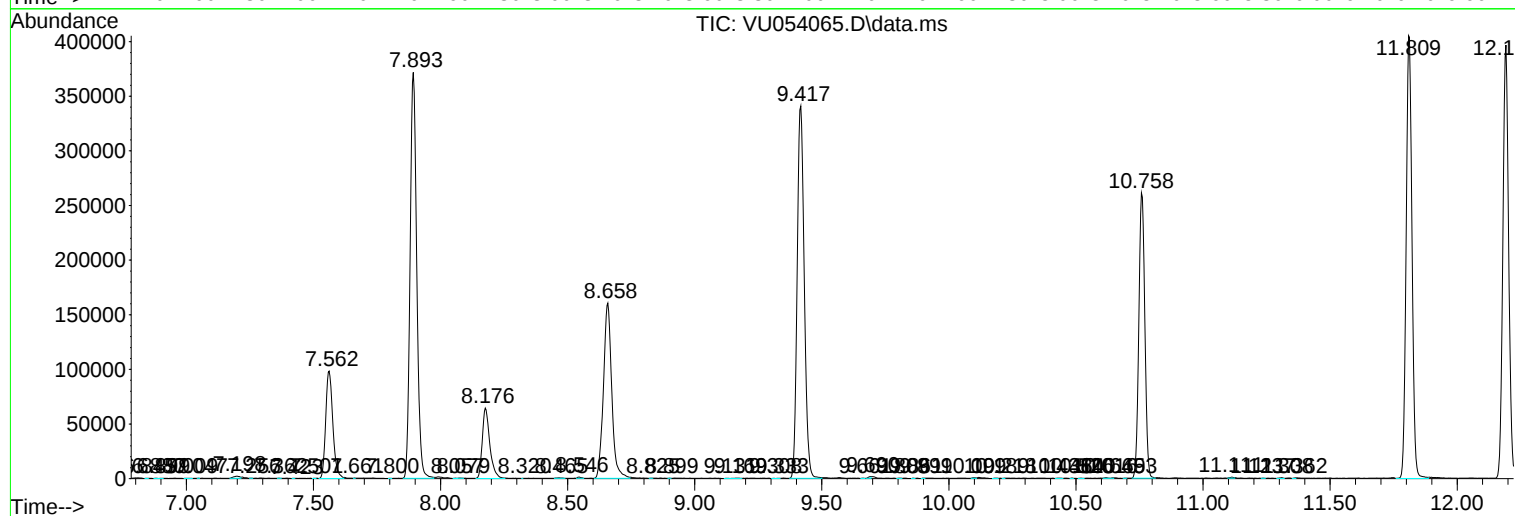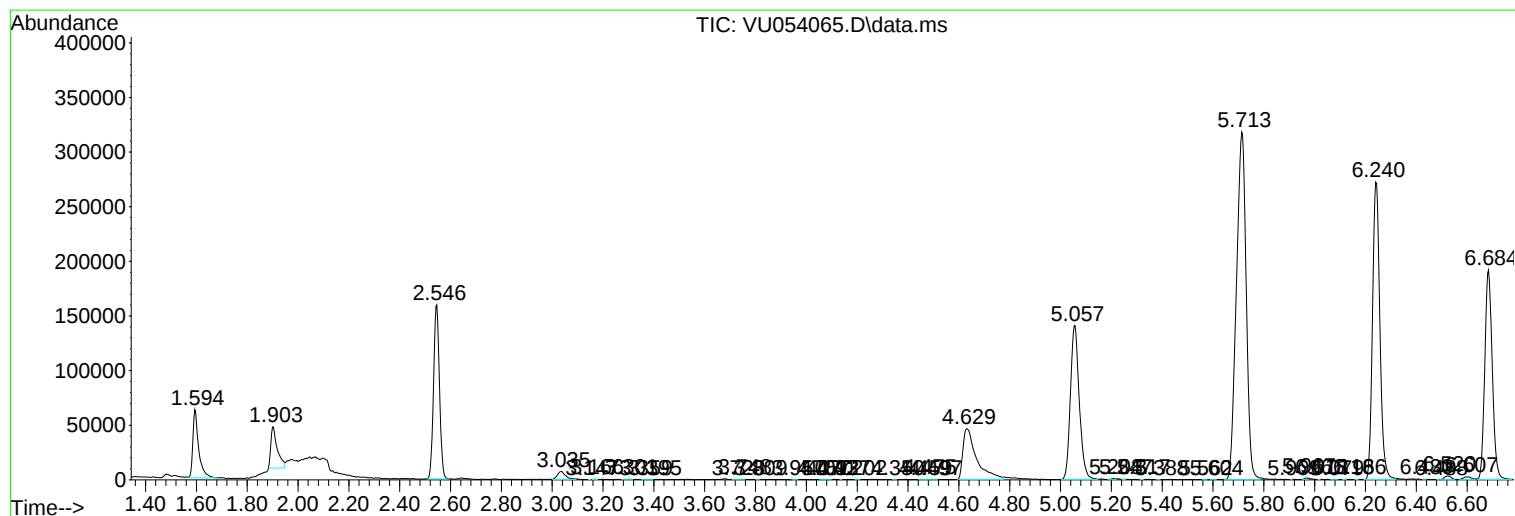

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054065.D
Acq On : 04 May 2023 16:27
Operator : JC/MD
Sample : 02574-10ME
Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
Data File : VU054065.D
Acq On : 04 May 2023 16:27
Operator : JC/MD
Sample : 02574-10ME
Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCP5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc