


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050423\
 Data File : VU054055.D
 Acq On : 04 May 2023 10:52
 Operator : JC/MD
 Sample : BFB185
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB185

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis
 Last Update : Fri May 05 04:34:01 2023

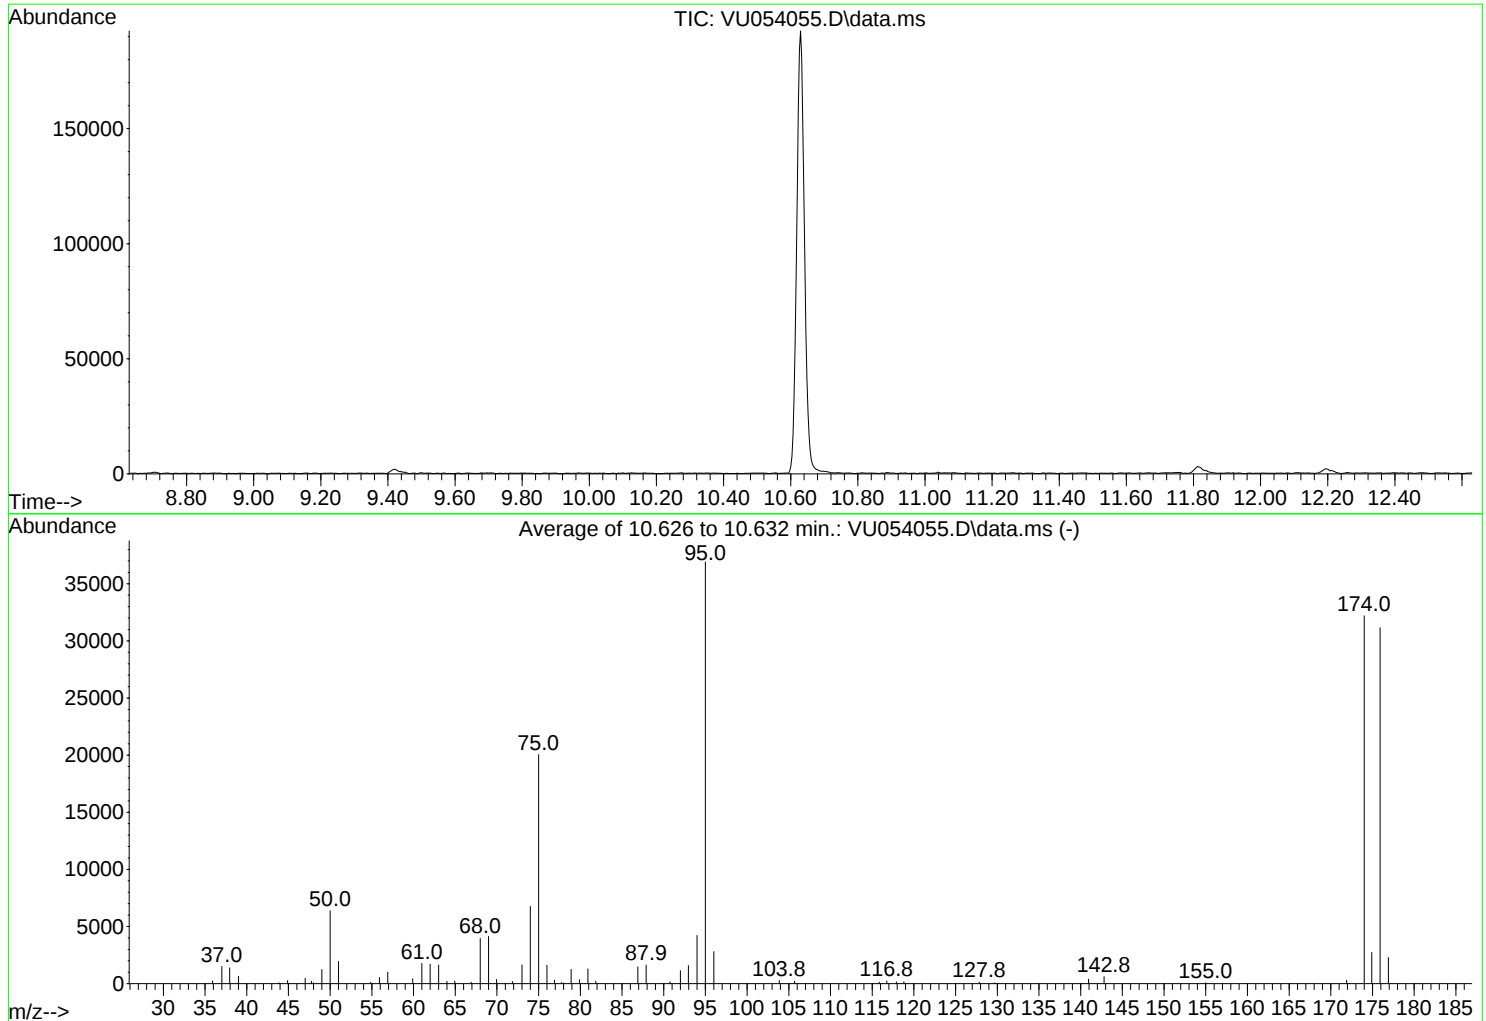

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	6373	PASS
75	95	30	80	54.3	20043	PASS
95	95	100	100	100.0	36920	PASS
96	95	5	9	7.6	2796	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.2	32197	PASS
175	174	5	9	8.5	2733	PASS
176	174	95	101	96.7	31149	PASS
177	176	5	9	7.3	2283	PASS

m/z	Abundance
39.90	173.0
43.80	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
35.90	236.0
37.00	1697.0
37.90	1487.0
39.00	670.0
39.80	126.0
43.90	272.0
44.90	272.0
47.00	498.0
47.80	205.0
48.00	206.0
49.00	1256.0
50.00	6379.0
51.00	1845.0
55.00	129.0
55.90	529.0
56.90	950.0
59.90	425.0
61.00	1813.0
62.00	1777.0
63.00	1655.0
64.00	211.0
65.00	219.0
66.90	140.0
68.00	3959.0
69.00	4096.0
69.90	352.0
71.80	186.0
73.00	1619.0
74.00	6665.0
75.00	20064.0
76.00	1707.0
76.90	281.0
77.70	201.0
78.90	1274.0
79.90	347.0
80.90	1252.0
81.80	259.0
86.90	1498.0
87.90	1621.0
90.80	135.0
92.00	1180.0
92.90	1458.0
94.00	4209.0
95.00	37080.0
96.00	2813.0
103.90	234.0
105.70	241.0
115.90	140.0
116.70	271.0
117.90	143.0
118.80	154.0
127.90	128.0
129.70	113.0
141.00	347.0
142.80	602.0
171.90	314.0
174.00	31416.0
174.90	2698.0
175.90	29816.0
176.90	2353.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
35.90	254.0
37.00	1516.0
38.00	1420.0
39.00	678.0
39.90	150.0
44.00	269.0
44.90	274.0
47.00	488.0
47.80	213.0
49.00	1253.0
50.00	6630.0
51.00	2058.0
54.80	118.0
55.90	545.0
56.90	1047.0
59.90	463.0
61.00	1846.0
62.00	1761.0
63.00	1723.0
64.00	199.0
65.00	235.0
66.90	129.0
68.00	4121.0
69.00	4289.0
70.00	377.0
71.90	197.0
73.00	1691.0
74.00	7018.0
75.00	20696.0
76.00	1602.0
76.90	316.0
77.80	138.0
78.00	134.0
78.90	1275.0
79.90	343.0
80.90	1330.0
81.90	233.0
86.90	1538.0
87.90	1709.0
90.80	179.0
92.00	1184.0
93.00	1626.0
94.00	4348.0
95.00	38040.0
96.00	2959.0
103.80	273.0
105.70	243.0
115.90	119.0
116.80	239.0
117.90	177.0
118.80	172.0
127.90	124.0
129.70	108.0
141.00	404.0
142.80	626.0
155.00	110.0
171.90	314.0
174.00	33288.0
174.90	2886.0
175.90	32296.0
176.90	2412.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
35.90	245.0
37.00	1327.0
38.00	1252.0
39.00	581.0
40.00	173.0
44.00	275.0
44.90	266.0
47.00	435.0
47.70	208.0
49.00	1191.0
50.00	6110.0
51.00	1931.0
54.80	121.0
55.90	508.0
56.90	1011.0
59.90	428.0
61.00	1644.0
62.00	1614.0
63.00	1522.0
64.00	162.0
64.90	222.0
66.90	114.0
68.00	3814.0
69.00	4005.0
70.00	369.0
71.90	199.0
73.00	1593.0
74.00	6557.0
75.00	19368.0
76.00	1511.0
76.90	337.0
78.90	1187.0
79.90	313.0
80.90	1295.0
81.90	201.0
86.90	1370.0
87.90	1536.0
90.70	154.0
92.00	1043.0
93.00	1681.0
94.00	4106.0
95.00	35640.0
96.00	2615.0
103.80	281.0
105.70	208.0
115.80	100.0
116.80	218.0
117.90	159.0
118.80	194.0
127.70	112.0
140.90	429.0
142.80	625.0
155.00	100.0
171.90	275.0
174.00	31888.0
174.90	2614.0
175.90	31336.0
176.90	2084.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185