

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU050518\
 Data File : VU023664.D
 Acq On : 05 May 2018 13:17
 Operator : MD/SY
 Sample : J2630-05DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 06 01:02:31 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMUTR050418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun May 06 01:00:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	143359	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	144072	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	63734	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	45539	4.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.60%
7) Chloroethane-d5	1.68	69	37624	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.27	63	64709	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	4.20	46	133996	44.54	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.08%
24) Chloroform-d	4.65	84	91021	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.31	65	48809	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
32) Benzene-d6	5.34	84	179037	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
36) 1,2-Dichloropropane-d6	6.34	67	61360	4.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.40%
41) Toluene-d8	7.57	98	146781	4.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.60%
43) trans-1,3-Dichloropropene-	7.86	79	19064	4.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.20%
46) 2-Hexanone-d5	8.32	63	101772	42.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.66%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	45224	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.20%
64) 1,2-Dichlorobenzene-d4	11.87	152	60003	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds


						Qvalue
5) Vinyl chloride	1.40	62	8410	0.63	ug/L	# 1
13) Acetone	2.33	43	2034	1.18	ug/L	81
18) trans-1,2-Dichloroethene	2.98	96	4206	0.45	ug/L	93
22) cis-1,2-Dichloroethene	4.23	96	83096	7.50	ug/L	99
34) Trichloroethene	6.19	95	16999	1.50	ug/L	99
37) 1,2-Dichloropropane	6.34	63	6376	0.53	ug/L	# 89
47) Tetrachloroethene	8.23	164	27368	3.06	ug/L	97
49) Dibromochloromethane	8.23	129	26035	3.00	ug/L	# 9
59) 1,2,3-Trichloropropane	11.49	75	7401	1.04	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_U\DATA\VU050518\
Data File : VU023664.D
Acq On : 05 May 2018 13:17
Operator : MD/SY
Sample : J2630-05DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 06 01:02:31 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMUTR050418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun May 06 01:00:29 2018
Response via : Initial Calibration

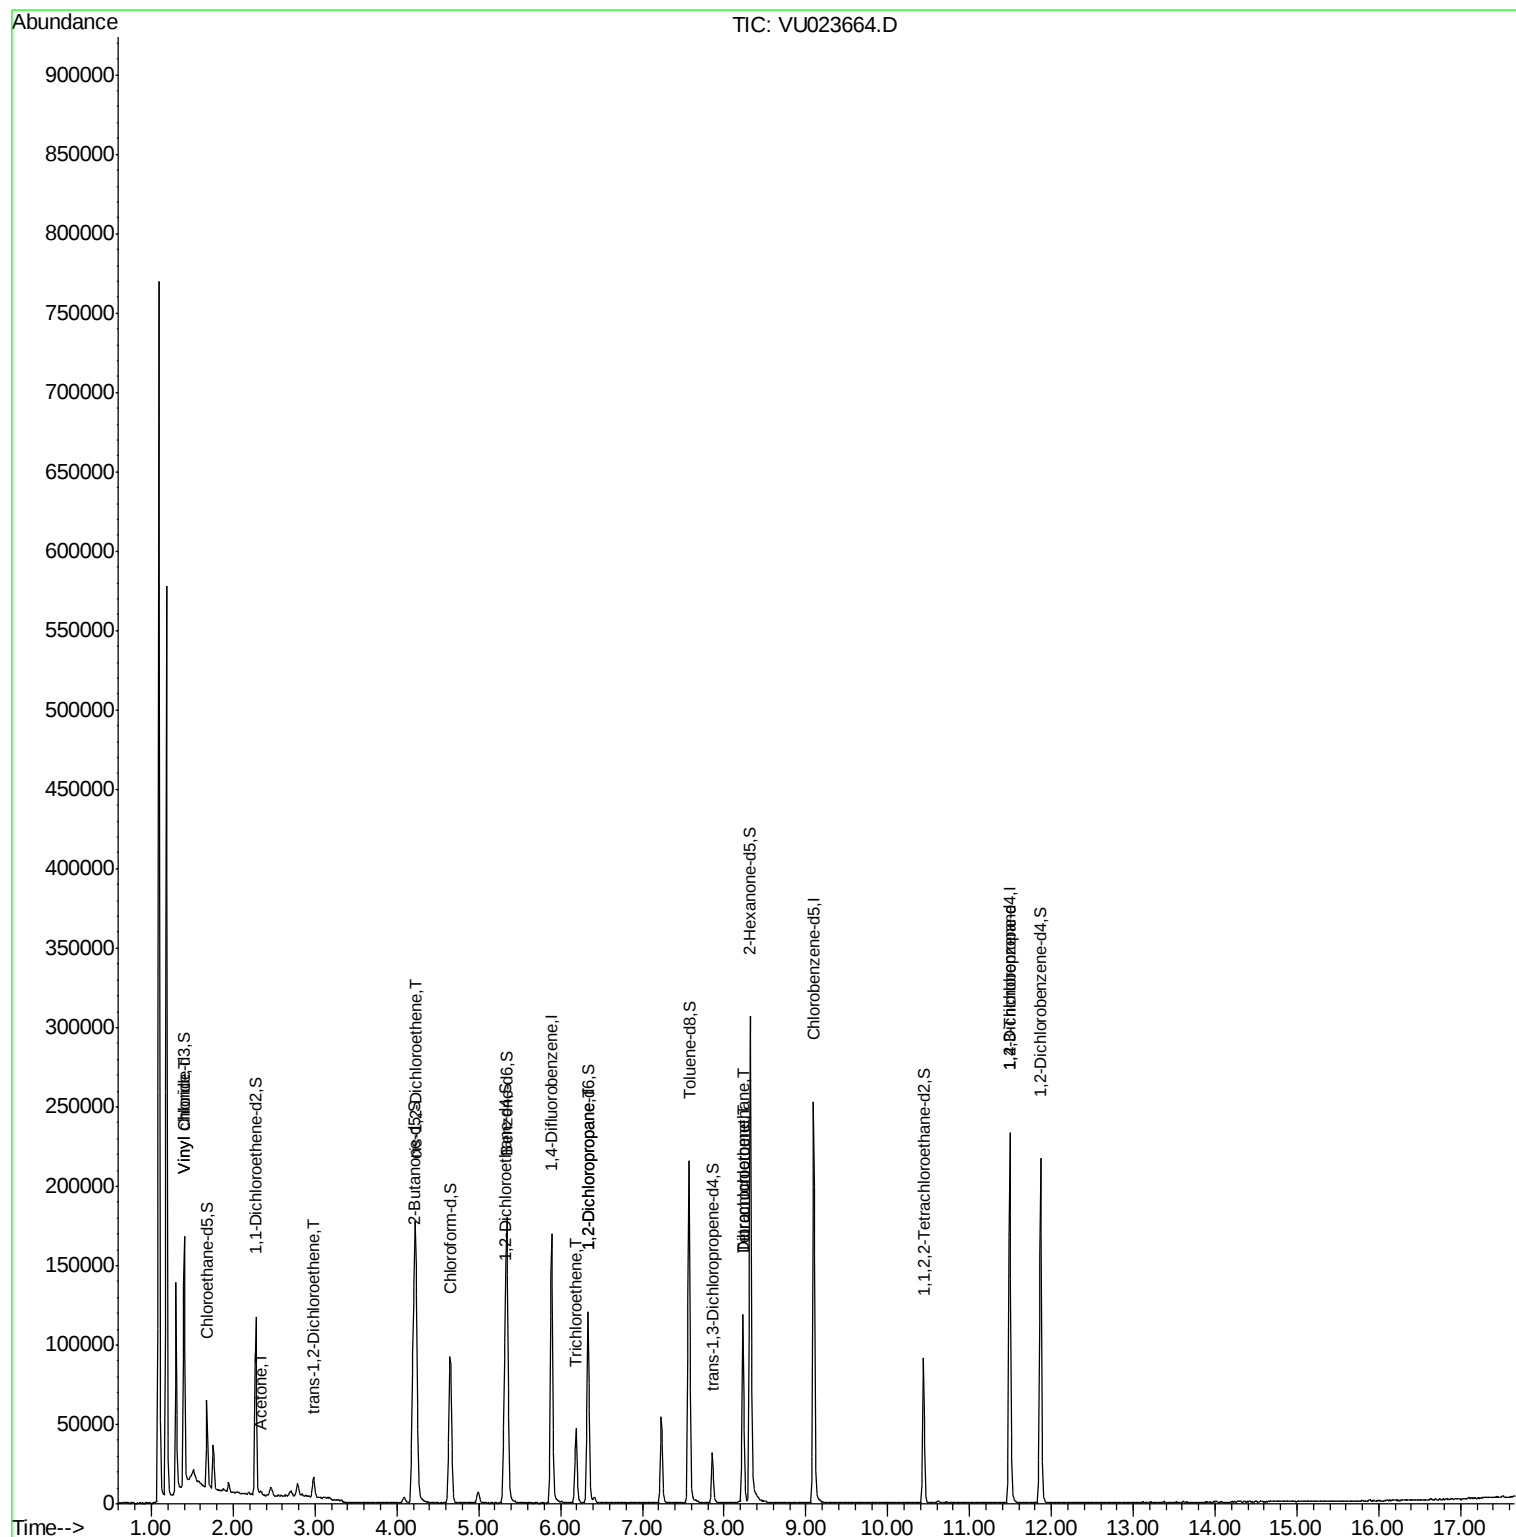

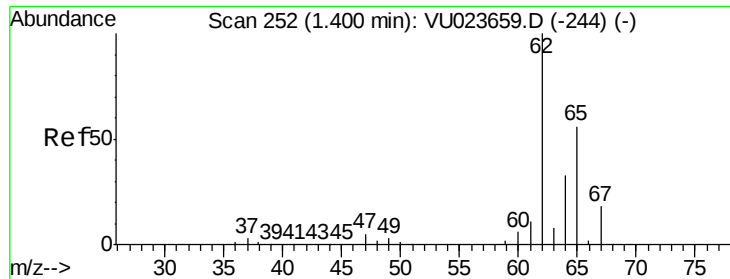

#5

Vinyl chloride

Concen: 0.63 ug/L

RT: 1.40 min Scan# 252

Delta R.T. -0.00 min

Lab File: VU023664.D





Acq: 05 May 2018 13:17

Tgt Ion: 62 Resp: 8410

Ion Ratio Lower Upper

62 100

64 105.9 26.9 49.9#

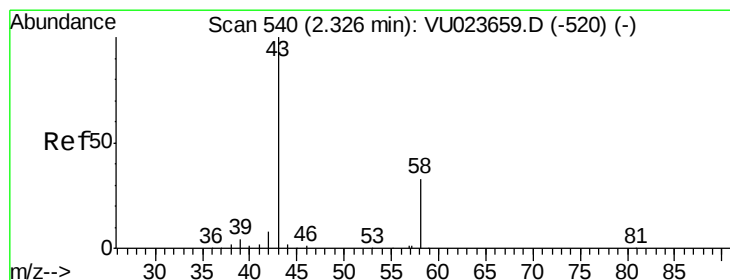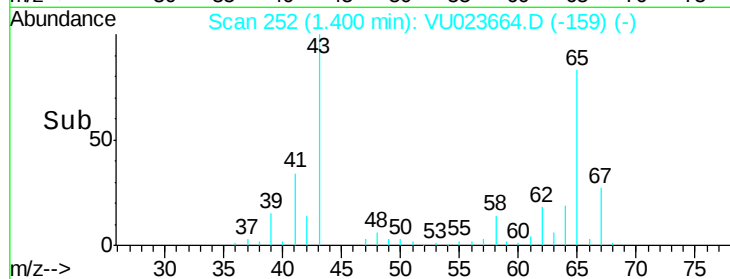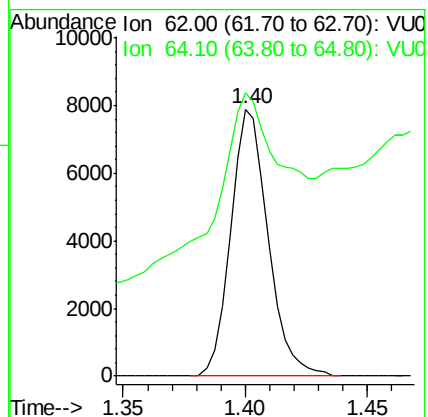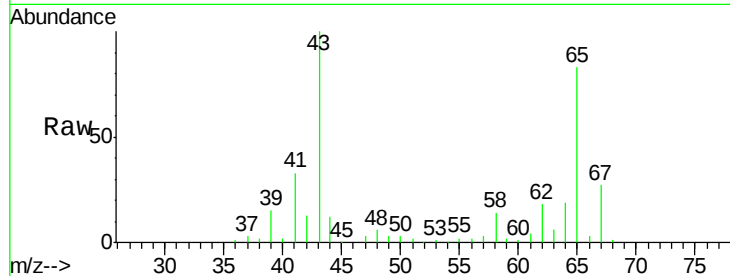

#13

Acetone

Concen: 1.18 ug/L

RT: 2.33 min Scan# 541

Delta R.T. 0.00 min

Lab File: VU023664.D




Acq: 05 May 2018 13:17


Tgt Ion: 43 Resp: 2034

Ion Ratio Lower Upper

43 100


58 21.3 0.0 63.8

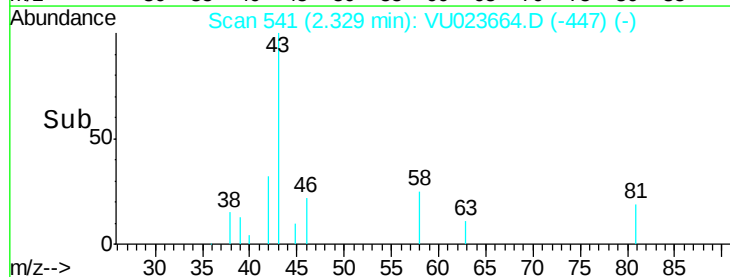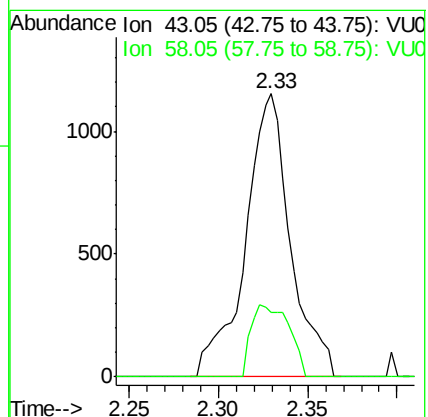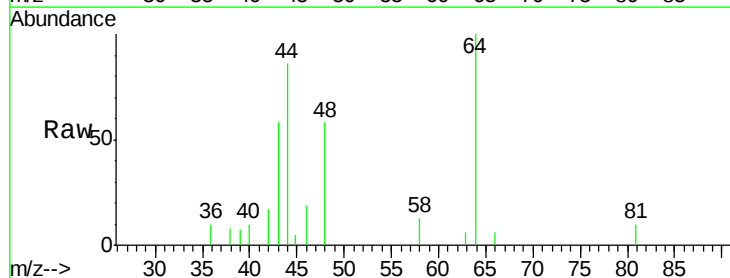



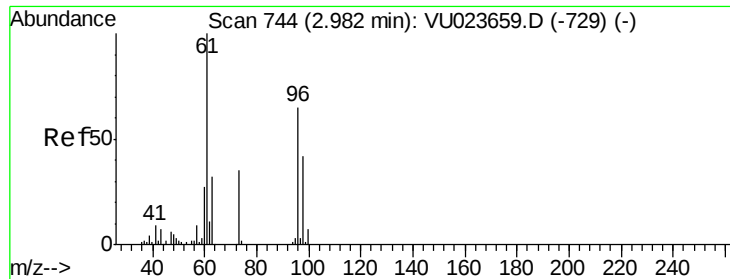


#18
trans-1,2-Dichloroethene
Concen: 0.45 ug/L
RT: 2.98 min Scan# 743
Delta R.T. -0.00 min
Lab File: VU023664.D
Acq: 05 May 2018 13:17

Tgt Ion: 96 Resp: 4206
Ion Ratio Lower Upper
96 100
61 163.5 109.0 202.4
98 70.7 44.7 83.1

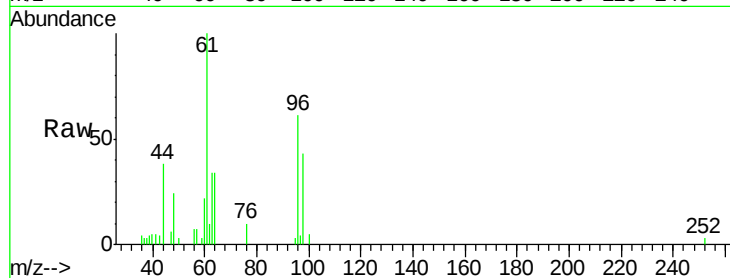


Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.05 (60.75 to 61.75): VU0
Ion 97.95 (97.65 to 98.65): VU0

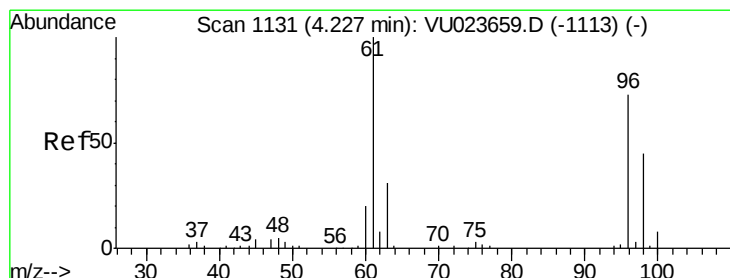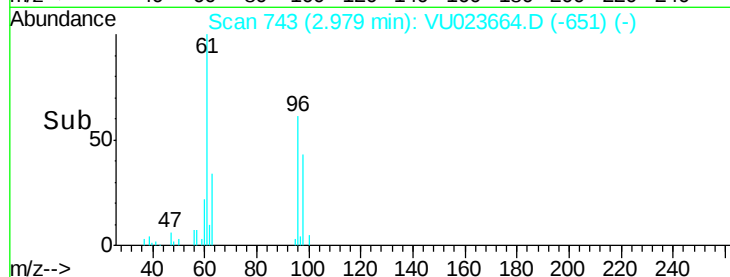
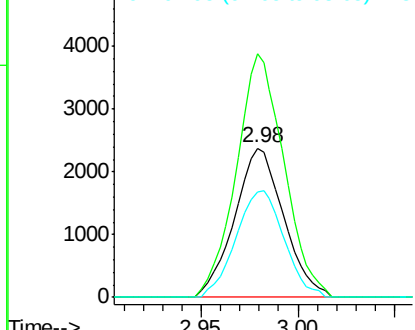



#22
cis-1,2-Dichloroethene
Concen: 7.50 ug/L
RT: 4.23 min Scan# 1132
Delta R.T. 0.00 min
Lab File: VU023664.D
Acq: 05 May 2018 13:17

Tgt Ion: 96 Resp: 83096
Ion Ratio Lower Upper
96 100
61 136.7 94.6 175.6
68 0.0 0.0 0.0

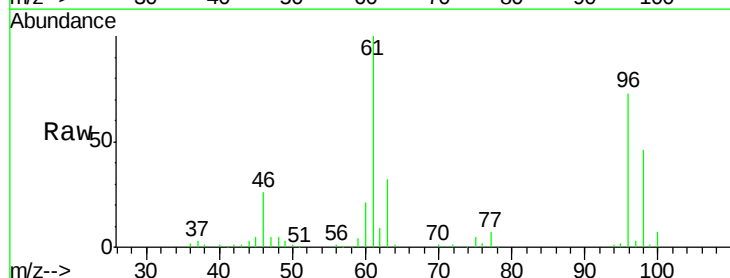


Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.05 (60.75 to 61.75): VU0
Ion 68.15 (67.85 to 68.85): VU0

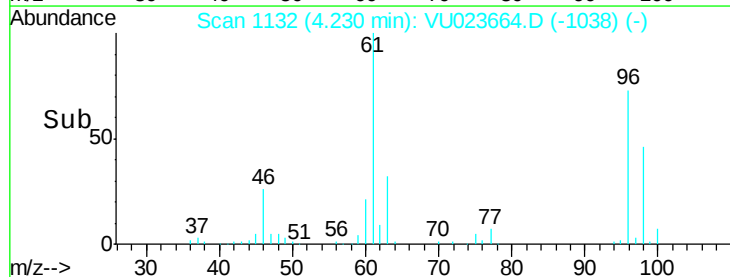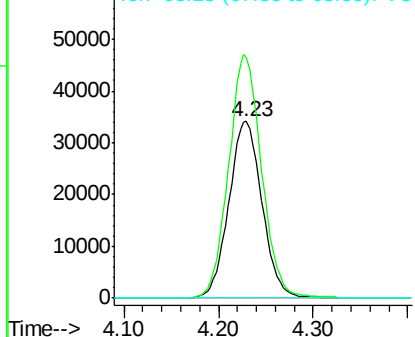

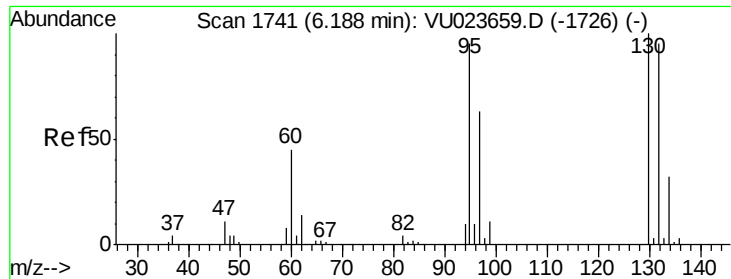

#34
 Trichloroethene
 Concen: 1.50 ug/L
 RT: 6.19 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: VU023664.D
 Acq: 05 May 2018 13:17

Tgt Ion:	95	Resp:	16999
Ion	Ratio	Lower	Upper
95	100		
97	65.1	46.0	85.4
132	96.6	68.1	126.5
130	98.3	70.1	130.1



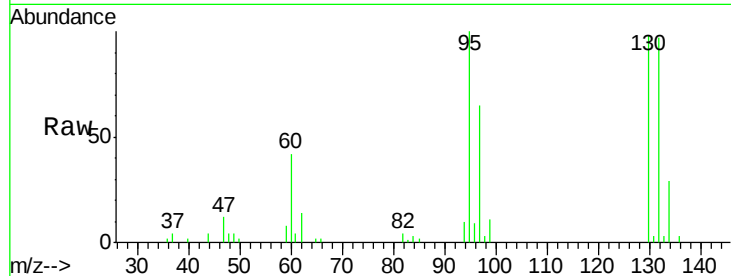


Abundance Ion 95.00 (94.70 to 95.70): VU023664.D (-1648) (-)

Ion 96.95 (96.65 to 97.65): VU023664.D (-1648) (-)


Ion 131.95 (131.65 to 132.65): VU023664.D (-1648) (-)

Ion 129.95 (129.65 to 130.65): VU023664.D (-1648) (-)

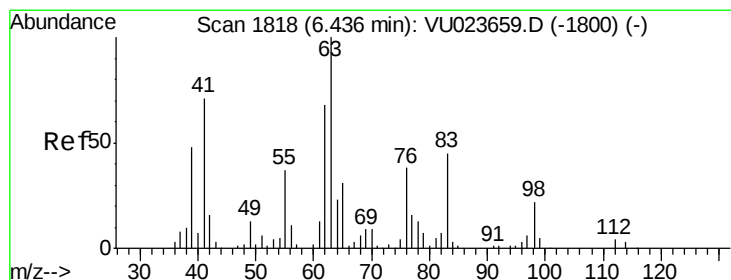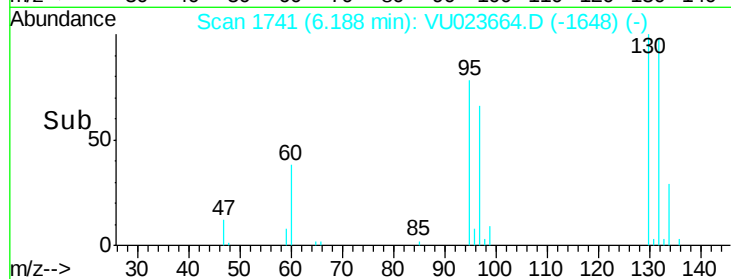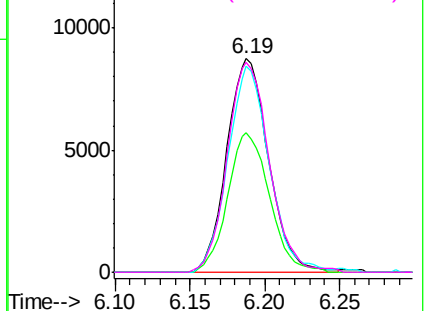



#37
 1,2-Dichloropropane
 Concen: 0.53 ug/L
 RT: 6.34 min Scan# 1787
 Delta R.T. -0.10 min
 Lab File: VU023664.D
 Acq: 05 May 2018 13:17


Tgt Ion:	63	Resp:	6376
Ion	Ratio	Lower	Upper
63	100		
112	0.0	3.0	4.4#

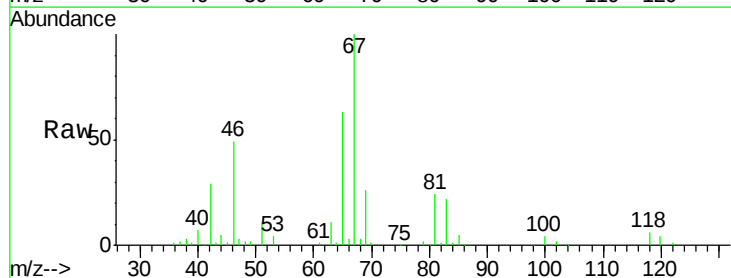

Abundance Ion 63.10 (62.80 to 63.80): VU023664.D (-1725) (-)

Ion 112.10 (111.80 to 112.80): VU023664.D (-1725) (-)

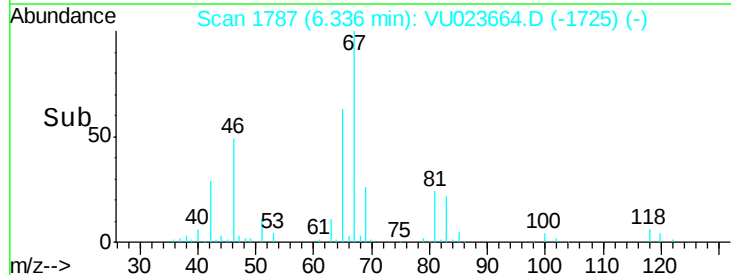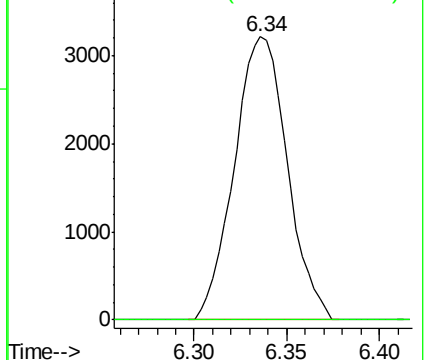

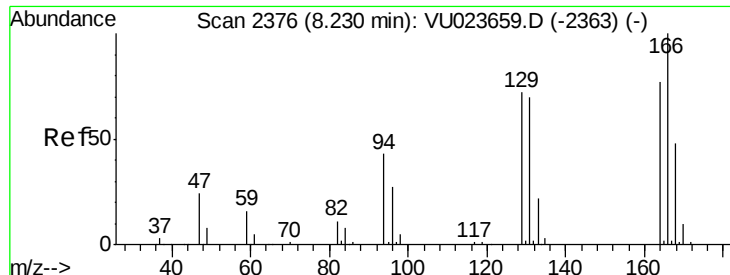

#47

Tetrachloroethene

Concen: 3.06 ug/L

RT: 8.23 min Scan# 2376

Delta R.T. -0.00 min

Lab File: VU023664.D

Acq: 05 May 2018 13:17

Tgt Ion:164 Resp: 27368


Ion Ratio Lower Upper

164 100

129 97.4 64.4 119.6

131 92.4 63.9 118.7

166 131.6 90.0 167.2



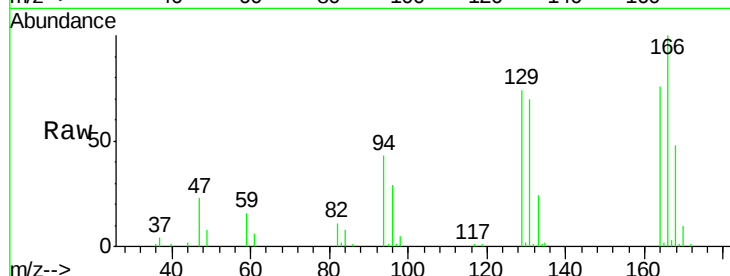


Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

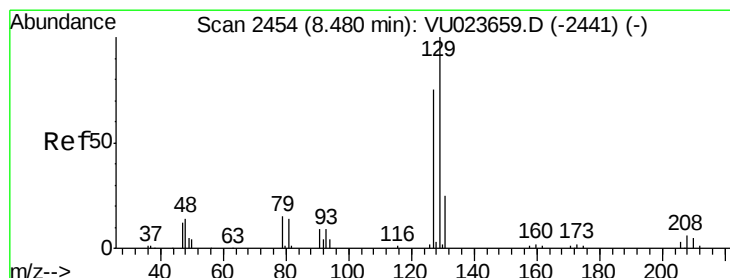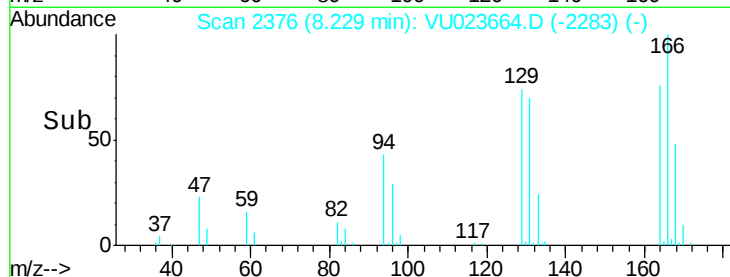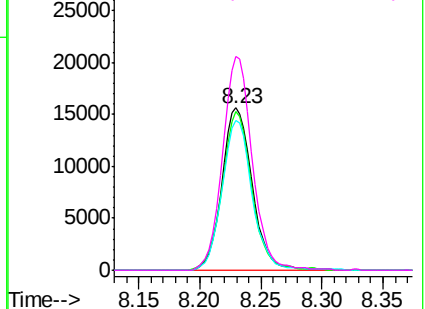

#49

Dibromochloromethane

Concen: 3.00 ug/L

RT: 8.23 min Scan# 2376

Delta R.T. -0.25 min

Lab File: VU023664.D


Acq: 05 May 2018 13:17

Tgt Ion:129 Resp: 26035

Ion Ratio Lower Upper



129 100


127 0.0 56.9 105.7#

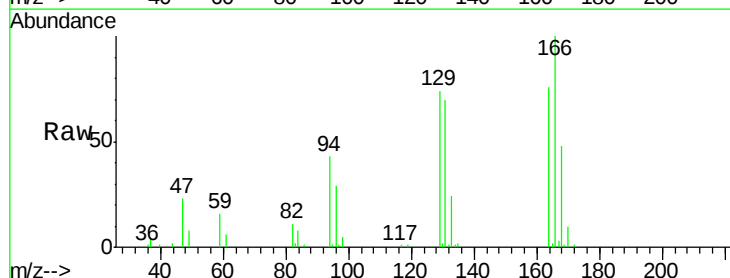

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

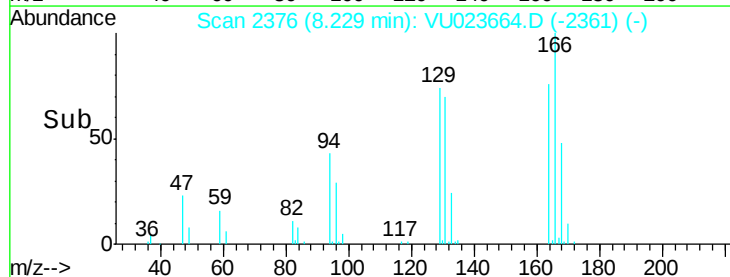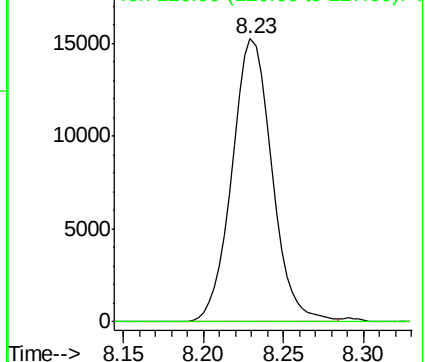

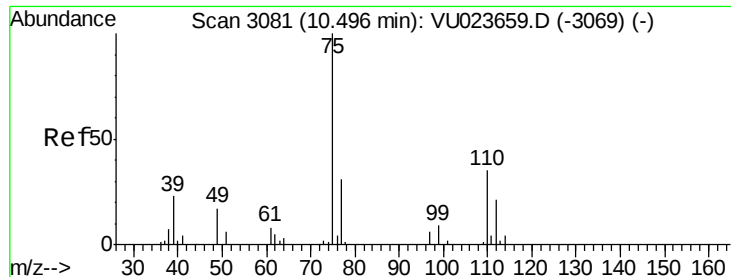

#59

1,2,3-Trichloropropane

Concen: 1.04 ug/L

RT: 11.49 min Scan# 3390

Delta R.T. 0.99 min

Lab File: VU023664.D

Acq: 05 May 2018 13:17

Tgt Ion: 75 Resp: 7401

Ion Ratio Lower Upper

75 100

77 36.2 26.0 39.0

