

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050518\
 Data File : VU023672.D
 Acq On : 05 May 2018 17:34
 Operator : MD/SY
 Sample : J2636-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: May 06 01:27:58 2018
 Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun May 06 01:00:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	138647	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	142100	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	64016	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	44085	4.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.60%
7) Chloroethane-d5	1.68	69	38015	5.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.80%
11) 1,1-Dichloroethene-d2	2.27	63	63607	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	4.20	46	152754	52.50	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.00%
24) Chloroform-d	4.65	84	91867	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
26) 1,2-Dichloroethane-d4	5.31	65	51146	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.80%
32) Benzene-d6	5.34	84	175939	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.34	67	61786	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.57	98	146643	4.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.80%
43) trans-1,3-Dichloropropene-	7.86	79	19455	4.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.00%
46) 2-Hexanone-d5	8.32	63	117456	50.11	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.22%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	48884	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	63832	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%


Target Compounds					Ovalue
13) Acetone	2.33	43	10207	6.14 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050518\
Data File : VU023672.D
Acq On : 05 May 2018 17:34
Operator : MD/SY
Sample : J2636-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: May 06 01:27:58 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun May 06 01:00:29 2018
Response via : Initial Calibration

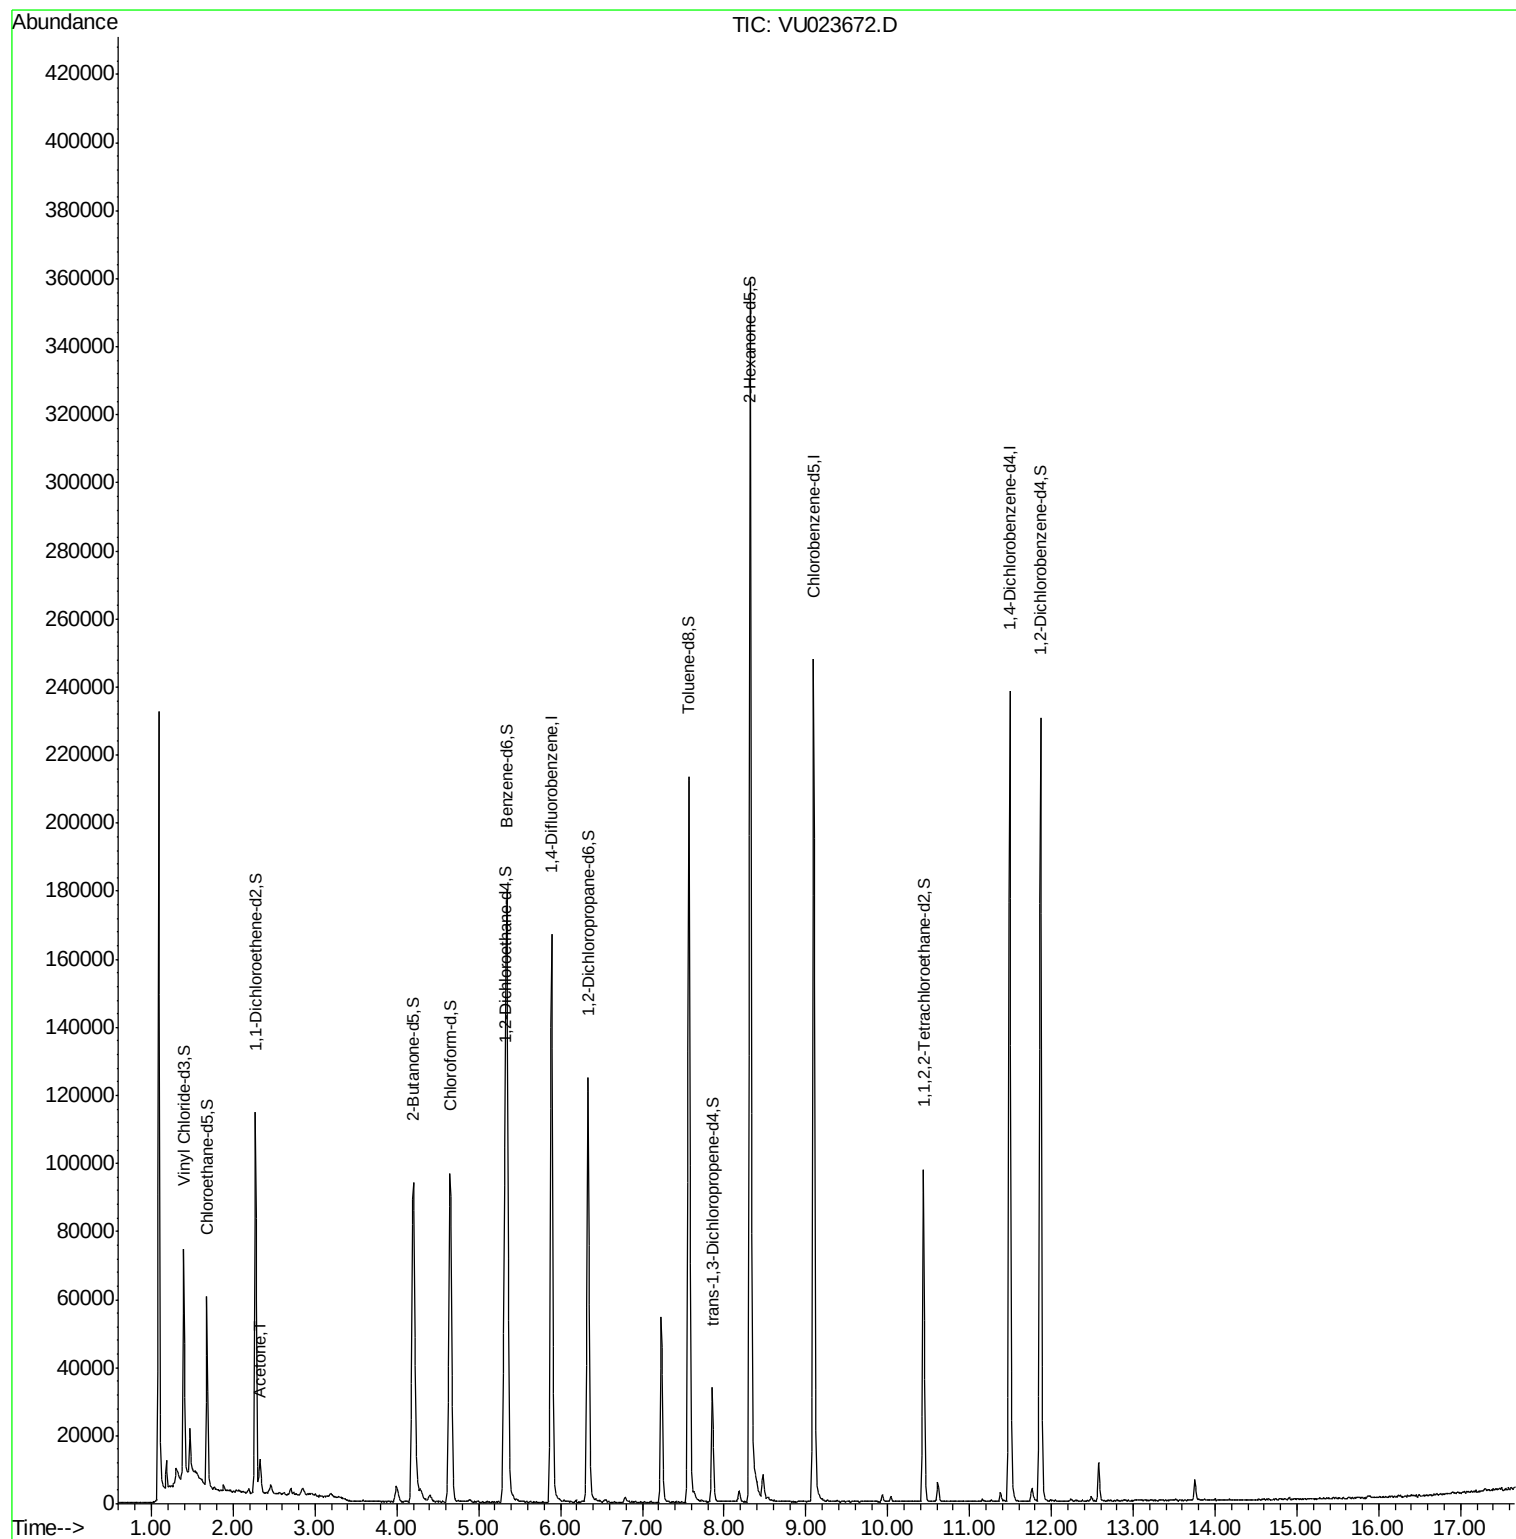

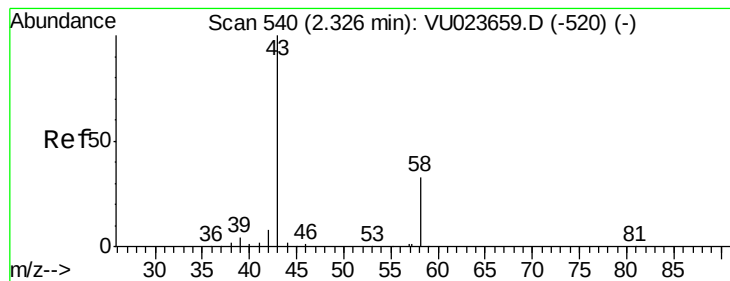

#13
 Acetone
 Concen: 6.14 ug/L
 RT: 2.33 min Scan# 540
 Delta R.T. 0.00 min
 Lab File: VU023672.D
 Acq: 05 May 2018 17:34

Tot Ion	Ratio	Lower	Upper
43	100		
58	29.5	0.0	63.8

