

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050518\
 Data File : VU023678.D
 Acq On : 05 May 2018 20:08
 Operator : MD/SY
 Sample : J2640-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 06 01:34:23 2018
 Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun May 06 01:00:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	143564	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	146884	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	65574	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	43041	4.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.60%
7) Chloroethane-d5	1.68	69	37285	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.40%
11) 1,1-Dichloroethene-d2	2.27	63	61735	3.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.40%
20) 2-Butanone-d5	4.20	46	153242	50.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.74%
24) Chloroform-d	4.65	84	89110	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.32	65	51058	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.00%
32) Benzene-d6	5.34	84	174606	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
36) 1,2-Dichloropropane-d6	6.34	67	61892	4.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.40%
41) Toluene-d8	7.57	98	145532	4.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.40%
43) trans-1,3-Dichloropropene-	7.86	79	18191	3.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.80%
46) 2-Hexanone-d5	8.32	63	116510	48.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.18%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	49358	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	11.87	152	62046	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	4004	2.33 ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050518\
Data File : VU023678.D
Acq On : 05 May 2018 20:08
Operator : MD/SY
Sample : J2640-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 06 01:34:23 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\SOMUTR050418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun May 06 01:00:29 2018
Response via : Initial Calibration

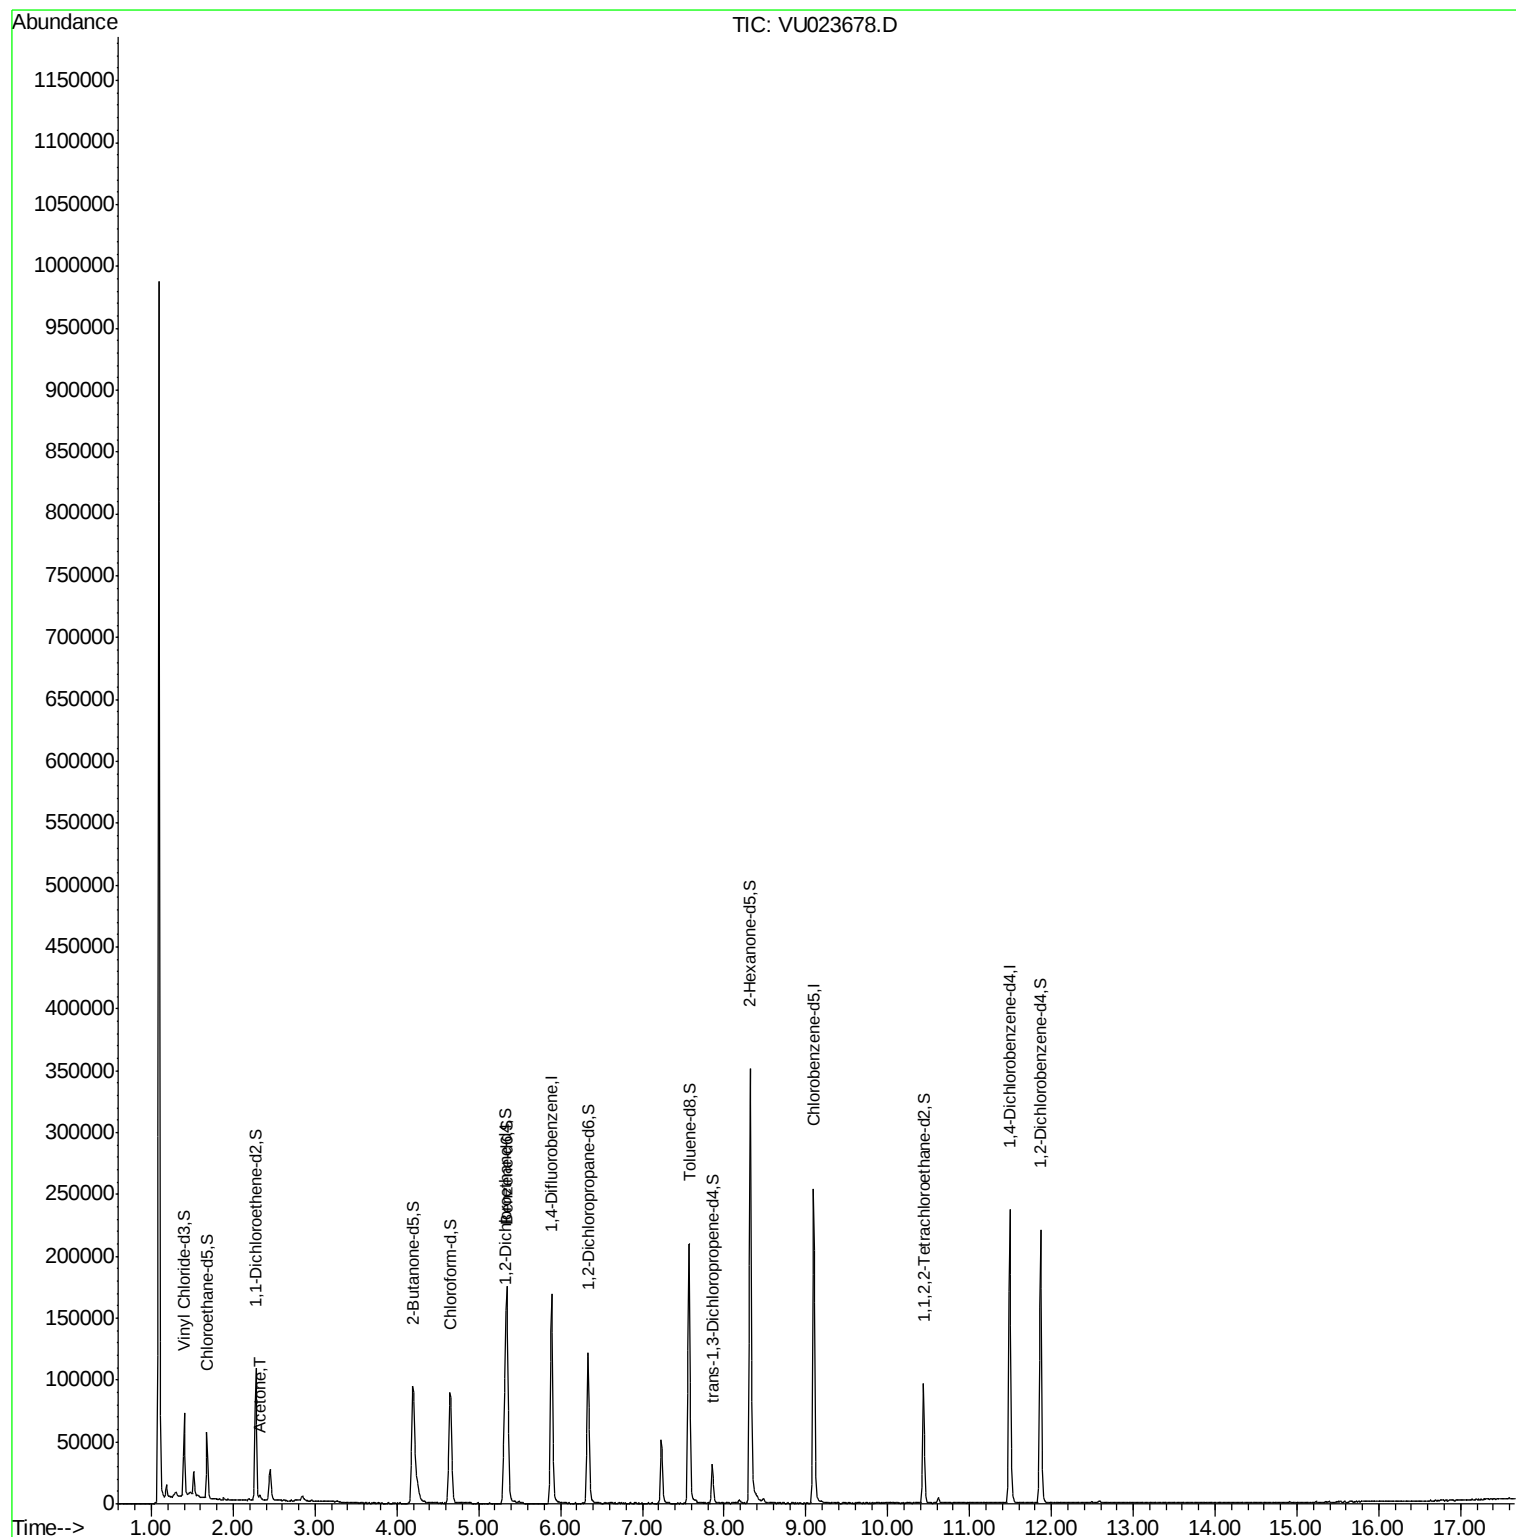

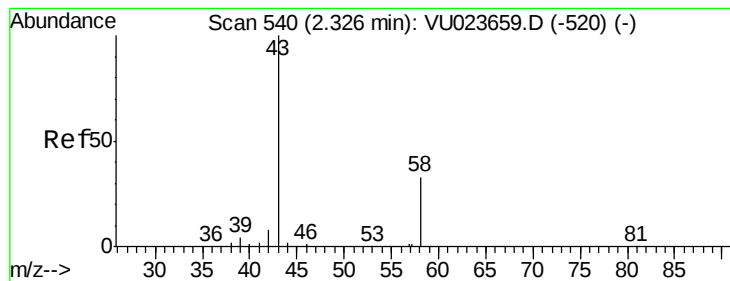

#13

Acetone

Concen: 2.33 ug/L

RT: 2.32 min Scan# 539

Delta R.T. -0.00 min

Lab File: VU023678.D

Acq: 05 May 2018 20:08

Tot Ion: 43 Resp: 4004

Ion Ratio Lower Upper

43 100

58 28.0 0.0 63.8

