

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050520\
Data File : VU038010.D
Acq On : 05 May 2020 11:26
Operator : JC/MD
Sample : VU0505WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0505WBL01

Quant Time: May 06 01:06:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U050420DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue May 05 02:20:02 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	6.15	96	85220	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.65	95	30353	0.92	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.00%	
68) 1,2-Dichlorobenzene-d4	12.20	152	29047	0.91	ug/l	0.00
Spiked Amount 1.000			Recovery	=	91.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050520\
Data File : VU038010.D
Acq On : 05 May 2020 11:26
Operator : JC/MD
Sample : VU0505WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0505WBL01

Quant Time: May 06 01:06:02 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U050420DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue May 05 02:20:02 2020
Response via : Initial Calibration

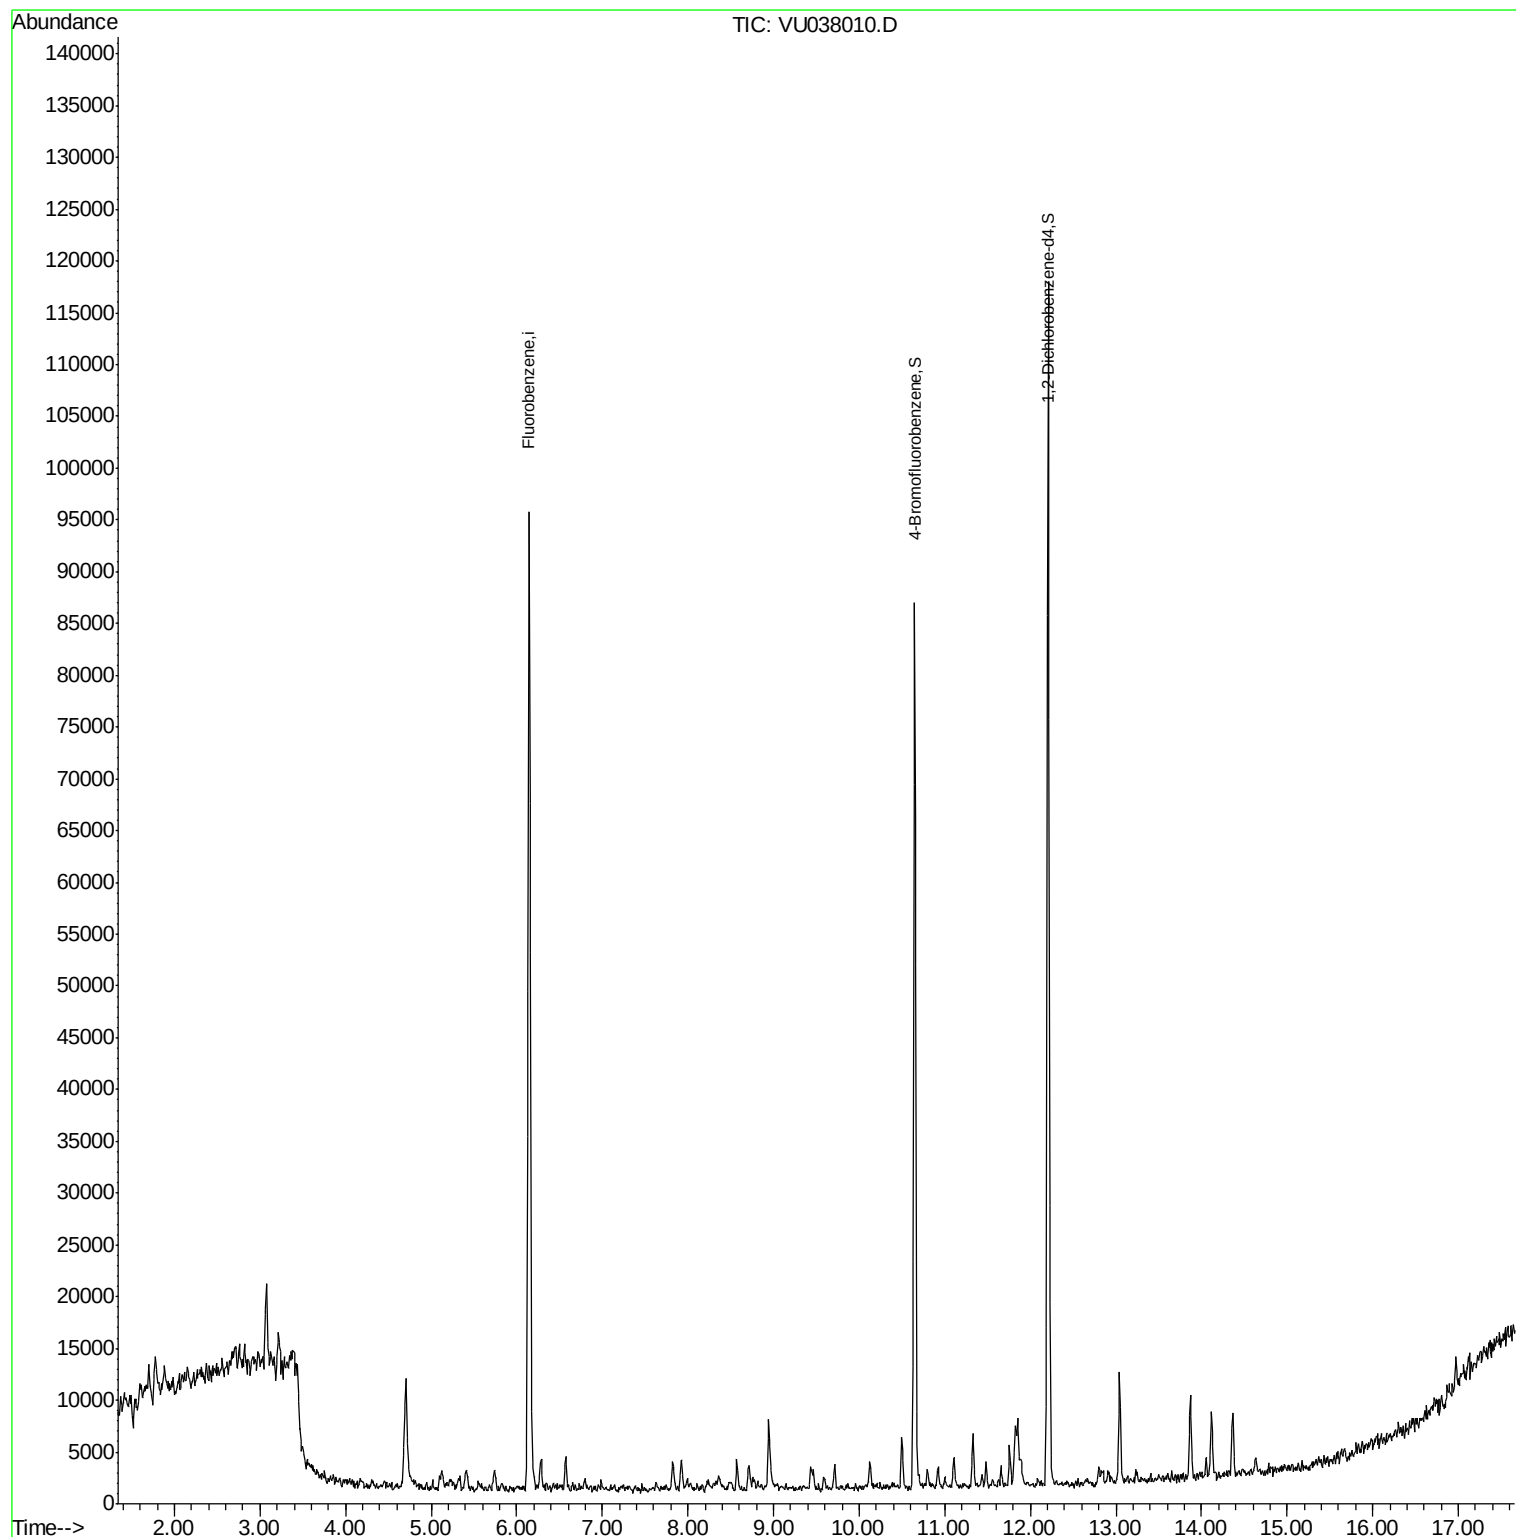

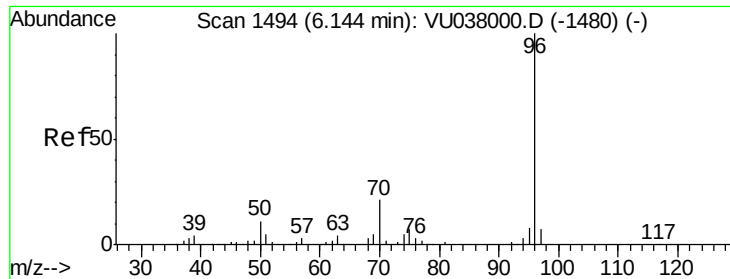

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.15 min Scan# 1495

Delta R.T. 0.00 min

Lab File: VU038010.D

Acq: 05 May 2020 11:26

Instrument :

MSVOA_U

ClientSampleId :

VU0505WBL01

Tot Ion: 96 Resp: 85220





Ion Ratio Lower Upper

96 100

70 21.1 14.4 21.6

95 9.5 7.1 10.7

97 6.3 0.0 0.0#

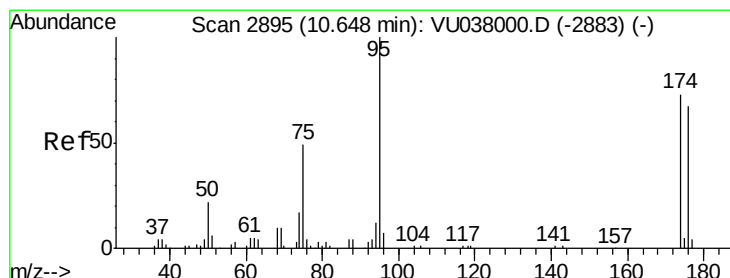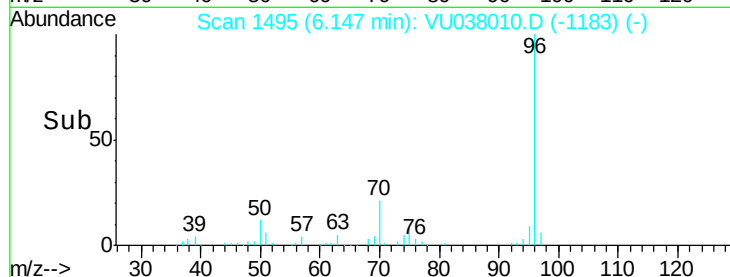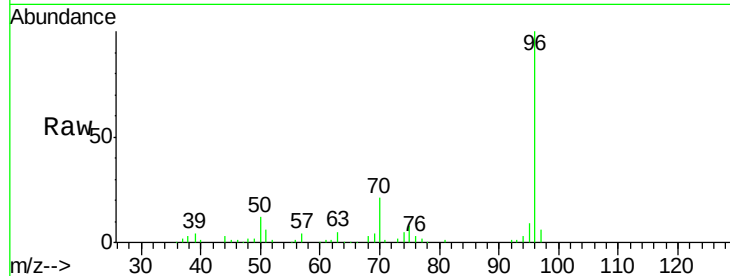

#57

4-Bromofluorobenzene

Concen: 0.918 ug/l

RT: 10.65 min Scan# 2895

Delta R.T. 0.00 min

Lab File: VU038010.D

Acq: 05 May 2020 11:26



Tgt Ion: 95 Resp: 30353


Ion Ratio Lower Upper

95 100

174 73.4 61.2 91.8

176 69.7 57.1 85.7

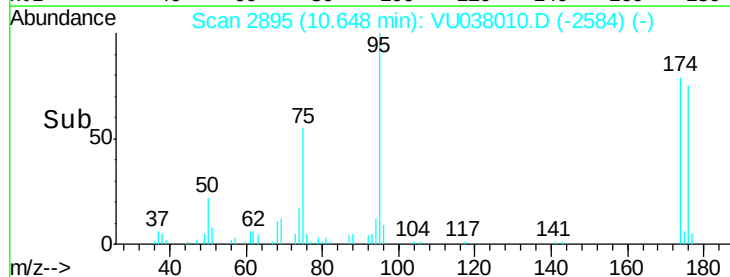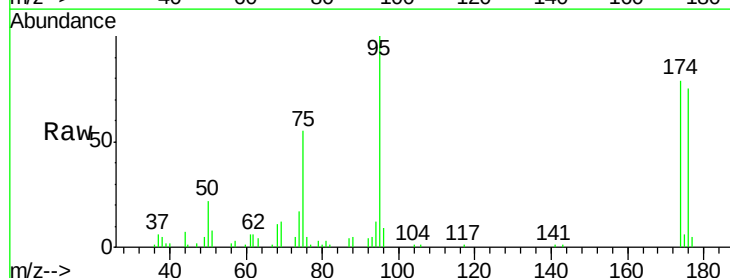


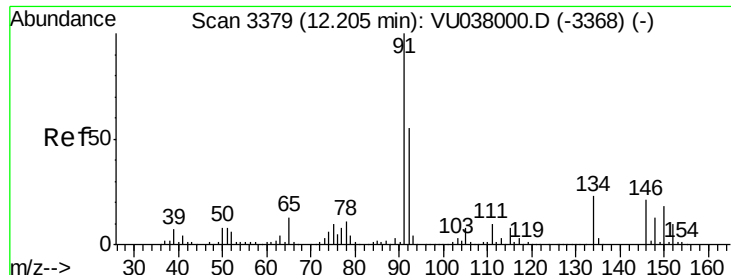

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.908 ug/l
 RT: 12.20 min Scan# 3379
 Delta R.T. 0.00 min
 Lab File: VU038010.D
 Acq: 05 May 2020 11:26

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0505WBL01

Tot Ion	Ratio	Lower	Upper
152	100		
115	63.6	0.0	261.0
150	161.2	0.0	650.2

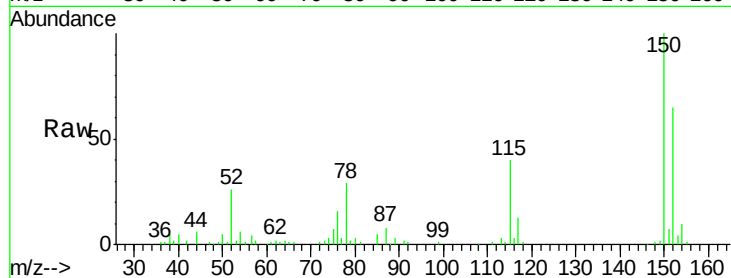

Abundance

Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

