

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050520\
 Data File : VU038010.D
 Acq On : 05 May 2020 11:26
 Operator : JC/MD
 Sample : VU0505WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0505WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.080	532	541	552	rVB5	7947	14717	7.43%	2.032%
2	4.707	1034	1047	1060	rBV2	10080	23099	11.66%	3.190%
3	5.121	1171	1176	1186	rVB9	1697	3338	1.69%	0.461%
4	5.411	1256	1266	1270	rBV6	1730	3166	1.60%	0.437%
5	5.742	1357	1369	1380	rBV6	2017	4305	2.17%	0.594%
6	6.144	1480	1494	1513	rBV	94588	187105	94.46%	25.838%
7	6.276	1527	1535	1537	rBV5	2606	2808	1.42%	0.388%
8	6.571	1620	1627	1635	rBV5	3283	4623	2.33%	0.638%
9	7.822	2007	2016	2030	rVB6	2798	5186	2.62%	0.716%
10	7.922	2039	2047	2054	rBV5	2992	4759	2.40%	0.657%
11	8.571	2242	2249	2256	rBV5	3060	4157	2.10%	0.574%
12	8.710	2284	2292	2298	rBV6	2511	4175	2.11%	0.577%
13	8.944	2356	2365	2382	rBV4	6584	11847	5.98%	1.636%
14	9.433	2511	2517	2522	rBV4	2107	3129	1.58%	0.432%
15	9.465	2525	2527	2535	rVB4	1994	2018	1.02%	0.279%
16	9.713	2596	2604	2611	rVB2	2264	3387	1.71%	0.468%
17	10.128	2723	2733	2741	rBV8	2463	3708	1.87%	0.512%
18	10.501	2841	2849	2858	rBV3	4784	7195	3.63%	0.994%
19	10.648	2879	2895	2908	rBV2	85698	142148	71.76%	19.630%
20	10.796	2936	2941	2949	rBV5	1659	2069	1.04%	0.286%
21	11.102	3029	3036	3037	rBV3	2920	2224	1.12%	0.307%
22	11.330	3099	3107	3115	rBV5	5154	7258	3.66%	1.002%
23	11.481	3147	3154	3161	rVB3	2418	2997	1.51%	0.414%
24	11.658	3204	3209	3218	rVB3	2094	2378	1.20%	0.328%
25	11.758	3232	3240	3249	rBV5	3936	5542	2.80%	0.765%
26	11.825	3249	3261	3266	rBV6	5701	10925	5.52%	1.509%
27	11.851	3267	3269	3277	rVB7	4142	3942	1.99%	0.544%
28	12.208	3368	3380	3397	rBV	116330	198086	100.00%	27.355%
29	12.800	3556	3564	3570	rBV2	1761	2799	1.41%	0.387%
30	13.044	3626	3640	3652	rBV5	10644	17377	8.77%	2.400%
31	13.870	3889	3897	3907	rVB6	7970	12323	6.22%	1.702%
32	14.053	3949	3954	3959	rVB5	1916	2027	1.02%	0.280%
33	14.118	3966	3974	3984	rVB2	5983	9240	4.66%	1.276%
34	14.365	4042	4051	4060	rVB6	6097	10082	5.09%	1.392%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050520\
Data File : VU038010.D
Acq On : 05 May 2020 11:26
Operator : JC/MD
Sample : VU0505WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0505WBL01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER


Sum of corrected areas: 724139

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050520\
Data File : VU038010.D
Acq On : 05 May 2020 11:26
Operator : JC/MD
Sample : VU0505WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0505WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U050420DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

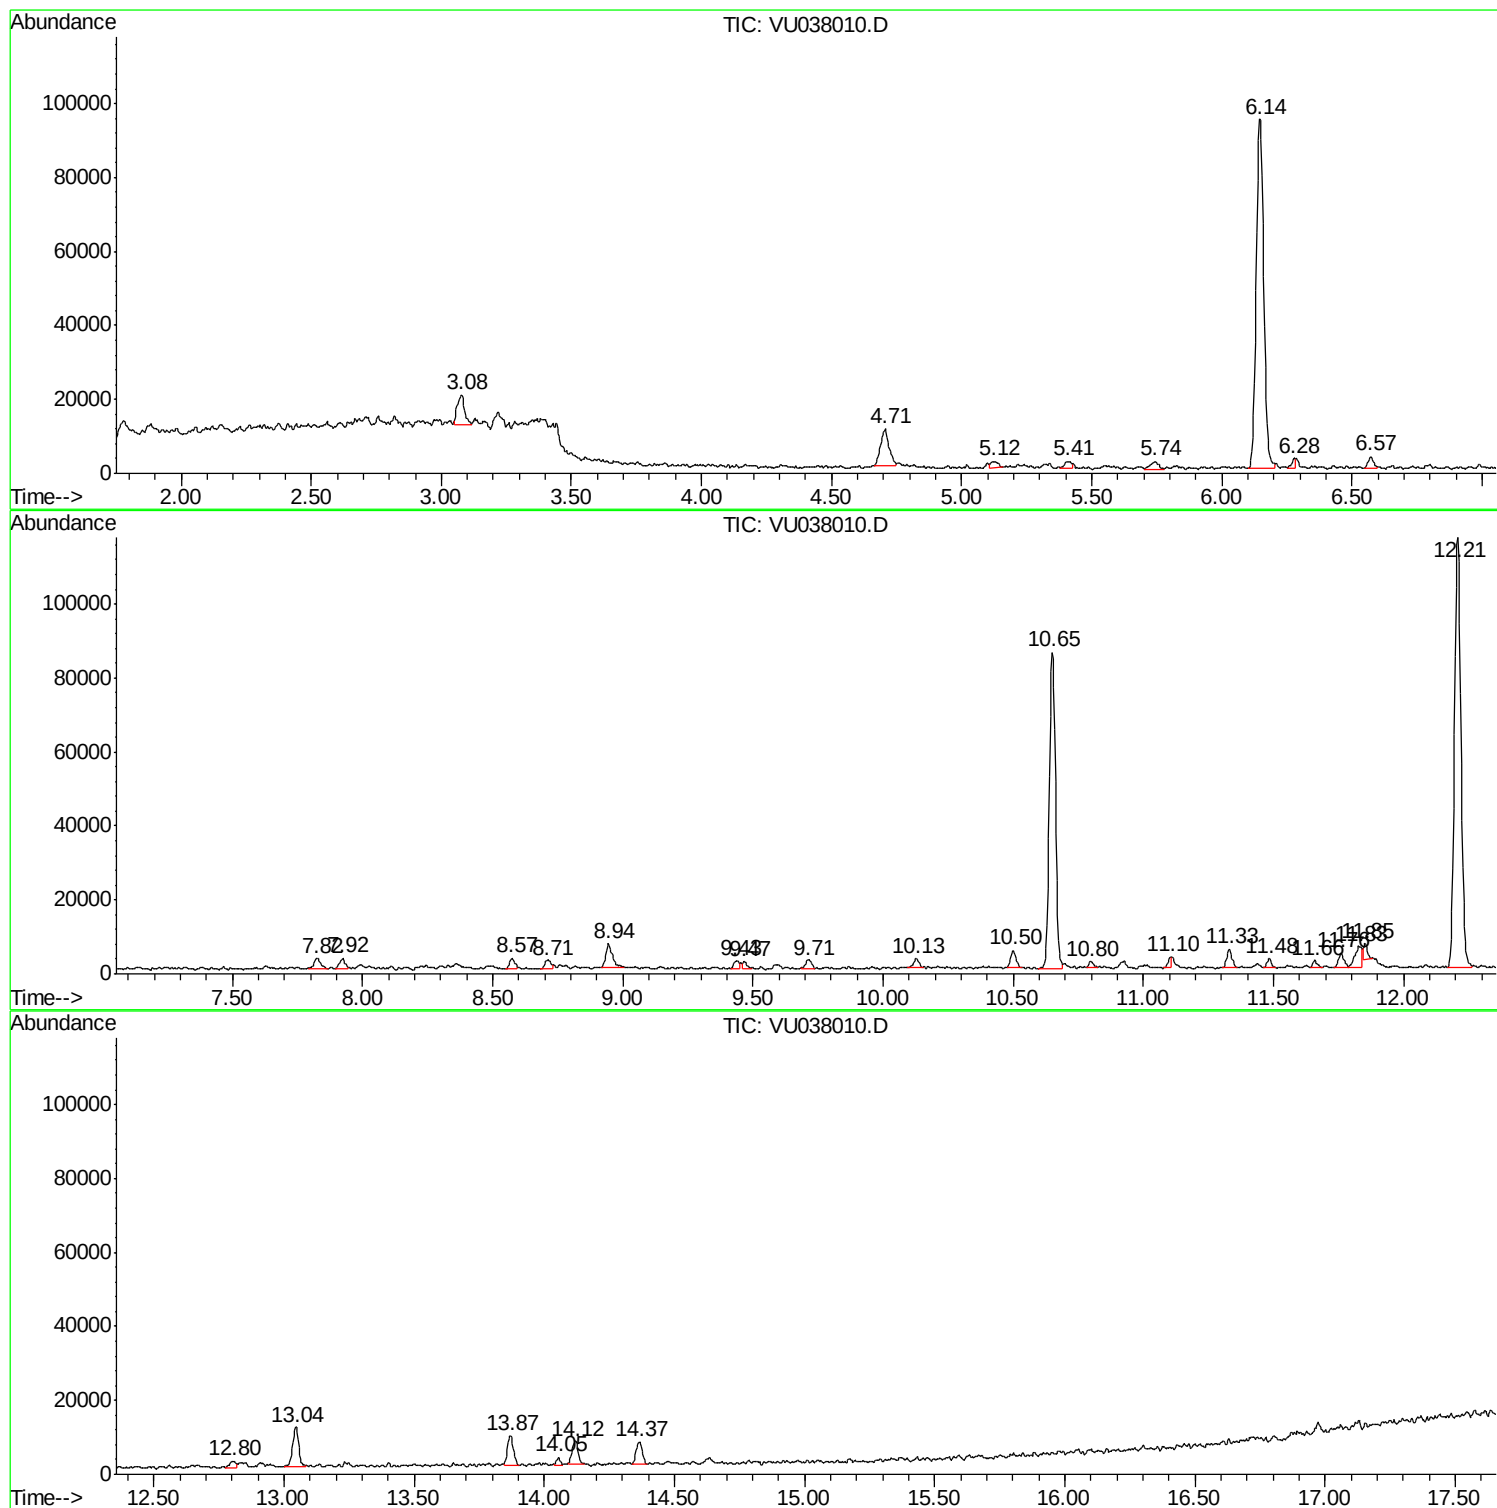

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050520\
Data File : VU038010.D
Acq On : 05 May 2020 11:26
Operator : JC/MD
Sample : VU0505WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0505WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U050420DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU050520\
Data File : VU038010.D
Acq On : 05 May 2020 11:26
Operator : JC/MD
Sample : VU0505WBL01
Misc : 25.0mL/MSV0A_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
VU0505WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\524U050420DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc