


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050521\
Data File : VU043549.D
Acq On : 05 May 2021 12:35
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Title : SW846 8260
Last Update : Mon Apr 12 13:17:29 2021

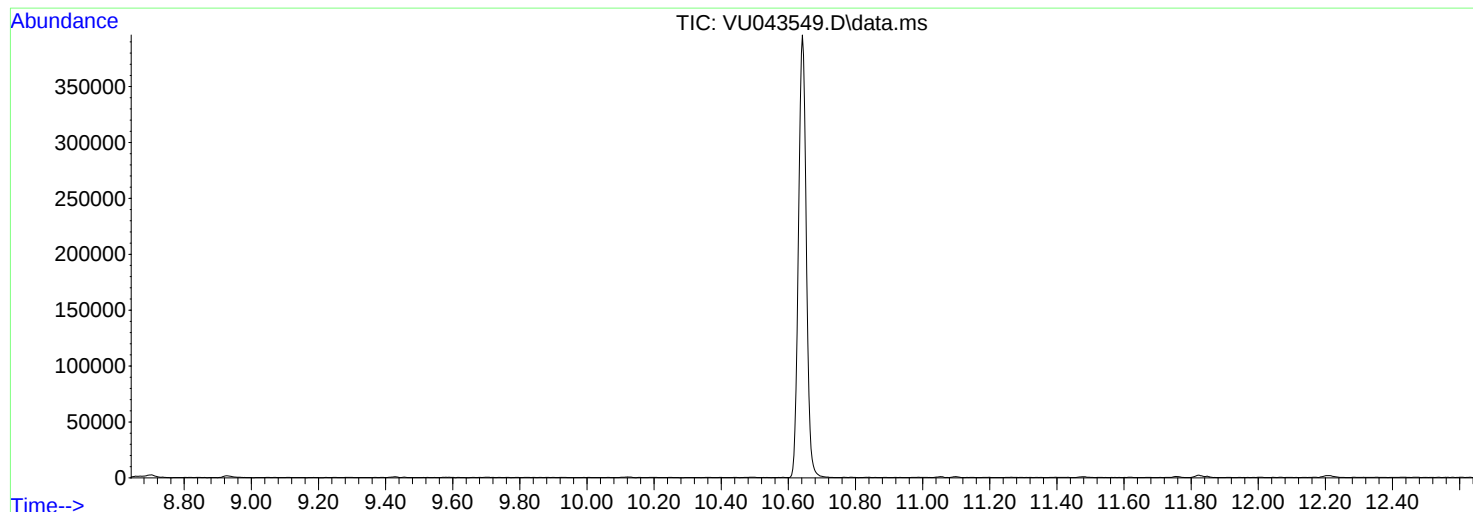

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.3	18075	PASS
75	95	30	60	57.8	41291	PASS
95	95	100	100	100.0	71416	PASS
96	95	5	9	7.2	5130	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.6	58251	PASS
175	174	5	9	8.1	4694	PASS
176	174	95	101	95.8	55792	PASS
177	176	5	9	6.5	3608	PASS