




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048429.D
Acq On : 05 May 2022 10:32
Operator : SY/MD
Sample : VU0505MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK115

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/06/2022
Supervised By :Mahesh Dadoda 05/06/2022

Quant Time: May 06 06:56:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 06 05:30:23 2022
Response via : Initial Calibration

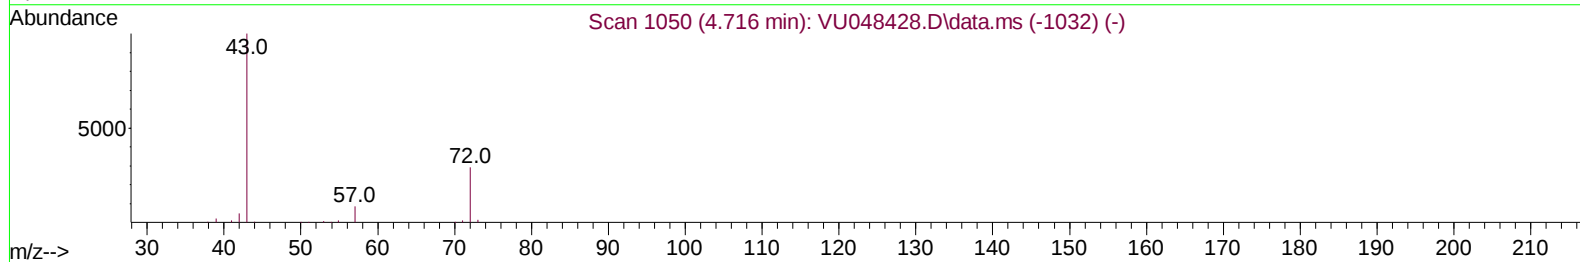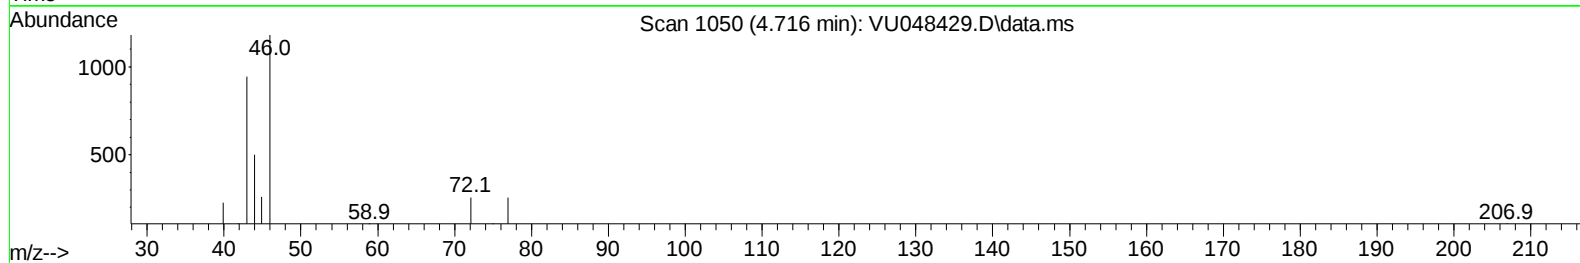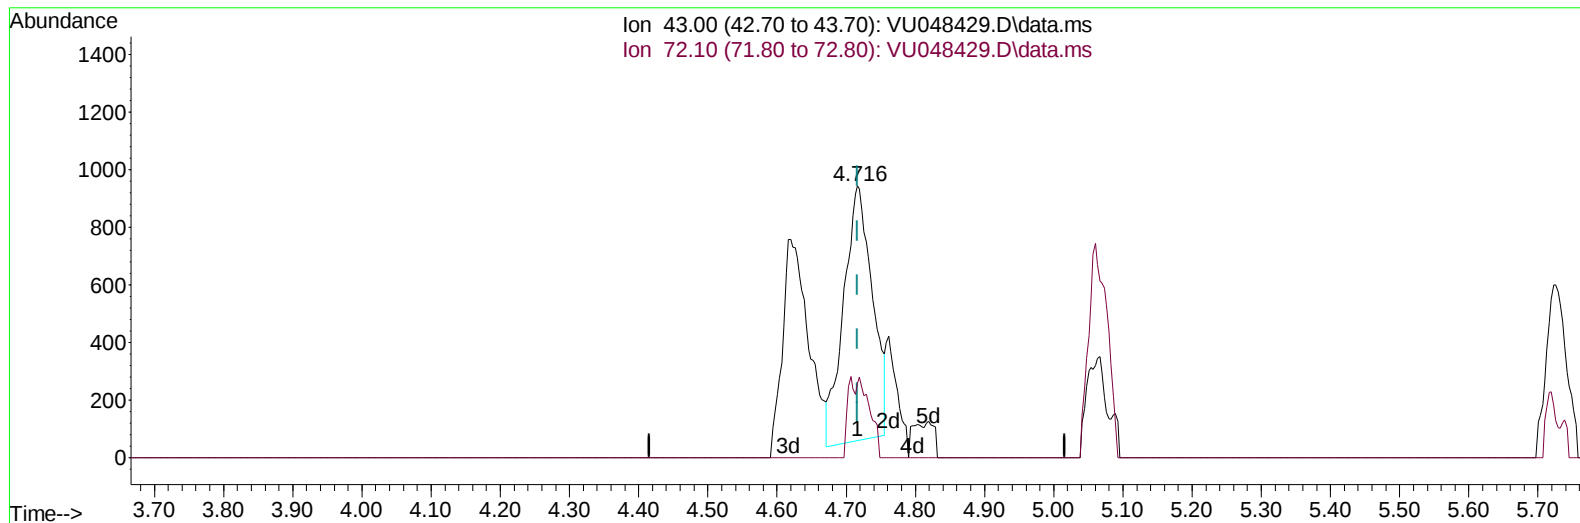

TIC: VU048429.D\data.ms

(22) 2-Butanone (T)

4.716min (+ 0.000) 0.97 ug/L

response 2556

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.20	7.94#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048429.D
 Acq On : 05 May 2022 10:32
 Operator : SY/MD
 Sample : VU0505MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK115

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/06/2022
 Supervised By :Mahesh Dadoda 05/06/2022

Quant Time: May 06 06:56:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 06 05:30:23 2022
 Response via : Initial Calibration

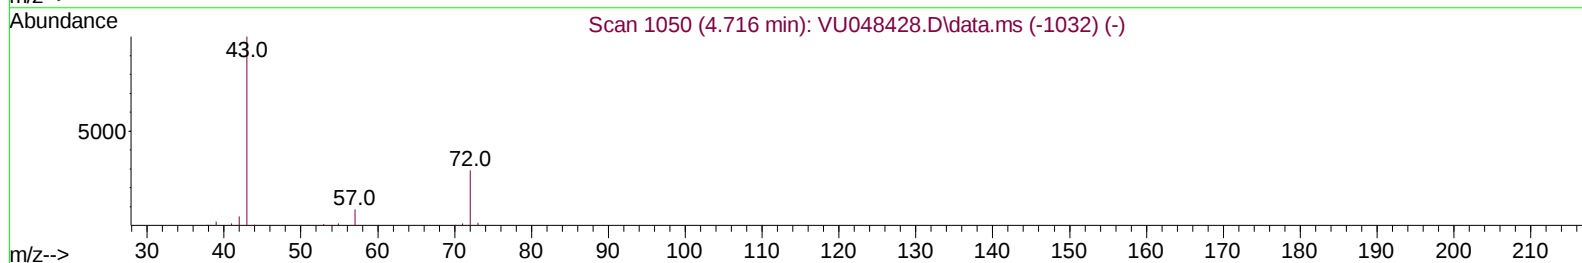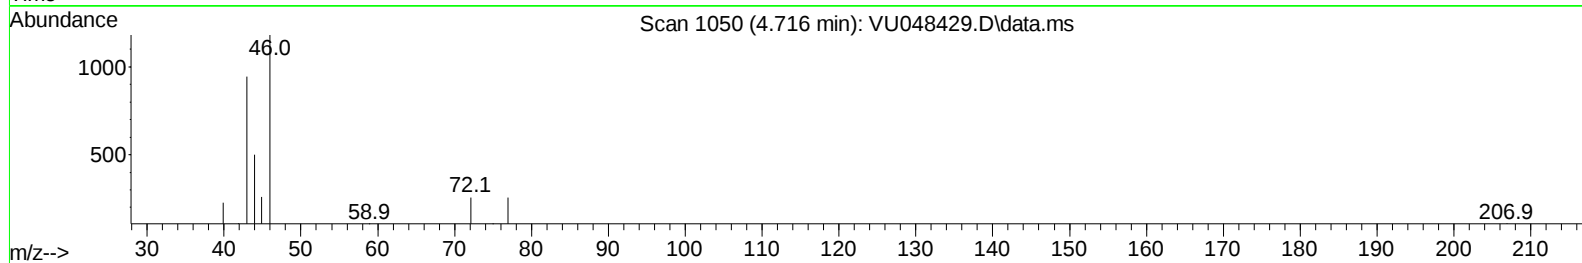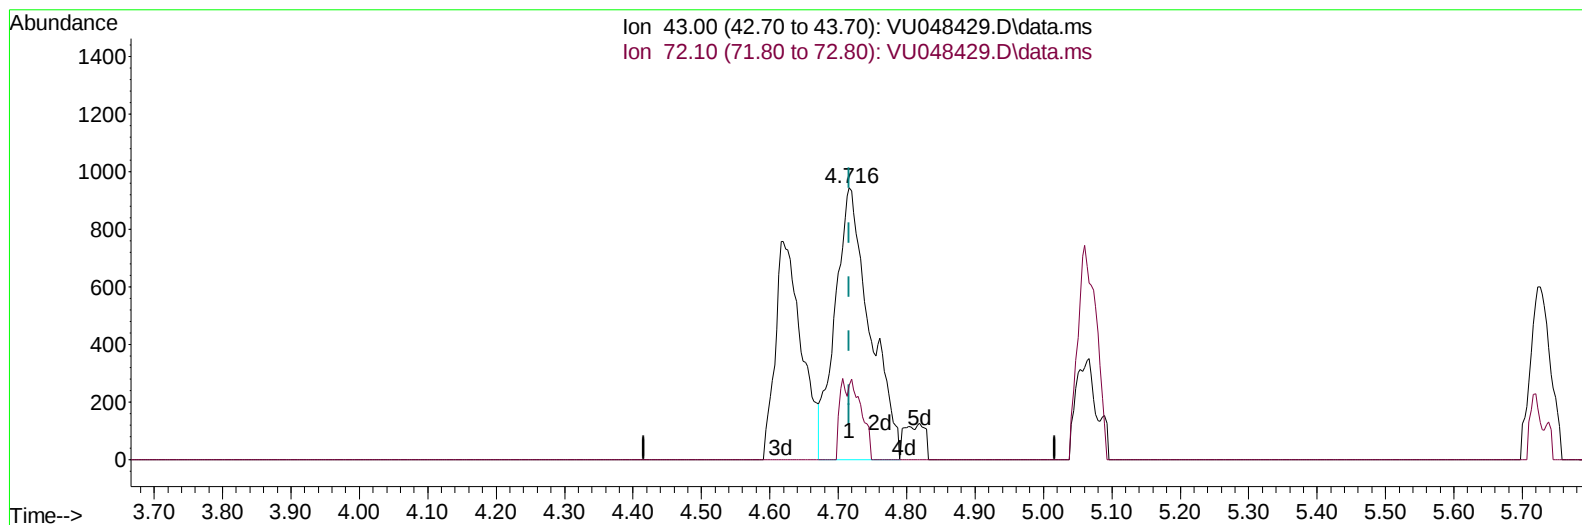

TIC: VU048429.D\data.ms

(22) 2-Butanone (T)

4.716min (+ 0.000) 1.27 ug/L m

response 3331

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.20	6.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048429.D
 Acq On : 05 May 2022 10:32
 Operator : SY/MD
 Sample : VU0505MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK115

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 05/06/2022
 Supervised By : Mahesh Dadoda 05/06/2022

Quant Time: May 06 06:56:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 06 05:30:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	352975	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	356306	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	167075	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	156769	48.298	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	96.600%	
7) Chloroethane-d5	1.896	69	113452	49.795	ug/L	-0.02
Spiked Amount 50.000	Range 70	- 130	Recovery	=	99.580%	
11) 1,1-Dichloroethene-d2	2.565	63	187850	36.119	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	72.240%	
21) 2-Butanone-d5	4.620	46	258094	93.228	ug/L	-0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	93.230%	
24) Chloroform-d	5.063	84	263193	44.704	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.400%	
26) 1,2-Dichloroethane-d4	5.700	65	159427	45.639	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.280%	
32) Benzene-d6	5.726	84	582463	51.832	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	103.660%	
36) 1,2-Dichloropropane-d6	6.690	67	186678	50.248	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	100.500%	
41) Toluene-d8	7.899	98	501619	49.246	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.500%	
43) trans-1,3-Dichloroprop...	8.179	79	74607	45.511	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	91.020%	
47) 2-Hexanone-d5	8.636	63	183494	91.546	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	91.550%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	297028	45.587	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	91.180%	
66) 1,2-Dichlorobenzene-d4	12.195	152	201032	53.489	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	106.980%	
Target Compounds						
22) 2-Butanone	4.716	43	3331m	1.267	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048429.D
Acq On : 05 May 2022 10:32
Operator : SY/MD
Sample : VU0505MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK115

Manual IntegrationsAPPROVED

Quant Time: May 06 06:56:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 06 05:30:23 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/06/2022
Supervised By :Mahesh Dadoda 05/06/2022

