

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048430.D
 Acq On : 05 May 2022 11:01
 Operator : SY/MD
 Sample : VU0505WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK116

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	105	rBV	174734	225959	15.49%	2.024%
2	1.896	165	173	189	rBV	112508	164183	11.25%	1.471%
3	2.565	368	381	400	rBV	302017	497540	34.11%	4.457%
4	2.755	437	440	444	rBV	255	206	0.01%	0.002%
5	2.944	495	499	506	rVV2	297	269	0.02%	0.002%
6	3.051	520	532	545	rBV3	2434	5004	0.34%	0.045%
7	3.182	559	573	591	rBV2	12084	28986	1.99%	0.260%
8	3.581	693	697	698	rBV	281	157	0.01%	0.001%
9	3.906	794	798	805	rBV	191	178	0.01%	0.002%
10	4.076	846	851	857	rVV2	173	225	0.02%	0.002%
11	4.620	1007	1020	1049	rBV	165317	401590	27.53%	3.597%
12	4.822	1078	1083	1086	rBV3	439	424	0.03%	0.004%
13	4.957	1123	1125	1130	rVB2	210	160	0.01%	0.001%
14	5.063	1140	1158	1179	rBV	253207	551482	37.80%	4.940%
15	5.285	1223	1227	1236	rVV4	466	554	0.04%	0.005%
16	5.333	1238	1242	1243	rBV3	241	179	0.01%	0.002%
17	5.423	1268	1270	1275	rVB	268	181	0.01%	0.002%
18	5.726	1342	1364	1388	rBV2	547823	1458765	100.00%	13.068%
19	5.970	1437	1440	1443	rVB3	402	281	0.02%	0.003%
20	6.047	1460	1464	1467	rBV2	495	460	0.03%	0.004%
21	6.250	1510	1527	1549	rBV	371625	703765	48.24%	6.304%
22	6.491	1598	1602	1606	rVB	265	208	0.01%	0.002%
23	6.529	1606	1614	1624	rBV7	2347	4907	0.34%	0.044%
24	6.690	1649	1664	1684	rBV	335194	653701	44.81%	5.856%
25	6.806	1696	1700	1702	rBV4	539	440	0.03%	0.004%
26	6.951	1739	1745	1753	rBV2	276	292	0.02%	0.003%
27	7.041	1770	1773	1779	rVV3	284	339	0.02%	0.003%
28	7.073	1779	1783	1786	rVB2	272	196	0.01%	0.002%
29	7.182	1805	1817	1831	rVB5	3624	7167	0.49%	0.064%
30	7.259	1838	1841	1844	rBV	247	174	0.01%	0.002%
31	7.301	1849	1854	1856	rBV	277	287	0.02%	0.003%
32	7.491	1908	1913	1915	rBV	205	188	0.01%	0.002%
33	7.565	1924	1936	1956	rBV	167006	294027	20.16%	2.634%
34	7.693	1968	1976	1984	rVB3	1498	2357	0.16%	0.021%
35	7.790	2000	2006	2011	rBV3	869	958	0.07%	0.009%
36	7.899	2024	2040	2058	rBV	670334	1179294	80.84%	10.564%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048430.D
 Acq On : 05 May 2022 11:01
 Operator : SY/MD
 Sample : VU0505WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK116

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	8.179	2114	2127	2152	rBV	116660	199655	13.69%	1.789%
38	8.472	2213	2218	2222	rBV3	292	390	0.03%	0.003%
39	8.545	2238	2241	2248	rBV3	645	665	0.05%	0.006%
40	8.635	2253	2269	2307	rBV2	480265	926423	63.51%	8.299%
41	8.790	2315	2317	2322	rVB2	905	594	0.04%	0.005%
42	8.812	2322	2324	2329	rVB2	403	280	0.02%	0.003%
43	8.838	2329	2332	2335	rVB	343	230	0.02%	0.002%
44	8.867	2335	2341	2342	rBV2	334	342	0.02%	0.003%
45	9.153	2428	2430	2433	rVV2	333	213	0.01%	0.002%
46	9.169	2433	2435	2443	rVB2	390	282	0.02%	0.003%
47	9.227	2447	2453	2458	rVB2	324	384	0.03%	0.003%
48	9.262	2458	2464	2467	rBV3	330	380	0.03%	0.003%
49	9.307	2474	2478	2482	rBV	185	221	0.02%	0.002%
50	9.417	2499	2512	2535	rBV	540942	914756	62.71%	8.194%
51	9.574	2556	2561	2565	rVB3	914	771	0.05%	0.007%
52	9.613	2569	2573	2580	rBV2	335	373	0.03%	0.003%
53	9.648	2580	2584	2586	rBV	270	208	0.01%	0.002%
54	9.697	2592	2599	2606	rBV4	897	1310	0.09%	0.012%
55	9.844	2643	2645	2650	rBV	218	160	0.01%	0.001%
56	10.005	2692	2695	2697	rBV	221	157	0.01%	0.001%
57	10.021	2697	2700	2707	rVB2	299	345	0.02%	0.003%
58	10.057	2707	2711	2713	rBV2	186	156	0.01%	0.001%
59	10.102	2723	2725	2727	rVV	433	225	0.02%	0.002%
60	10.115	2727	2729	2733	rVV2	498	321	0.02%	0.003%
61	10.214	2757	2760	2762	rBV	247	203	0.01%	0.002%
62	10.304	2785	2788	2790	rBV	266	180	0.01%	0.002%
63	10.375	2807	2810	2812	rBV2	274	164	0.01%	0.001%
64	10.397	2814	2817	2823	rVB2	216	227	0.02%	0.002%
65	10.439	2825	2830	2833	rBV2	164	160	0.01%	0.001%
66	10.484	2837	2844	2847	rBV2	539	726	0.05%	0.007%
67	10.568	2867	2870	2877	rVB	224	296	0.02%	0.003%
68	10.606	2877	2882	2884	rBV	245	245	0.02%	0.002%
69	10.642	2891	2893	2898	rBV5	493	372	0.03%	0.003%
70	10.674	2898	2903	2910	rVB4	1580	1888	0.13%	0.017%
71	10.758	2915	2929	2952	rBV	554134	896937	61.49%	8.035%
72	10.870	2959	2964	2965	rBV3	377	315	0.02%	0.003%
73	11.060	3019	3023	3026	rVB2	218	161	0.01%	0.001%
74	11.082	3026	3030	3034	rBV3	432	450	0.03%	0.004%
75	11.118	3038	3041	3047	rVB4	492	487	0.03%	0.004%
76	11.150	3047	3051	3053	rBV2	304	245	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048430.D
 Acq On : 05 May 2022 11:01
 Operator : SY/MD
 Sample : VU0505WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK116

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.317	3100	3103	3106	rBV2	419	373	0.03%	0.003%
78	11.391	3121	3126	3128	rBV2	307	275	0.02%	0.002%
79	11.420	3133	3135	3138	rVV	387	195	0.01%	0.002%
80	11.462	3142	3148	3162	rVB6	1469	2769	0.19%	0.025%
81	11.536	3167	3171	3174	rBV2	326	346	0.02%	0.003%
82	11.642	3201	3204	3208	rVB3	278	194	0.01%	0.002%
83	11.687	3215	3218	3220	rBV2	322	192	0.01%	0.002%
84	11.812	3244	3257	3276	rBV	557834	898104	61.57%	8.045%
85	11.970	3303	3306	3313	rVB3	927	933	0.06%	0.008%
86	12.124	3351	3354	3355	rBV	408	186	0.01%	0.002%
87	12.195	3362	3376	3397	rBV	674286	1101237	75.49%	9.865%
88	12.333	3413	3419	3421	rBV3	629	550	0.04%	0.005%
89	12.568	3487	3492	3496	rBV2	424	397	0.03%	0.004%
90	12.716	3532	3538	3544	rVB3	419	583	0.04%	0.005%
91	12.741	3544	3546	3549	rBV2	278	188	0.01%	0.002%
92	12.770	3549	3555	3556	rBV	923	892	0.06%	0.008%
93	12.880	3585	3589	3590	rBV	317	218	0.01%	0.002%
94	12.918	3597	3601	3603	rBV	605	460	0.03%	0.004%
95	13.227	3691	3697	3706	rVB2	916	1416	0.10%	0.013%
96	13.291	3714	3717	3721	rBV2	317	328	0.02%	0.003%
97	13.847	3883	3890	3896	rBV3	2220	2987	0.20%	0.027%
98	14.095	3957	3967	3984	rBV	4965	8775	0.60%	0.079%
99	14.333	4036	4041	4055	rVB5	2970	4379	0.30%	0.039%
100	15.108	4279	4282	4283	rBV	539	287	0.02%	0.003%




Sum of corrected areas: 11163244

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048430.D
Acq On : 05 May 2022 11:01
Operator : SY/MD
Sample : VU0505WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

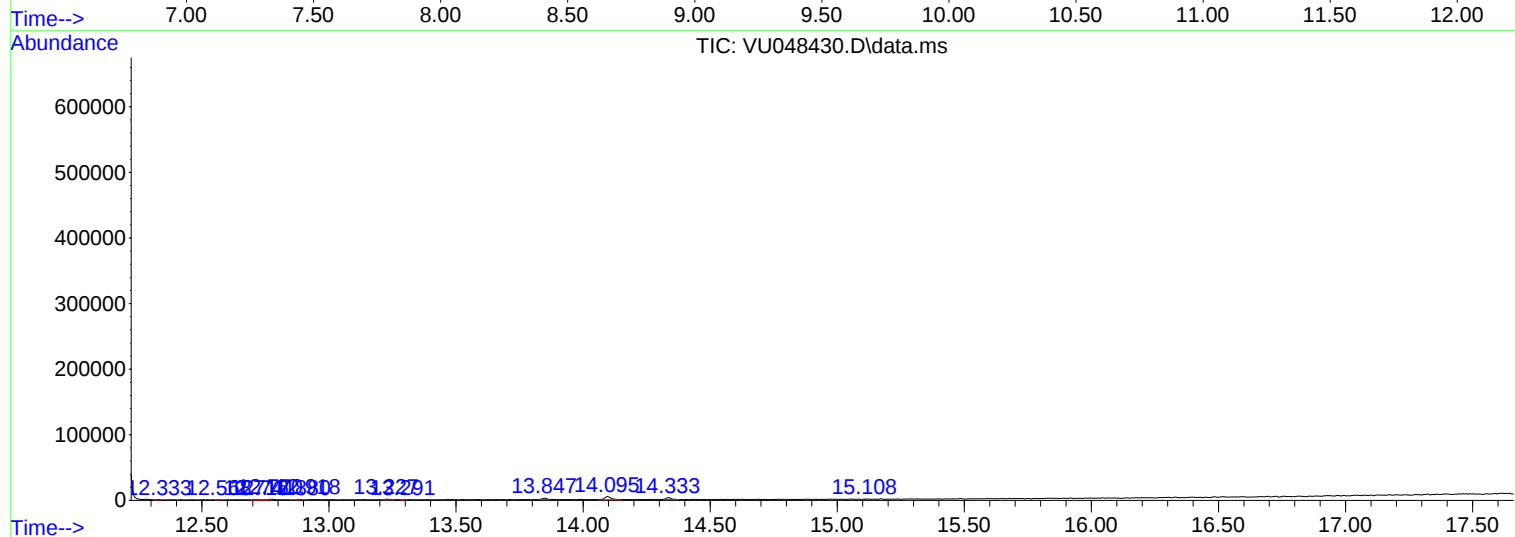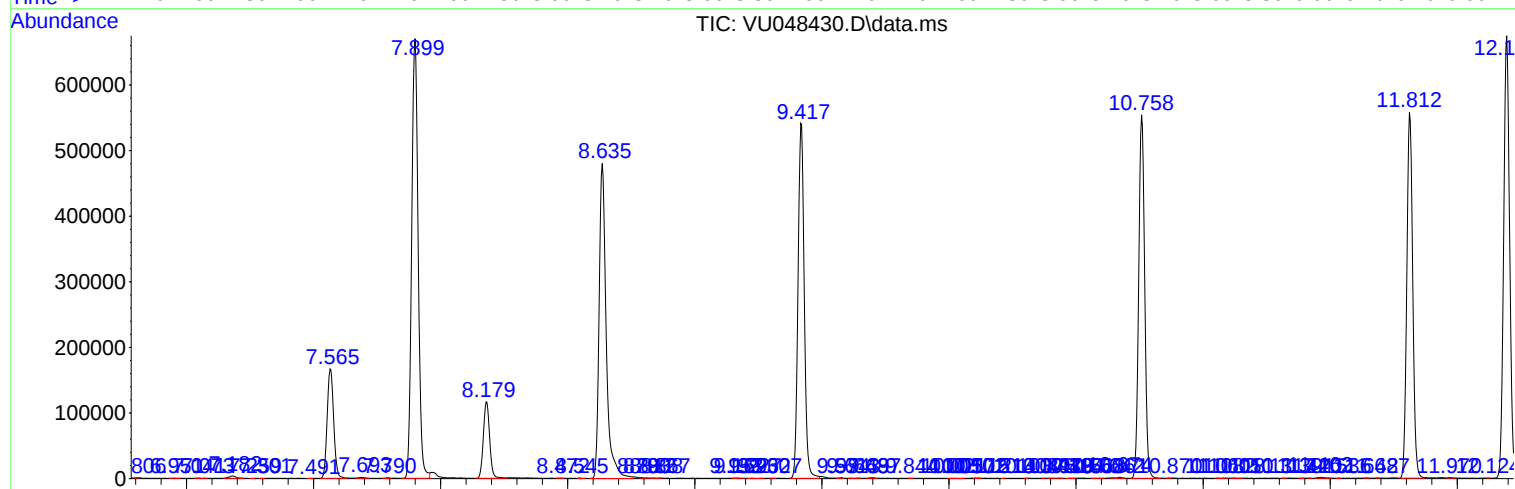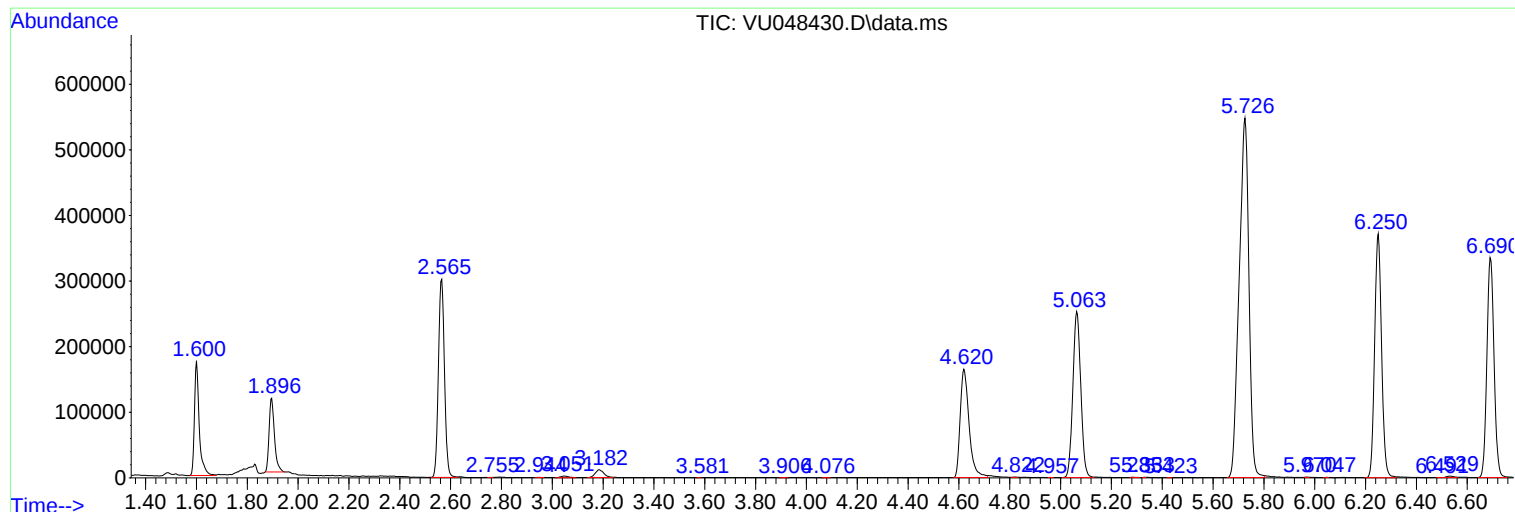

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048430.D
Acq On : 05 May 2022 11:01
Operator : SY/MD
Sample : VU0505WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048430.D
Acq On : 05 May 2022 11:01
Operator : SY/MD
Sample : VU0505WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------