

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048439.D
 Acq On : 05 May 2022 15:58
 Operator : SY/MD
 Sample : N2710-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	36	44	52	rBV2	19217	32287	2.04%	0.275%
2	1.601	74	81	99	rBV	183524	233695	14.80%	1.994%
3	1.900	166	174	186	rBV	125245	178788	11.32%	1.525%
4	2.565	368	381	397	rBV	318856	525016	33.25%	4.480%
5	2.716	426	428	431	rVB2	360	226	0.01%	0.002%
6	2.736	431	434	436	rBV	332	172	0.01%	0.001%
7	2.761	439	442	445	rVV2	393	306	0.02%	0.003%
8	2.790	445	451	460	rVB3	1067	1525	0.10%	0.013%
9	2.961	498	504	505	rBV2	356	299	0.02%	0.003%
10	3.006	512	518	525	rVB3	248	411	0.03%	0.004%
11	3.051	525	532	538	rBV5	810	1268	0.08%	0.011%
12	3.192	558	576	583	rBV3	2625	6319	0.40%	0.054%
13	3.395	636	639	641	rBV	265	173	0.01%	0.001%
14	3.472	656	663	666	rBV3	288	302	0.02%	0.003%
15	3.491	666	669	675	rVV2	168	180	0.01%	0.002%
16	3.581	691	697	701	rVB2	238	246	0.02%	0.002%
17	3.613	701	707	711	rBV2	325	316	0.02%	0.003%
18	3.671	719	725	729	rBV2	210	267	0.02%	0.002%
19	3.771	753	756	760	rVV3	268	204	0.01%	0.002%
20	3.819	767	771	776	rBV2	163	176	0.01%	0.002%
21	4.141	866	871	877	rVB	183	164	0.01%	0.001%
22	4.176	877	882	885	rBV2	186	166	0.01%	0.001%
23	4.346	931	935	940	rVB2	223	204	0.01%	0.002%
24	4.388	945	948	954	rVV2	166	171	0.01%	0.001%
25	4.620	1006	1020	1047	rBV	177866	424738	26.90%	3.624%
26	4.896	1103	1106	1110	rVB3	399	321	0.02%	0.003%
27	5.063	1139	1158	1182	rBV	275206	599832	37.98%	5.118%
28	5.276	1220	1224	1225	rBV	394	240	0.02%	0.002%
29	5.488	1284	1290	1293	rBV2	274	299	0.02%	0.003%
30	5.726	1342	1364	1397	rBV2	592983	1579207	100.00%	13.474%
31	5.970	1436	1440	1446	rVB4	730	802	0.05%	0.007%
32	6.028	1456	1458	1463	rBV2	477	338	0.02%	0.003%
33	6.105	1476	1482	1486	rBV3	458	424	0.03%	0.004%
34	6.250	1512	1527	1552	rBV	395477	752004	47.62%	6.416%
35	6.446	1585	1588	1595	rBV3	225	259	0.02%	0.002%
36	6.530	1607	1614	1621	rBV4	2142	4060	0.26%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048439.D
 Acq On : 05 May 2022 15:58
 Operator : SY/MD
 Sample : N2710-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1690	rBV	363604	702994	44.52%	5.998%
38	6.809	1698	1701	1708	rVB4	1134	1390	0.09%	0.012%
39	6.838	1708	1710	1715	rVB2	372	312	0.02%	0.003%
40	6.880	1717	1723	1725	rBV	184	207	0.01%	0.002%
41	6.912	1730	1733	1738	rVB3	313	271	0.02%	0.002%
42	7.009	1761	1763	1766	rBV	271	176	0.01%	0.002%
43	7.044	1766	1774	1777	rBV2	449	541	0.03%	0.005%
44	7.179	1805	1816	1828	rBV7	4062	8640	0.55%	0.074%
45	7.324	1859	1861	1867	rVB3	259	191	0.01%	0.002%
46	7.430	1889	1894	1900	rVB2	249	288	0.02%	0.002%
47	7.565	1922	1936	1964	rBV	188755	329195	20.85%	2.809%
48	7.690	1967	1975	1985	rVB6	2208	4056	0.26%	0.035%
49	7.761	1994	1997	1999	rBV2	268	210	0.01%	0.002%
50	7.787	2001	2005	2006	rBV2	300	169	0.01%	0.001%
51	7.848	2021	2024	2026	rBV2	239	177	0.01%	0.002%
52	7.899	2026	2040	2057	rBV	708282	1250285	79.17%	10.668%
53	8.179	2115	2127	2145	rBV	129910	217820	13.79%	1.859%
54	8.472	2209	2218	2228	rVB3	4337	7341	0.46%	0.063%
55	8.536	2234	2238	2241	rBV2	233	190	0.01%	0.002%
56	8.578	2247	2251	2256	rVB2	397	318	0.02%	0.003%
57	8.632	2256	2268	2297	rBV2	514815	957254	60.62%	8.168%
58	8.890	2346	2348	2354	rVB3	312	246	0.02%	0.002%
59	8.925	2354	2359	2362	rBV3	268	279	0.02%	0.002%
60	9.086	2404	2409	2412	rBV	359	282	0.02%	0.002%
61	9.153	2427	2430	2432	rBV3	310	204	0.01%	0.002%
62	9.205	2439	2446	2449	rVB3	265	295	0.02%	0.003%
63	9.417	2499	2512	2532	rBV	570983	940978	59.59%	8.029%
64	9.571	2557	2560	2566	rVB3	530	496	0.03%	0.004%
65	9.620	2571	2575	2579	rBV3	199	166	0.01%	0.001%
66	9.697	2594	2599	2602	rBV2	670	570	0.04%	0.005%
67	9.828	2638	2640	2643	rBV	233	165	0.01%	0.001%
68	10.070	2712	2715	2720	rVB2	189	171	0.01%	0.001%
69	10.102	2720	2725	2726	rBV	508	406	0.03%	0.003%
70	10.160	2739	2743	2746	rVB	210	175	0.01%	0.001%
71	10.179	2746	2749	2752	rBV2	303	227	0.01%	0.002%
72	10.295	2780	2785	2790	rBV	278	358	0.02%	0.003%
73	10.369	2804	2808	2814	rVB2	349	326	0.02%	0.003%
74	10.443	2828	2831	2834	rBV2	242	189	0.01%	0.002%
75	10.484	2839	2844	2849	rBV3	359	377	0.02%	0.003%
76	10.671	2894	2902	2914	rVB6	1678	2531	0.16%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048439.D
 Acq On : 05 May 2022 15:58
 Operator : SY/MD
 Sample : N2710-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.758	2915	2929	2952	rBV	577966	931122	58.96%	7.945%
78	10.893	2958	2971	2987	rBV	10678	19073	1.21%	0.163%
79	11.118	3037	3041	3042	rBV2	411	346	0.02%	0.003%
80	11.150	3048	3051	3053	rVB2	351	183	0.01%	0.002%
81	11.250	3079	3082	3085	rBV	216	165	0.01%	0.001%
82	11.304	3095	3099	3103	rVB2	377	296	0.02%	0.003%
83	11.330	3103	3107	3110	rVV2	220	202	0.01%	0.002%
84	11.349	3110	3113	3116	rVB3	479	321	0.02%	0.003%
85	11.410	3129	3132	3133	rBV3	367	193	0.01%	0.002%
86	11.462	3140	3148	3161	rVB3	1274	2448	0.16%	0.021%
87	11.539	3167	3172	3173	rBV	247	178	0.01%	0.002%
88	11.697	3216	3221	3227	rVB2	658	655	0.04%	0.006%
89	11.812	3245	3257	3281	rBV	558824	878661	55.64%	7.497%
90	11.941	3294	3297	3301	rBV4	537	463	0.03%	0.004%
91	11.970	3303	3306	3314	rVB5	1369	1593	0.10%	0.014%
92	12.060	3329	3334	3335	rBV2	886	639	0.04%	0.005%
93	12.195	3359	3376	3395	rBV	673991	1098952	69.59%	9.377%
94	12.510	3471	3474	3479	rBV3	272	262	0.02%	0.002%
95	12.558	3486	3489	3493	rBV2	256	292	0.02%	0.002%
96	12.616	3504	3507	3509	rBV2	340	236	0.01%	0.002%
97	12.732	3540	3543	3545	rBV3	309	173	0.01%	0.001%
98	12.771	3545	3555	3566	rBV2	3963	7105	0.45%	0.061%
99	13.201	3686	3689	3692	rBV2	361	324	0.02%	0.003%
100	15.137	4289	4291	4294	rBV3	483	295	0.02%	0.003%




Sum of corrected areas: 11720048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048439.D
Acq On : 05 May 2022 15:58
Operator : SY/MD
Sample : N2710-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

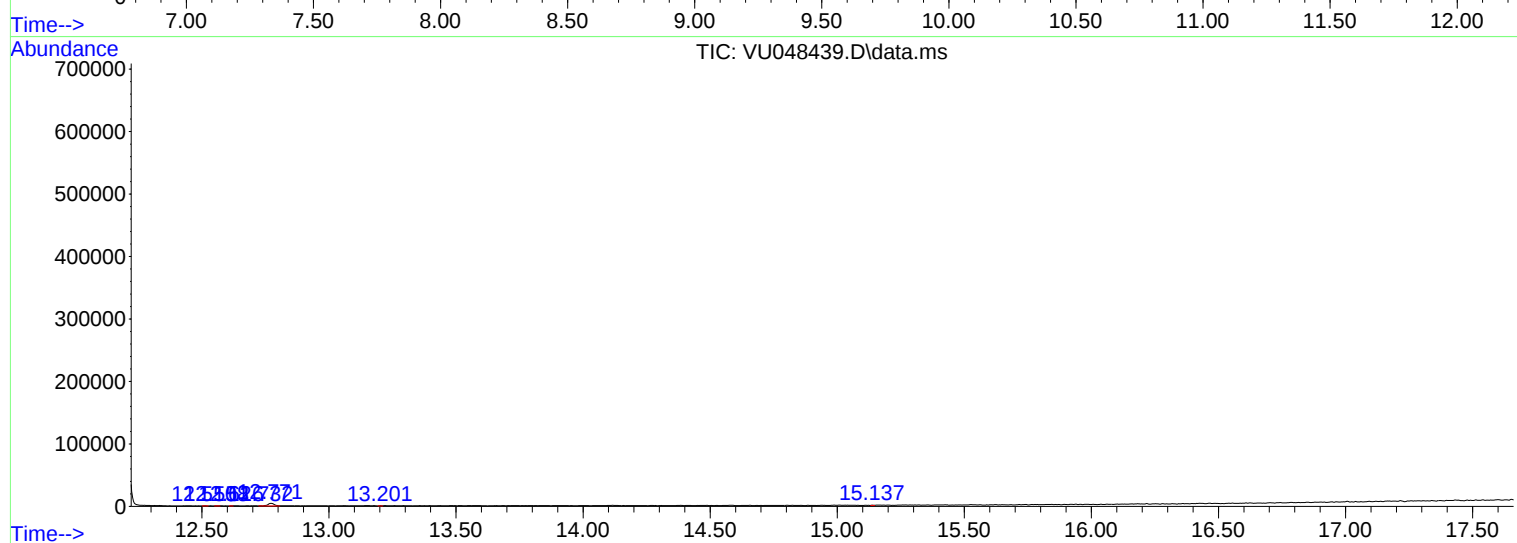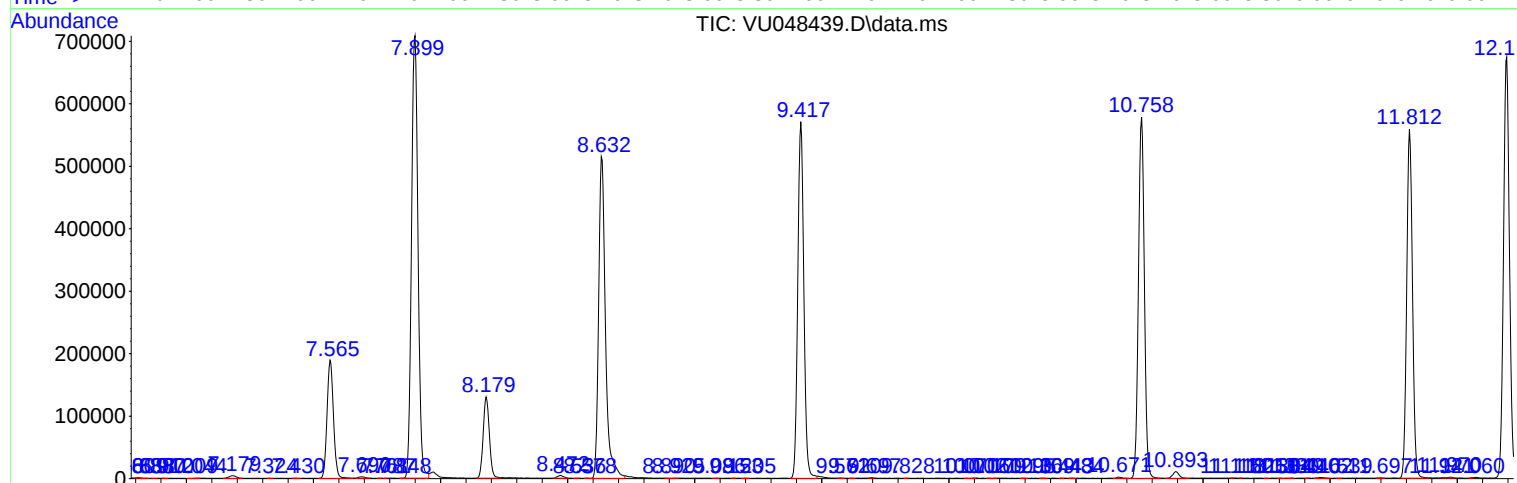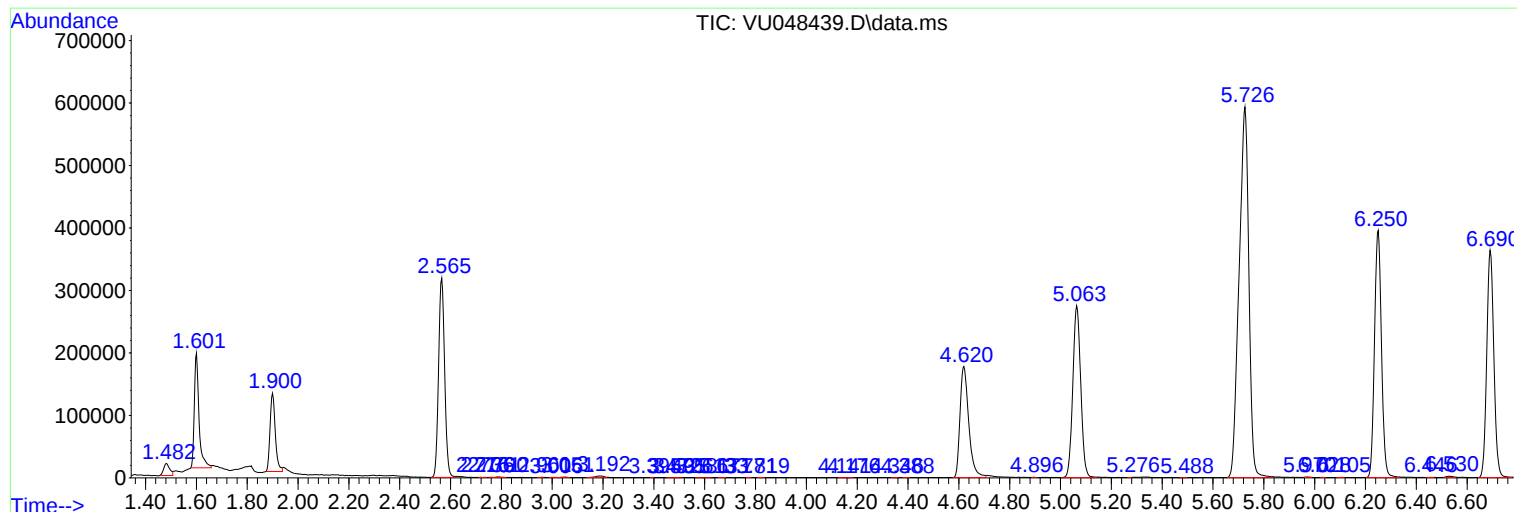

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048439.D
Acq On : 05 May 2022 15:58
Operator : SY/MD
Sample : N2710-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048439.D
Acq On : 05 May 2022 15:58
Operator : SY/MD
Sample : N2710-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc