

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048442.D
 Acq On : 05 May 2022 17:10
 Operator : SY/MD
 Sample : N2710-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	38	45	52	rBV2	11102	16928	1.13%	0.147%
2	1.601	73	81	104	rBV	168180	231814	15.51%	2.014%
3	1.890	163	171	187	rVB	117347	174485	11.67%	1.516%
4	2.562	368	380	397	rBV	301916	494508	33.08%	4.296%
5	2.687	416	419	424	rVB3	366	339	0.02%	0.003%
6	2.787	435	450	456	rBV6	1895	4259	0.28%	0.037%
7	2.896	481	484	491	rBV3	371	336	0.02%	0.003%
8	2.945	495	499	503	rBV3	287	306	0.02%	0.003%
9	3.044	521	530	537	rBV3	795	1135	0.08%	0.010%
10	3.183	560	573	596	rVV2	11125	26456	1.77%	0.230%
11	3.305	609	611	617	rVB3	274	247	0.02%	0.002%
12	3.453	649	657	660	rBV2	171	223	0.01%	0.002%
13	3.752	746	750	756	rBV2	234	185	0.01%	0.002%
14	3.945	807	810	816	rVB2	238	187	0.01%	0.002%
15	4.086	851	854	862	rVB2	196	188	0.01%	0.002%
16	4.170	873	880	883	rBV2	258	258	0.02%	0.002%
17	4.321	922	927	932	rBV2	225	274	0.02%	0.002%
18	4.507	982	985	992	rVB2	305	373	0.02%	0.003%
19	4.620	1006	1020	1047	rBV	174870	421044	28.16%	3.658%
20	4.813	1078	1080	1087	rVB3	493	383	0.03%	0.003%
21	5.063	1138	1158	1187	rBV	261764	571154	38.20%	4.962%
22	5.208	1200	1203	1208	rVB2	339	243	0.02%	0.002%
23	5.292	1222	1229	1231	rBV3	448	630	0.04%	0.005%
24	5.337	1235	1243	1255	rVB3	1375	2837	0.19%	0.025%
25	5.549	1306	1309	1314	rVB2	268	246	0.02%	0.002%
26	5.584	1314	1320	1324	rBV2	315	325	0.02%	0.003%
27	5.626	1329	1333	1337	rVB2	222	187	0.01%	0.002%
28	5.726	1342	1364	1395	rBV2	558054	1495083	100.00%	12.989%
29	5.970	1433	1440	1448	rBV4	871	1452	0.10%	0.013%
30	6.047	1458	1464	1468	rVB2	396	446	0.03%	0.004%
31	6.125	1484	1488	1491	rVB2	358	278	0.02%	0.002%
32	6.144	1491	1494	1497	rVB3	290	216	0.01%	0.002%
33	6.166	1497	1501	1507	rVB2	272	253	0.02%	0.002%
34	6.250	1511	1527	1556	rBV	379965	718496	48.06%	6.242%
35	6.530	1607	1614	1624	rVV6	1950	3580	0.24%	0.031%
36	6.690	1649	1664	1687	rBV	343974	670019	44.81%	5.821%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048442.D
 Acq On : 05 May 2022 17:10
 Operator : SY/MD
 Sample : N2710-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.800	1695	1698	1705	rBV2	1038	1291	0.09%	0.011%
38	6.861	1715	1717	1722	rVB2	394	220	0.01%	0.002%
39	7.041	1769	1773	1784	rVB4	477	679	0.05%	0.006%
40	7.134	1798	1802	1805	rBV2	345	197	0.01%	0.002%
41	7.179	1805	1816	1829	rVV5	4661	9542	0.64%	0.083%
42	7.227	1829	1831	1834	rVV2	288	192	0.01%	0.002%
43	7.366	1869	1874	1881	rVB3	323	319	0.02%	0.003%
44	7.411	1881	1888	1892	rBV3	193	277	0.02%	0.002%
45	7.504	1912	1917	1922	rBV2	182	260	0.02%	0.002%
46	7.565	1922	1936	1955	rBV	180205	312354	20.89%	2.714%
47	7.636	1955	1958	1962	rVB3	310	241	0.02%	0.002%
48	7.687	1967	1974	1987	rBV2	2417	4206	0.28%	0.037%
49	7.800	2006	2009	2015	rVB3	583	441	0.03%	0.004%
50	7.896	2025	2039	2056	rBV	689003	1192571	79.77%	10.361%
51	8.134	2107	2113	2114	rBV2	228	228	0.02%	0.002%
52	8.179	2115	2127	2146	rVV	126047	208047	13.92%	1.808%
53	8.308	2165	2167	2169	rBV2	331	185	0.01%	0.002%
54	8.333	2173	2175	2179	rVB3	850	478	0.03%	0.004%
55	8.407	2196	2198	2204	rVB3	302	256	0.02%	0.002%
56	8.469	2212	2217	2226	rVB4	1196	1914	0.13%	0.017%
57	8.552	2232	2243	2256	rBV	86664	144794	9.68%	1.258%
58	8.636	2256	2269	2302	rBV2	517072	977322	65.37%	8.491%
59	8.825	2326	2328	2334	rVB3	309	300	0.02%	0.003%
60	8.864	2338	2340	2345	rVB2	448	277	0.02%	0.002%
61	8.935	2357	2362	2365	rBV4	596	608	0.04%	0.005%
62	9.028	2388	2391	2395	rVV3	375	250	0.02%	0.002%
63	9.157	2429	2431	2433	rBV2	509	246	0.02%	0.002%
64	9.237	2453	2456	2462	rVB2	392	277	0.02%	0.002%
65	9.285	2462	2471	2477	rBV2	197	338	0.02%	0.003%
66	9.314	2477	2480	2483	rBV2	216	183	0.01%	0.002%
67	9.417	2498	2512	2537	rBV	555234	918131	61.41%	7.977%
68	9.571	2553	2560	2565	rVB4	422	627	0.04%	0.005%
69	9.632	2573	2579	2580	rBV	323	313	0.02%	0.003%
70	9.690	2591	2597	2599	rBV2	640	643	0.04%	0.006%
71	10.102	2718	2725	2730	rBV2	321	376	0.03%	0.003%
72	10.292	2779	2784	2787	rBV	237	209	0.01%	0.002%
73	10.484	2838	2844	2846	rBV3	295	330	0.02%	0.003%
74	10.533	2856	2859	2863	rBV2	265	183	0.01%	0.002%
75	10.668	2894	2901	2909	rBV5	1523	2262	0.15%	0.020%
76	10.758	2915	2929	2953	rBV	576448	922503	61.70%	8.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048442.D
 Acq On : 05 May 2022 17:10
 Operator : SY/MD
 Sample : N2710-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.867	2960	2963	2964	rBV2	488	274	0.02%	0.002%
78	10.893	2964	2971	2984	rVB3	3965	6575	0.44%	0.057%
79	11.092	3031	3033	3036	rBV2	361	261	0.02%	0.002%
80	11.118	3036	3041	3045	rVV4	655	693	0.05%	0.006%
81	11.140	3045	3048	3051	rVB2	322	199	0.01%	0.002%
82	11.285	3090	3093	3096	rBV	274	183	0.01%	0.002%
83	11.343	3108	3111	3113	rBV	261	185	0.01%	0.002%
84	11.385	3121	3124	3128	rBV3	254	189	0.01%	0.002%
85	11.465	3142	3149	3157	rVB4	1119	1769	0.12%	0.015%
86	11.571	3179	3182	3184	rBV	299	236	0.02%	0.002%
87	11.629	3196	3200	3202	rBV2	445	320	0.02%	0.003%
88	11.812	3244	3257	3277	rBV	548614	864669	57.83%	7.512%
89	12.195	3362	3376	3396	rBV	655695	1078977	72.17%	9.374%
90	12.333	3416	3419	3428	rVB4	660	819	0.05%	0.007%
91	12.735	3541	3544	3547	rBV3	335	255	0.02%	0.002%
92	12.774	3547	3556	3568	rVV	1625	2738	0.18%	0.024%
93	13.867	3891	3896	3900	rBV	2003	1986	0.13%	0.017%
94	13.918	3908	3912	3915	rBV2	1324	1057	0.07%	0.009%
95	14.057	3950	3955	3962	rBV2	1657	2205	0.15%	0.019%
96	14.115	3970	3973	3982	rVB3	659	632	0.04%	0.005%
97	14.163	3984	3988	3991	rBV2	856	902	0.06%	0.008%
98	14.217	4001	4005	4008	rBV	1008	671	0.04%	0.006%
99	14.494	4088	4091	4094	rBV	803	452	0.03%	0.004%
100	14.809	4187	4189	4194	rVB3	690	367	0.02%	0.003%




Sum of corrected areas: 11510057

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048442.D
Acq On : 05 May 2022 17:10
Operator : SY/MD
Sample : N2710-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

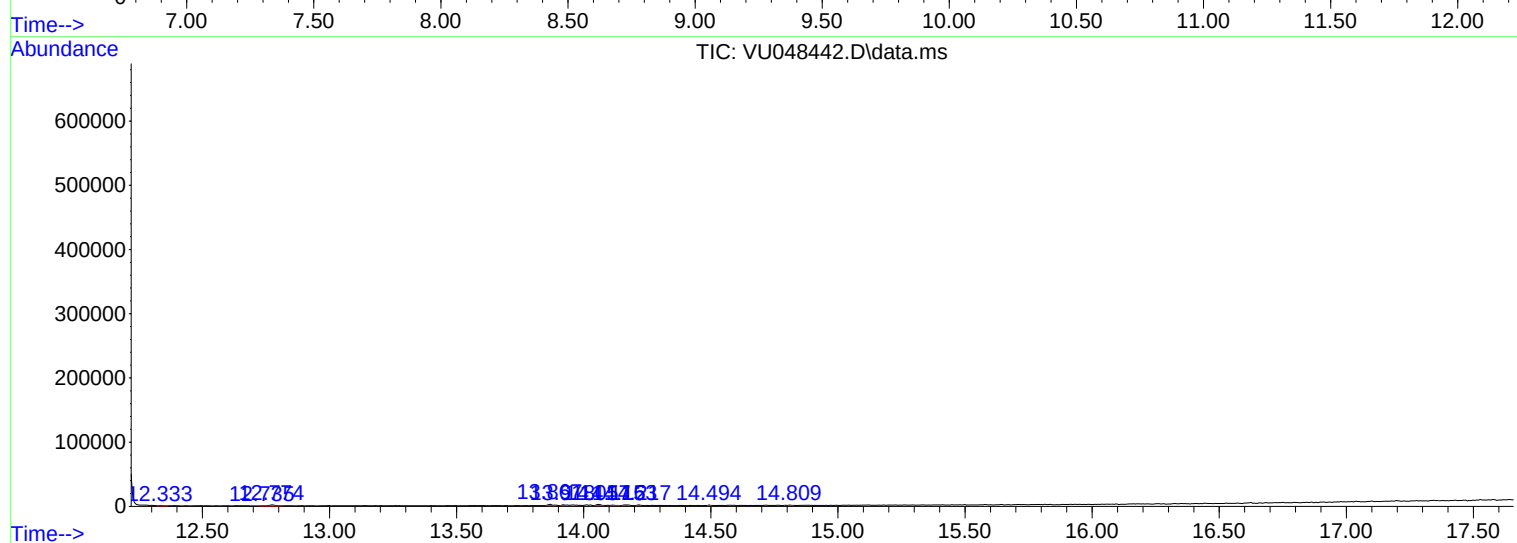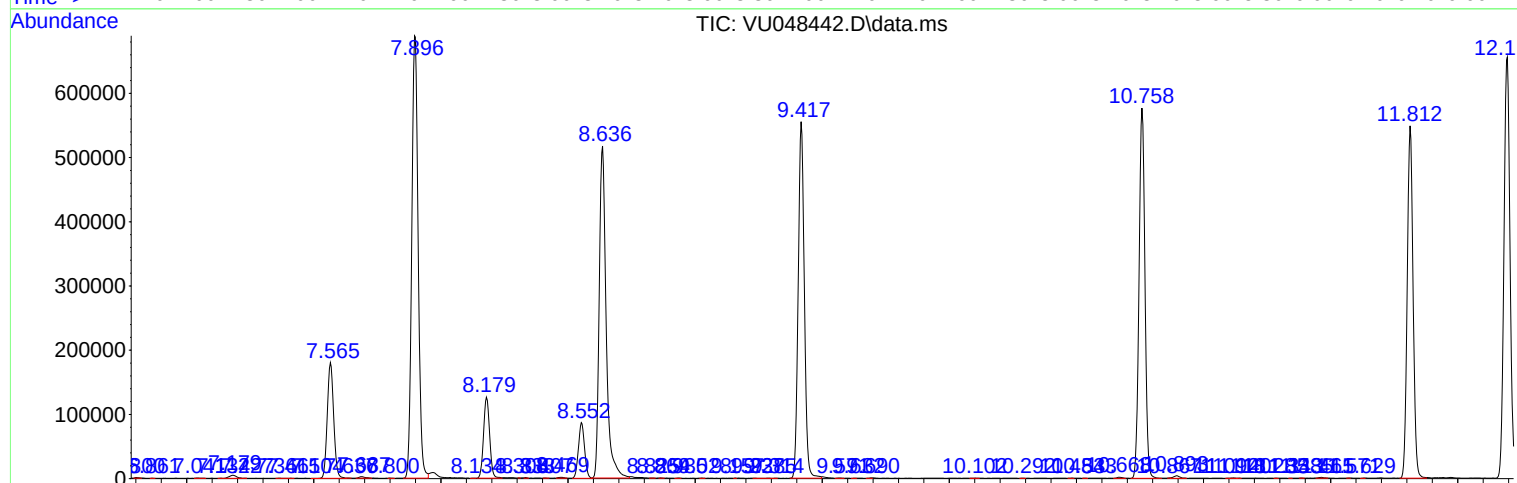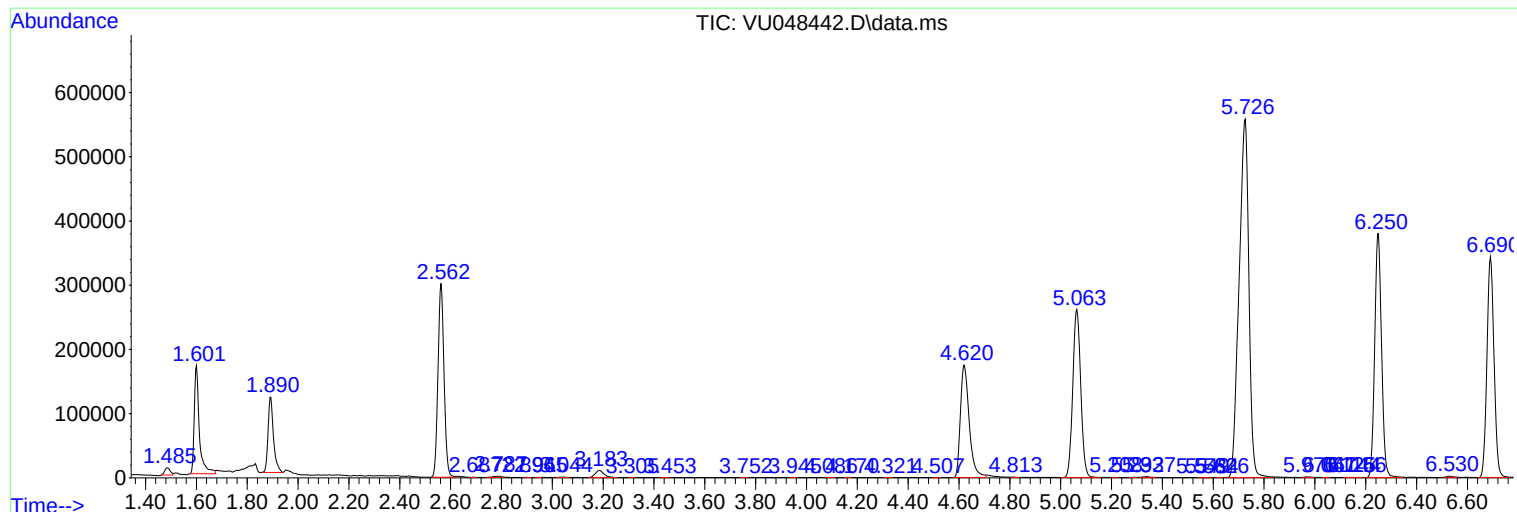

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048442.D
Acq On : 05 May 2022 17:10
Operator : SY/MD
Sample : N2710-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048442.D
Acq On : 05 May 2022 17:10
Operator : SY/MD
Sample : N2710-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------