

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048443.D
 Acq On : 05 May 2022 17:34
 Operator : SY/MD
 Sample : N2714-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	38	45	53	rBV2	9768	14771	0.96%	0.127%
2	1.601	73	81	105	rBV	170612	236221	15.32%	2.024%
3	1.893	164	172	186	rVB	119025	173861	11.28%	1.490%
4	2.517	363	366	367	rBV	489	290	0.02%	0.002%
5	2.562	367	380	395	rVV	307887	505877	32.81%	4.335%
6	2.726	428	431	435	rVB2	290	186	0.01%	0.002%
7	2.832	462	464	470	rVB4	392	347	0.02%	0.003%
8	2.874	473	477	481	rBV2	203	203	0.01%	0.002%
9	2.925	490	493	496	rVB3	247	192	0.01%	0.002%
10	2.948	496	500	503	rBV3	315	275	0.02%	0.002%
11	2.967	503	506	507	rBV	347	178	0.01%	0.002%
12	3.044	524	530	538	rVB4	1004	1326	0.09%	0.011%
13	3.102	543	548	553	rVB2	385	417	0.03%	0.004%
14	3.131	553	557	562	rBV	205	229	0.01%	0.002%
15	3.182	562	573	591	rVB3	3517	9024	0.59%	0.077%
16	3.359	625	628	632	rBV	126	129	0.01%	0.001%
17	3.379	632	634	639	rVB	246	137	0.01%	0.001%
18	3.411	640	644	646	rBV2	195	145	0.01%	0.001%
19	3.764	750	754	758	rVB2	199	184	0.01%	0.002%
20	3.790	758	762	765	rBV2	172	150	0.01%	0.001%
21	3.989	821	824	826	rBV	222	182	0.01%	0.002%
22	4.012	826	831	843	rVV2	431	704	0.05%	0.006%
23	4.141	864	871	876	rBV2	142	239	0.02%	0.002%
24	4.430	956	961	964	rBV2	132	129	0.01%	0.001%
25	4.620	1004	1020	1039	rBV	178641	420849	27.30%	3.606%
26	4.858	1092	1094	1100	rVB3	386	257	0.02%	0.002%
27	4.944	1116	1121	1123	rBV3	286	259	0.02%	0.002%
28	5.063	1141	1158	1181	rBV	270864	591329	38.36%	5.067%
29	5.208	1201	1203	1207	rBV3	402	235	0.02%	0.002%
30	5.263	1216	1220	1222	rBV	179	159	0.01%	0.001%
31	5.314	1234	1236	1237	rBV	360	153	0.01%	0.001%
32	5.330	1237	1241	1253	rVB2	1039	1690	0.11%	0.014%
33	5.517	1295	1299	1300	rBV	402	264	0.02%	0.002%
34	5.726	1342	1364	1401	rBV2	573879	1541613	100.00%	13.210%
35	5.912	1420	1422	1429	rVB2	419	405	0.03%	0.003%
36	5.967	1433	1439	1448	rVB4	1027	1412	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048443.D
 Acq On : 05 May 2022 17:34
 Operator : SY/MD
 Sample : N2714-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.038	1458	1461	1470	rVB3	399	486	0.03%	0.004%
38	6.108	1479	1483	1486	rBV3	365	317	0.02%	0.003%
39	6.247	1511	1526	1553	rBV	389371	747184	48.47%	6.402%
40	6.398	1571	1573	1576	rVB2	249	137	0.01%	0.001%
41	6.526	1605	1613	1625	rBV4	2664	4683	0.30%	0.040%
42	6.591	1631	1633	1638	rBV3	239	129	0.01%	0.001%
43	6.626	1641	1644	1647	rVB2	437	308	0.02%	0.003%
44	6.690	1648	1664	1686	rBV	357288	688472	44.66%	5.899%
45	6.784	1691	1693	1694	rBV2	611	246	0.02%	0.002%
46	6.928	1731	1738	1748	rBV3	450	861	0.06%	0.007%
47	7.179	1805	1816	1831	rVV6	4905	10134	0.66%	0.087%
48	7.349	1866	1869	1873	rVB2	214	136	0.01%	0.001%
49	7.565	1923	1936	1957	rBV	185573	319724	20.74%	2.740%
50	7.690	1966	1975	1984	rBV4	2524	4075	0.26%	0.035%
51	7.787	2000	2005	2008	rBV3	515	466	0.03%	0.004%
52	7.829	2014	2018	2022	rBV2	352	311	0.02%	0.003%
53	7.899	2025	2040	2057	rBV	703997	1224129	79.41%	10.489%
54	8.179	2115	2127	2144	rBV	129171	214341	13.90%	1.837%
55	8.385	2188	2191	2195	rBV2	340	278	0.02%	0.002%
56	8.446	2206	2210	2211	rBV3	320	182	0.01%	0.002%
57	8.552	2239	2243	2250	rBV3	1662	1906	0.12%	0.016%
58	8.636	2255	2269	2308	rBV2	528291	1005205	65.20%	8.613%
59	8.896	2348	2350	2354	rVB2	288	187	0.01%	0.002%
60	8.941	2361	2364	2366	rBV2	366	204	0.01%	0.002%
61	8.960	2367	2370	2373	rVV2	563	434	0.03%	0.004%
62	8.992	2377	2380	2383	rVV2	304	213	0.01%	0.002%
63	9.009	2383	2385	2389	rVB	246	165	0.01%	0.001%
64	9.038	2389	2394	2397	rBV2	135	161	0.01%	0.001%
65	9.079	2405	2407	2412	rVB3	359	261	0.02%	0.002%
66	9.169	2426	2435	2439	rBV2	497	645	0.04%	0.006%
67	9.314	2477	2480	2487	rVV2	311	236	0.02%	0.002%
68	9.343	2487	2489	2494	rBV	230	190	0.01%	0.002%
69	9.417	2499	2512	2550	rVV	569903	948250	61.51%	8.125%
70	9.571	2556	2560	2564	rBV2	712	552	0.04%	0.005%
71	9.645	2580	2583	2586	rBV	250	187	0.01%	0.002%
72	9.690	2591	2597	2608	rVB3	1718	2684	0.17%	0.023%
73	9.835	2639	2642	2645	rBV2	191	130	0.01%	0.001%
74	10.105	2720	2726	2729	rBV2	937	972	0.06%	0.008%
75	10.121	2729	2731	2732	rBV2	428	155	0.01%	0.001%
76	10.279	2775	2780	2784	rBV2	274	236	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048443.D
 Acq On : 05 May 2022 17:34
 Operator : SY/MD
 Sample : N2714-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.671	2894	2902	2910	rVB4	1481	1810	0.12%	0.016%
78	10.758	2916	2929	2951	rBV	592124	950736	61.67%	8.147%
79	10.893	2963	2971	2979	rBV2	2151	3194	0.21%	0.027%
80	10.999	3002	3004	3007	rVB	227	135	0.01%	0.001%
81	11.092	3030	3033	3037	rVB2	497	471	0.03%	0.004%
82	11.118	3039	3041	3045	rVB2	657	406	0.03%	0.003%
83	11.147	3049	3050	3054	rVB2	287	139	0.01%	0.001%
84	11.237	3073	3078	3080	rVB2	328	262	0.02%	0.002%
85	11.259	3080	3085	3087	rBV	183	162	0.01%	0.001%
86	11.410	3127	3132	3135	rBV3	600	479	0.03%	0.004%
87	11.433	3136	3139	3140	rVV	403	237	0.02%	0.002%
88	11.465	3141	3149	3160	rVB6	1553	3086	0.20%	0.026%
89	11.581	3181	3185	3188	rBV	427	269	0.02%	0.002%
90	11.690	3215	3219	3224	rBV2	522	456	0.03%	0.004%
91	11.745	3229	3236	3244	rBV6	3523	4819	0.31%	0.041%
92	11.812	3244	3257	3279	rBV	574297	903947	58.64%	7.746%
93	11.889	3279	3281	3284	rBV3	586	365	0.02%	0.003%
94	12.195	3362	3376	3396	rBV	688219	1112220	72.15%	9.530%
95	12.423	3445	3447	3449	rBV2	283	185	0.01%	0.002%
96	12.459	3454	3458	3461	rVB2	334	264	0.02%	0.002%
97	12.770	3550	3555	3563	rVB2	1396	1846	0.12%	0.016%
98	12.906	3595	3597	3600	rVB2	303	166	0.01%	0.001%
99	13.008	3621	3629	3633	rBV2	519	827	0.05%	0.007%
100	13.079	3648	3651	3657	rBV2	336	360	0.02%	0.003%




Sum of corrected areas: 11670434

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048443.D
Acq On : 05 May 2022 17:34
Operator : SY/MD
Sample : N2714-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

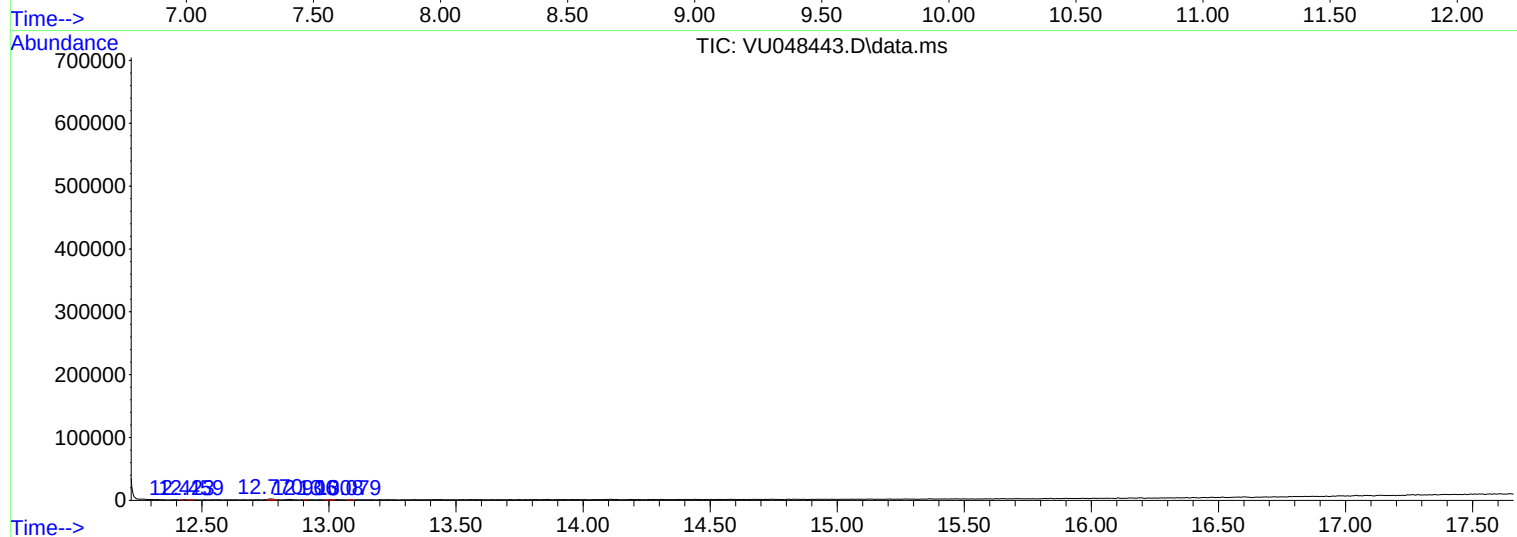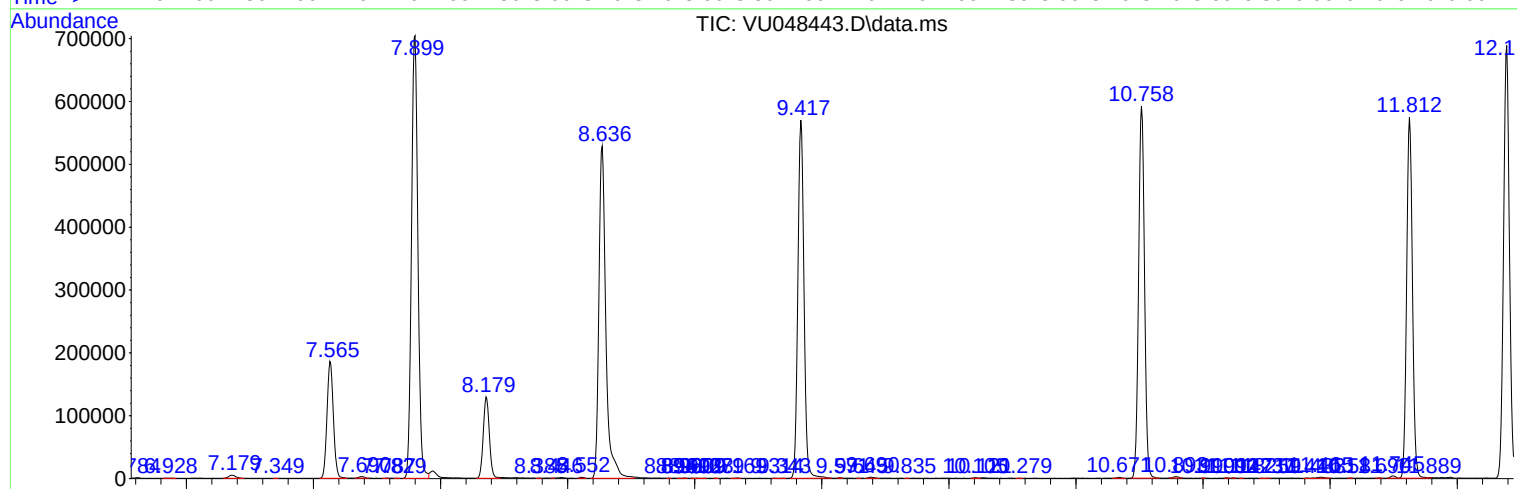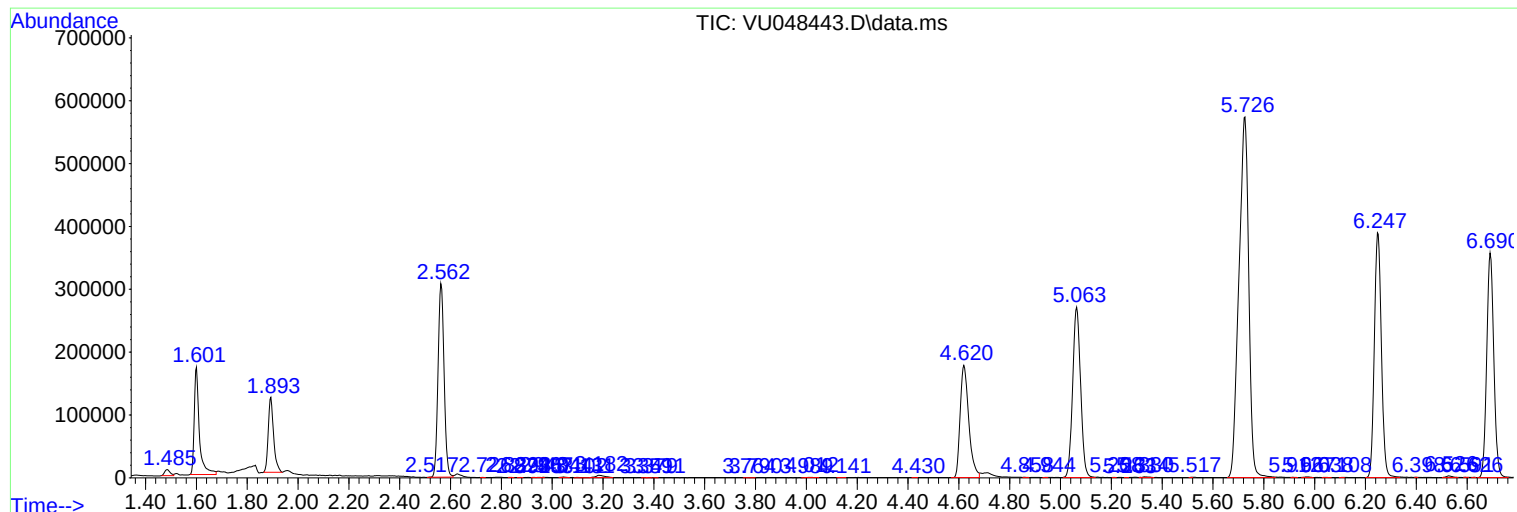

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048443.D
Acq On : 05 May 2022 17:34
Operator : SY/MD
Sample : N2714-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
Data File : VU048443.D
Acq On : 05 May 2022 17:34
Operator : SY/MD
Sample : N2714-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------