


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050522\
 Data File : VU048427.D
 Acq On : 05 May 2022 08:59
 Operator : SY/MD
 Sample : BFB080
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB080

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis
 Last Update : Fri May 06 05:30:23 2022

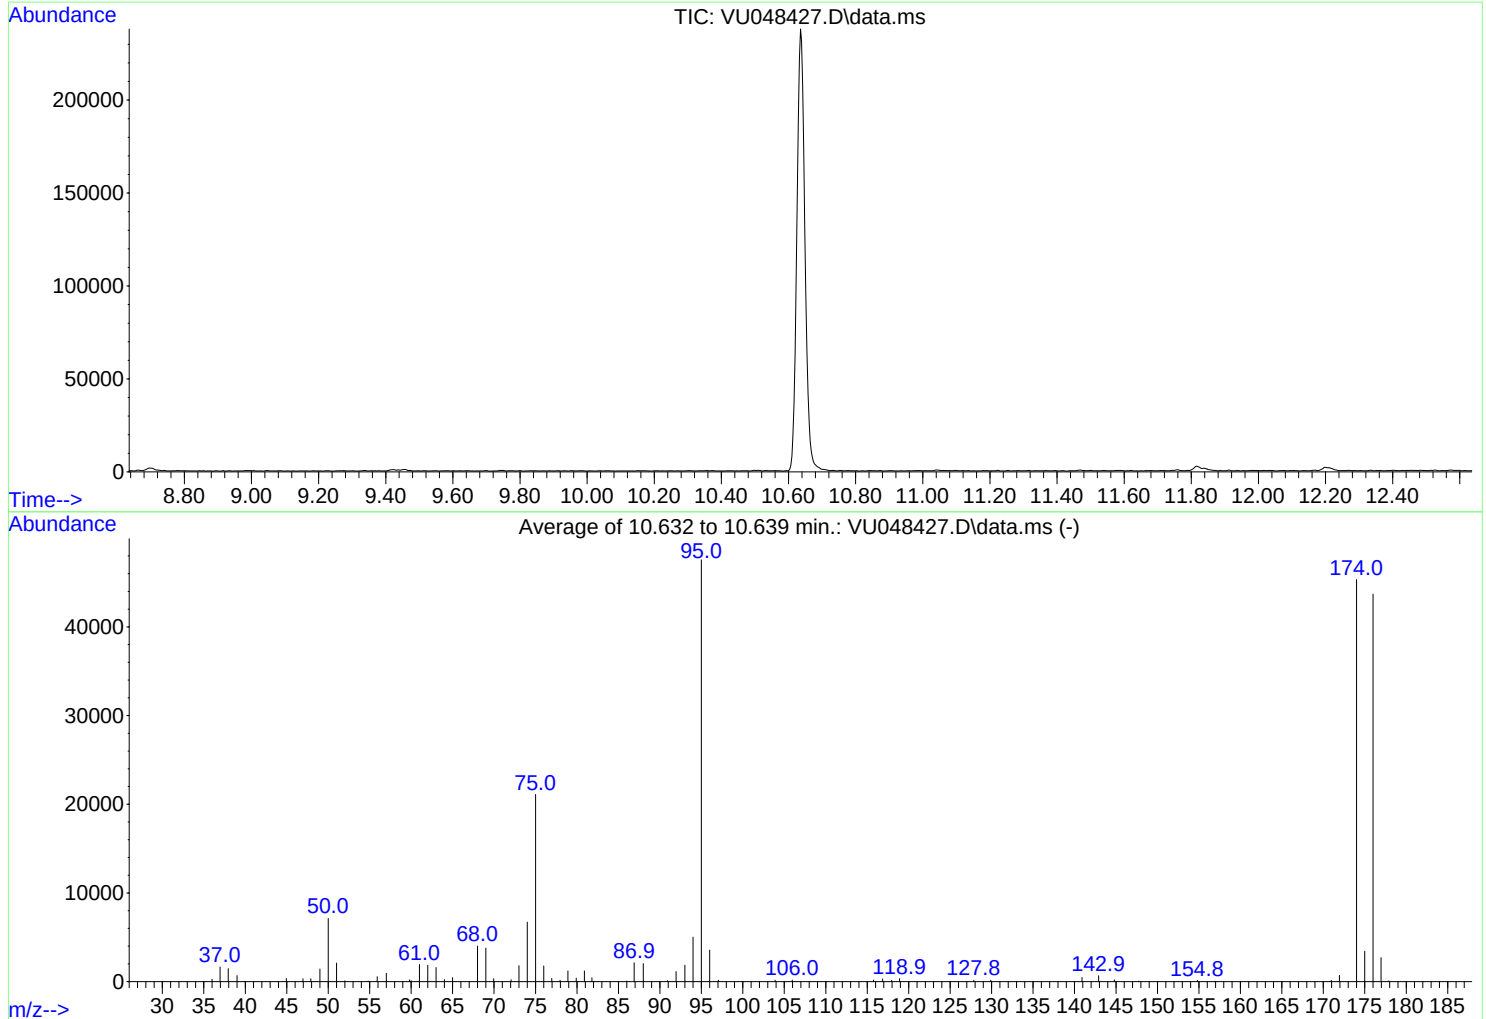

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	7134	PASS
75	95	30	80	44.4	21104	PASS
95	95	100	100	100.0	47555	PASS
96	95	5	9	7.5	3548	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	95.3	45336	PASS
175	174	5	9	7.6	3429	PASS
176	174	95	101	96.4	43685	PASS
177	176	5	9	6.2	2714	PASS

m/z	Abundance
39.80	227.0
43.90	472.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
36.00	247.0
37.00	1530.0
37.90	1464.0
39.00	653.0
39.90	252.0
44.00	538.0
44.90	369.0
46.90	351.0
47.90	392.0
49.00	1360.0
50.00	7067.0
51.00	1983.0
52.00	133.0
54.80	106.0
55.90	540.0
57.00	932.0
59.80	284.0
61.00	1758.0
62.00	1898.0
63.00	1568.0
64.00	289.0
65.00	387.0
68.00	3963.0
69.00	3700.0
69.90	338.0
72.10	211.0
73.00	1739.0
74.00	6334.0
75.00	20648.0
76.00	1690.0
77.00	344.0
78.10	147.0
78.90	1228.0
80.00	445.0
80.90	1100.0
81.80	377.0
86.00	113.0
86.90	2104.0
88.00	2055.0
91.90	1131.0
93.00	1728.0
94.00	4723.0
95.00	46480.0
96.00	3592.0
97.10	127.0
103.90	161.0
105.90	182.0
115.80	172.0
116.90	315.0
118.00	139.0
118.90	290.0
127.80	168.0
129.90	170.0
140.90	478.0
142.90	665.0
144.80	169.0
147.80	108.0
154.80	130.0
156.90	112.0
170.90	122.0
171.90	636.0
174.00	42992.0
175.00	3419.0
176.00	41000.0
177.00	2641.0
177.90	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
36.00	279.0
36.90	1714.0
38.00	1512.0
39.00	714.0
39.90	272.0
43.90	449.0
45.00	394.0
47.00	322.0
47.90	336.0
49.00	1483.0
50.00	7398.0
51.00	2157.0
52.00	127.0
54.80	110.0
55.90	587.0
57.00	955.0
59.80	298.0
61.00	2026.0
62.00	1892.0
63.00	1633.0
64.00	242.0
65.00	447.0
68.00	4122.0
69.00	3880.0
70.00	338.0
72.00	226.0
73.00	1820.0
74.00	6900.0
75.00	21664.0
76.00	1840.0
76.90	377.0
77.90	164.0
78.90	1233.0
79.90	390.0
80.90	1238.0
81.80	475.0
86.00	110.0
86.90	2154.0
88.00	2121.0
90.90	141.0
92.00	1144.0
93.00	1884.0
94.00	5187.0
95.00	49152.0
96.00	3693.0
97.10	179.0
103.90	171.0
105.90	184.0
115.70	191.0
116.90	299.0
117.90	140.0
118.90	356.0
127.90	169.0
129.90	157.0
140.90	486.0
142.90	722.0
144.80	201.0
147.70	119.0
154.80	141.0
171.00	144.0
172.00	711.0
174.00	46728.0
175.00	3563.0
176.00	45064.0
177.00	2762.0
177.90	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
36.00	279.0
36.90	1732.0
38.00	1428.0
39.00	679.0
39.90	266.0
43.90	433.0
45.00	348.0
47.00	308.0
47.90	240.0
49.00	1451.0
50.00	6937.0
51.00	2167.0
55.90	549.0
57.00	903.0
60.00	335.0
61.00	2024.0
62.00	1742.0
63.00	1562.0
64.00	193.0
65.00	519.0
68.00	3953.0
69.00	3808.0
70.00	284.0
72.00	224.0
73.00	1830.0
74.00	6888.0
75.00	21000.0
76.00	1788.0
76.90	388.0
77.90	192.0
78.90	1149.0
79.80	341.0
80.90	1288.0
81.80	439.0
86.90	2133.0
88.00	1929.0
90.90	190.0
92.00	1146.0
93.00	1938.0
94.00	5130.0
95.00	47032.0
96.00	3360.0
97.00	178.0
103.90	156.0
106.00	176.0
115.70	189.0
116.80	314.0
117.90	143.0
118.90	371.0
127.90	156.0
129.90	153.0
140.90	442.0
142.90	635.0
144.80	216.0
154.80	143.0
171.00	144.0
172.00	753.0
174.00	46288.0
175.00	3305.0
176.00	44992.0
176.90	2740.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080