

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050618\
 Data File : VU023696.D
 Acq On : 06 May 2018 18:08
 Operator : MD/SY
 Sample : J2721-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: May 07 02:20:42 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 07 00:51:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	372284	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	351713	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	173385	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	112156	42.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.02%
7) Chloroethane-d5	1.68	69	91634	45.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.12%
11) 1,1-Dichloroethene-d2	2.27	63	167075	32.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.96%
21) 2-Butanone-d5	4.18	46	197277	108.22	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.22%
24) Chloroform-d	4.65	84	209233	47.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.90%
26) 1,2-Dichloroethane-d4	5.31	65	138750	45.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.44%
32) Benzene-d6	5.35	84	451093	47.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.34	67	154224	48.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.58%
41) Toluene-d8	7.57	98	401831	46.19	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.38%
43) trans-1,3-Dichloropropene-	7.85	79	61295	45.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.10%
47) 2-Hexanone-d5	8.31	63	143669	119.69	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	119.69%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	199792	48.87	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.74%
64) 1,2-Dichlorobenzene-d4	11.86	152	169407	50.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.16%


Target Compounds					Ovalue
13) Acetone	2.32	43	10938	4.04 ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050618\
Data File : VU023696.D
Acq On : 06 May 2018 18:08
Operator : MD/SY
Sample : J2721-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: May 07 02:20:42 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 07 00:51:10 2018
Response via : Initial Calibration

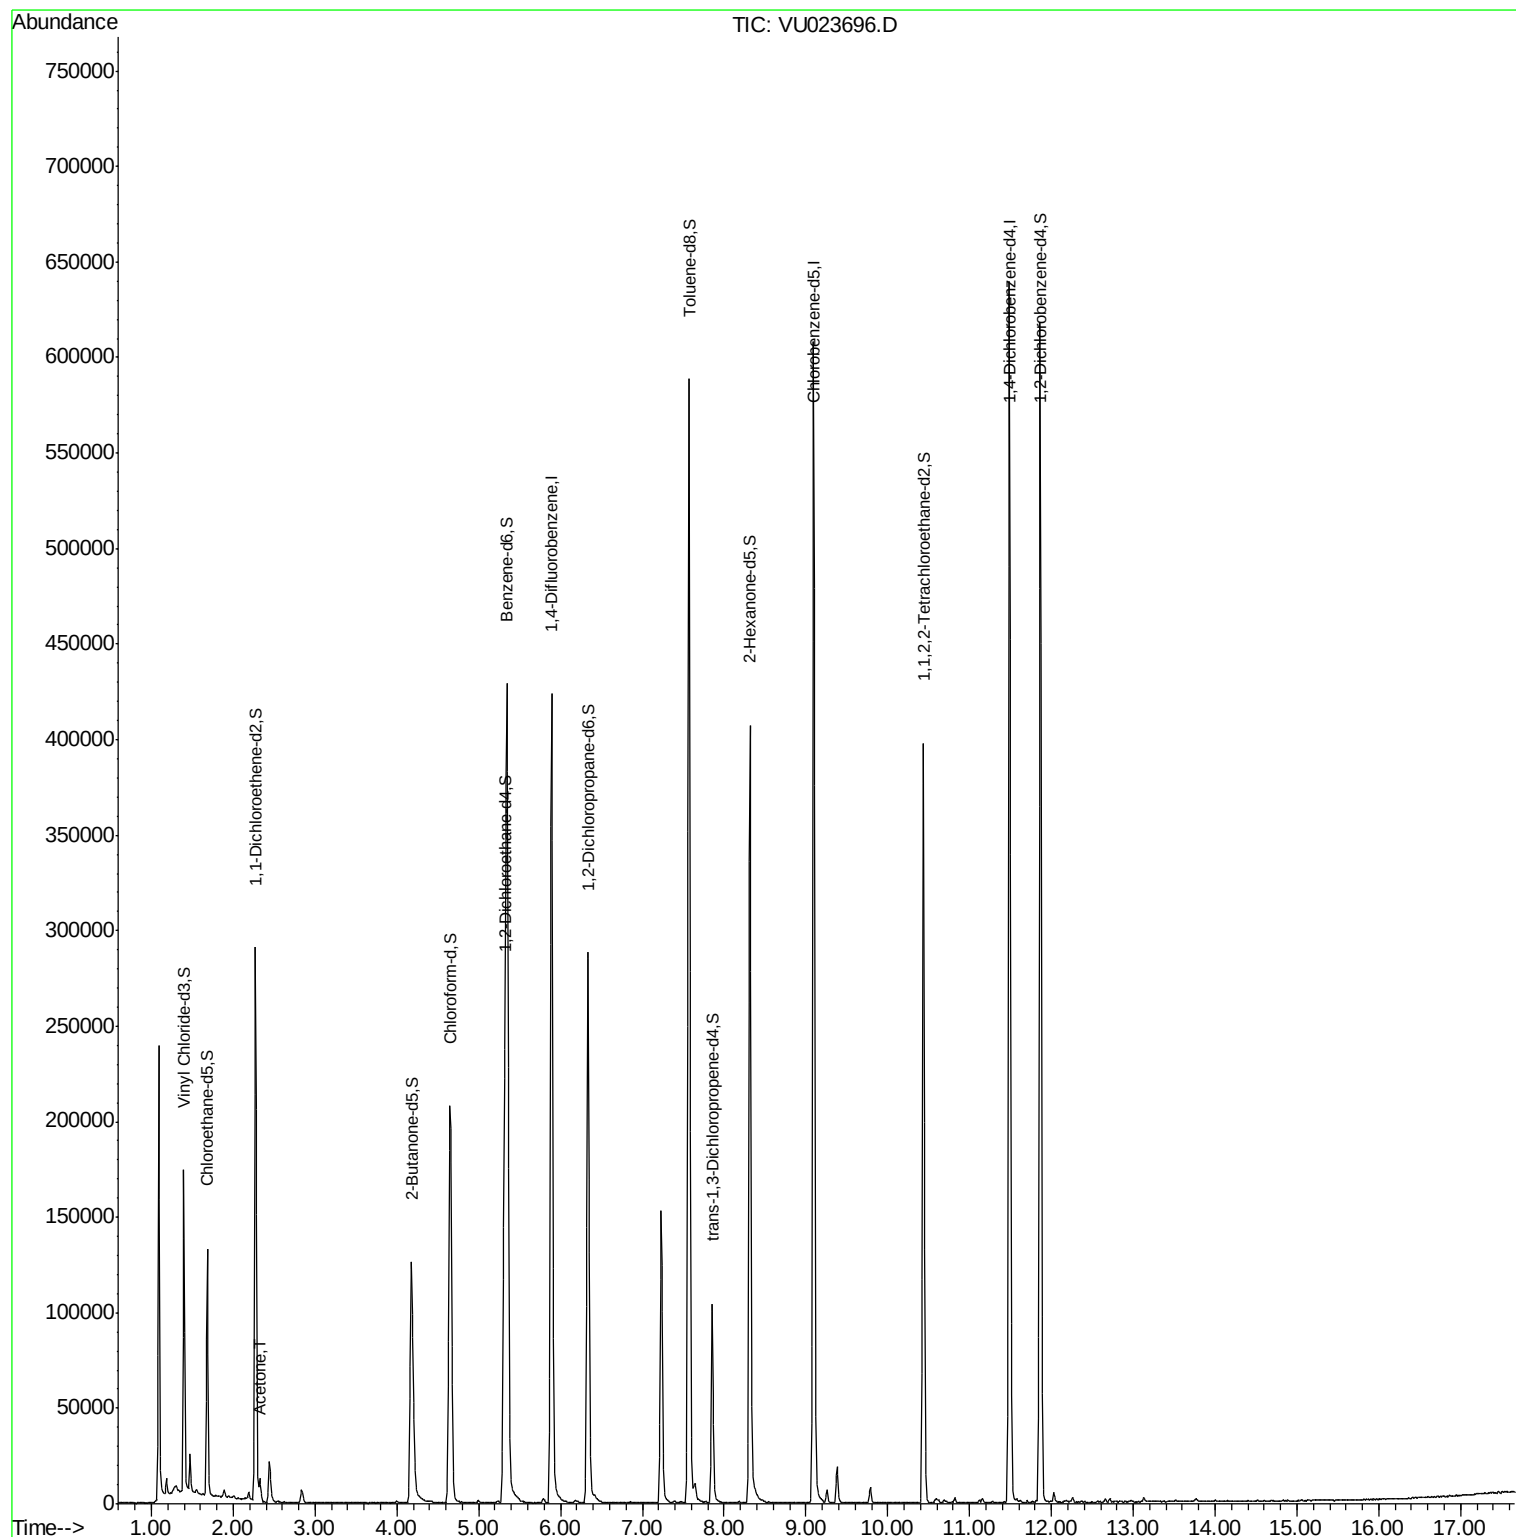

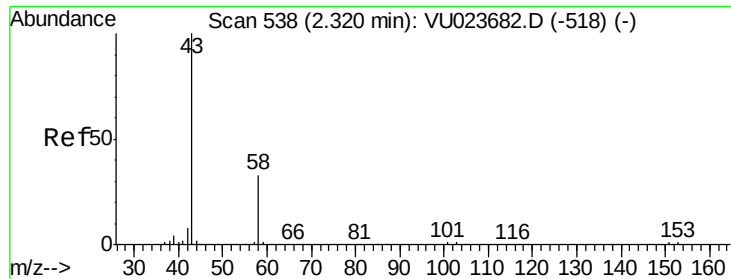

#13

Acetone

Concen: 4.04 ug/L

RT: 2.32 min Scan# 538

Delta R.T. 0.00 min

Lab File: VU023696.D

Acq: 06 May 2018 18:08

Tot Ion: 43 Resp: 10938

Ion Ratio Lower Upper

43 100

58 34.1 0.0 64.8

