


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050618\
 Data File : VU023681.D
 Acq On : 06 May 2018 09:49
 Operator : MD/SY
 Sample : BFB48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Title : VOC Analysis
 Last Update : Mon May 07 00:51:10 2018

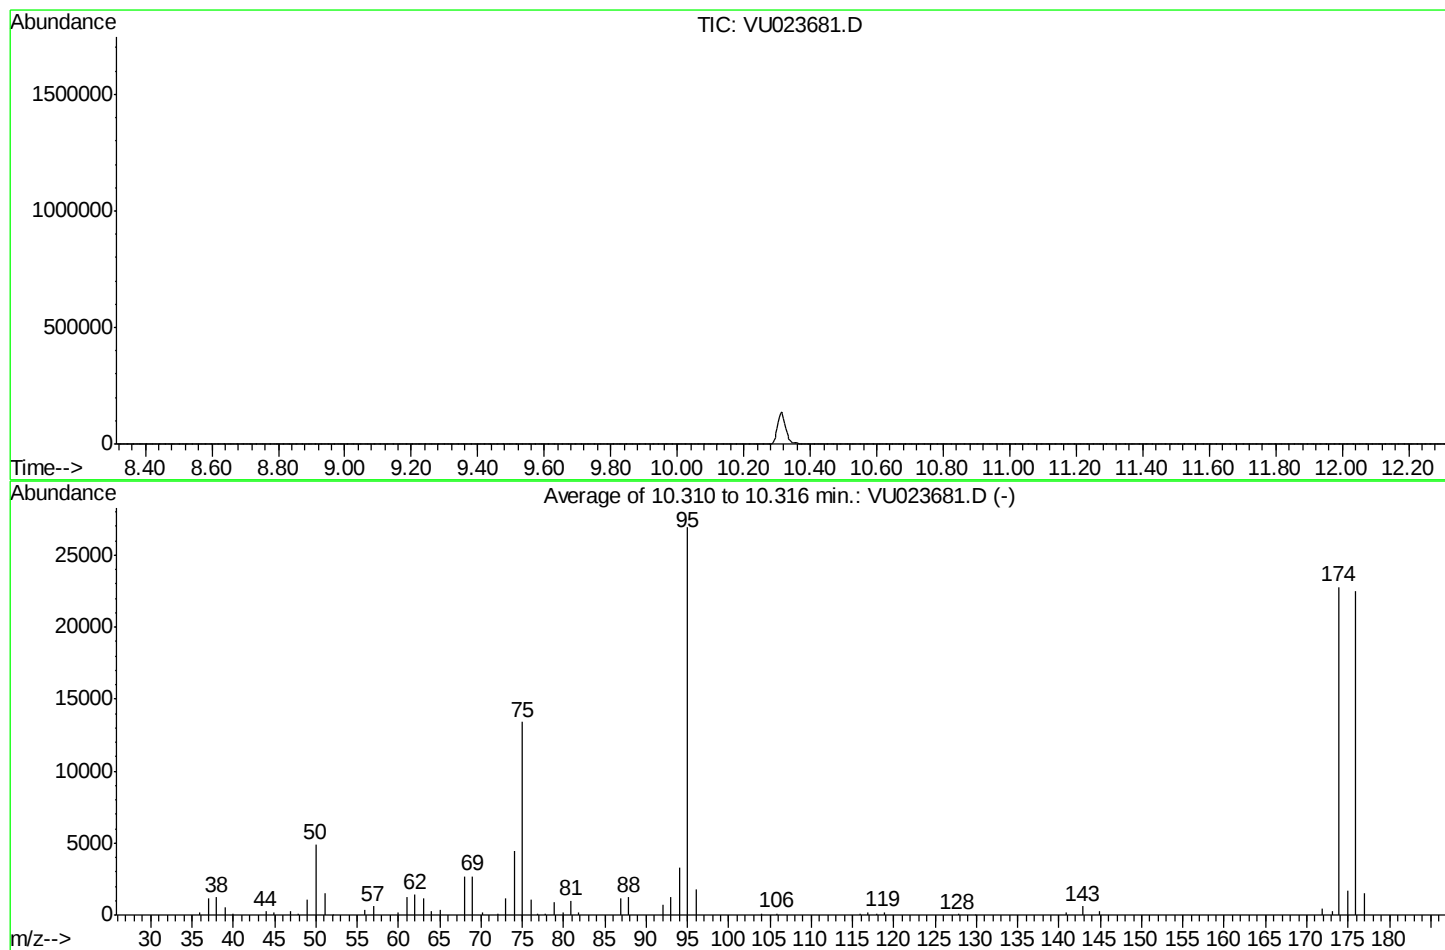

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	4878	PASS
75	95	30	80	49.8	13418	PASS
95	95	100	100	100.0	26938	PASS
96	95	5	9	6.6	1772	PASS
173	174	0.00	2	1.1	255	PASS
174	95	50	120	84.6	22792	PASS
175	174	5	9	7.4	1682	PASS
176	174	95	101	98.7	22488	PASS
177	176	5	9	6.9	1542	PASS

Scan 3011 (10.271 min): VU023681.D
BFB48

m/z	Abundance
40.00	135.0
43.90	379.0

m/z	Abundance
35.90	212.0
37.00	1217.0
38.00	1264.0
39.00	517.0
40.00	174.0
44.00	586.0
44.90	200.0
47.00	271.0
47.80	131.0
49.00	1046.0
50.00	5012.0
51.00	1600.0
52.00	114.0
55.90	339.0
57.00	610.0
59.90	194.0
61.00	1240.0
62.00	1433.0
63.00	1164.0
64.10	293.0
65.00	386.0
68.00	2580.0
69.00	2780.0
70.10	185.0
72.00	128.0
73.00	1216.0
74.00	4422.0
75.00	13419.0
76.00	1039.0
76.80	140.0
77.80	136.0
78.90	907.0
79.90	213.0
80.90	989.0
81.80	220.0
86.90	1184.0
87.90	1176.0
92.00	722.0
92.90	1246.0
94.00	3219.0
95.00	27128.0
96.00	1902.0
104.00	101.0
105.90	125.0
116.90	170.0
117.90	113.0
118.90	225.0
129.80	105.0
140.80	215.0
142.90	563.0
144.80	307.0
171.90	466.0
173.00	247.0
173.90	22400.0
174.90	1720.0
175.90	22312.0
176.90	1534.0

Scan 3024 (10.313 min): VU023681.D
BFB48

m/z	Abundance
35.90	183.0
37.00	1232.0
38.00	1275.0
39.00	523.0
40.00	191.0
44.00	620.0
44.90	179.0
47.00	282.0
47.80	133.0
49.00	1079.0
50.00	5063.0
51.00	1532.0
55.90	384.0
57.00	614.0
59.90	178.0
61.00	1286.0
62.00	1466.0
63.10	1243.0
64.10	251.0
65.00	361.0
68.00	2761.0
69.00	2776.0
70.10	198.0
72.00	138.0
73.00	1246.0
74.00	4546.0
75.00	13856.0
76.00	1072.0
76.80	123.0
77.80	118.0
78.90	950.0
79.90	192.0
80.90	1014.0
81.80	221.0
86.90	1190.0
87.90	1305.0
92.00	747.0
92.90	1331.0
94.00	3431.0
95.00	27816.0
96.00	1828.0
104.00	111.0
105.80	123.0
116.00	117.0
116.90	173.0
117.90	121.0
118.80	212.0
127.80	103.0
140.80	226.0
142.90	652.0
144.90	317.0
171.90	474.0
173.00	257.0
173.90	23512.0
174.90	1707.0
175.90	23240.0
176.90	1574.0

Scan 3025 (10.316 min): VU023681.D
BFB48

m/z	Abundance
35.90	188.0
37.00	1137.0
38.00	1156.0
38.90	518.0
40.00	184.0
44.00	645.0
45.00	165.0
46.90	273.0
47.90	111.0
49.00	996.0
50.00	4559.0
51.10	1389.0
56.00	409.0
57.00	608.0
60.00	161.0
61.00	1280.0
62.00	1331.0
63.00	1201.0
64.00	201.0
65.00	301.0
68.00	2645.0
69.00	2577.0
70.10	181.0
72.00	134.0
73.00	1100.0
74.00	4359.0
75.00	12980.0
76.00	1031.0
76.90	131.0
78.90	902.0
79.90	183.0
80.90	954.0
81.80	189.0
86.90	1096.0
87.90	1224.0
92.00	679.0
93.00	1232.0
94.00	3180.0
95.00	25872.0
96.00	1586.0
103.90	115.0
105.80	101.0
115.90	124.0
116.80	207.0
117.80	104.0
118.80	186.0
127.80	105.0
140.80	219.0
142.90	634.0
144.90	249.0
171.90	447.0
173.10	263.0
173.90	22464.0
174.90	1620.0
175.90	21912.0
176.90	1518.0