
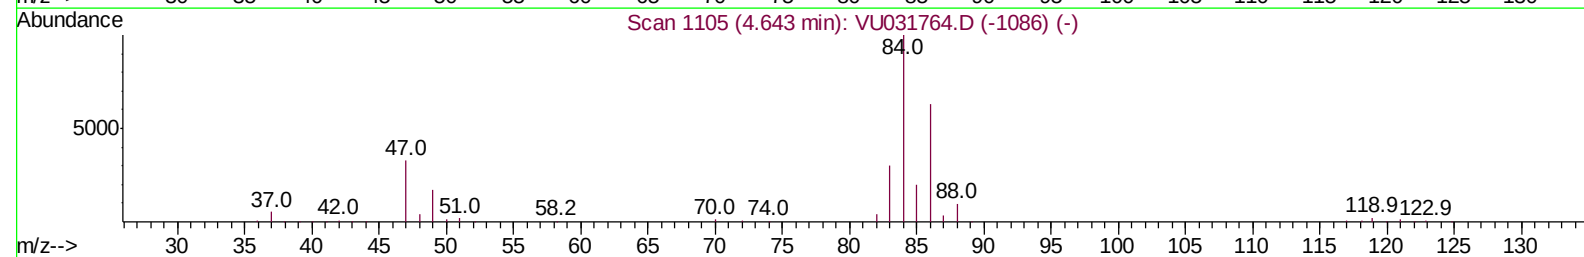
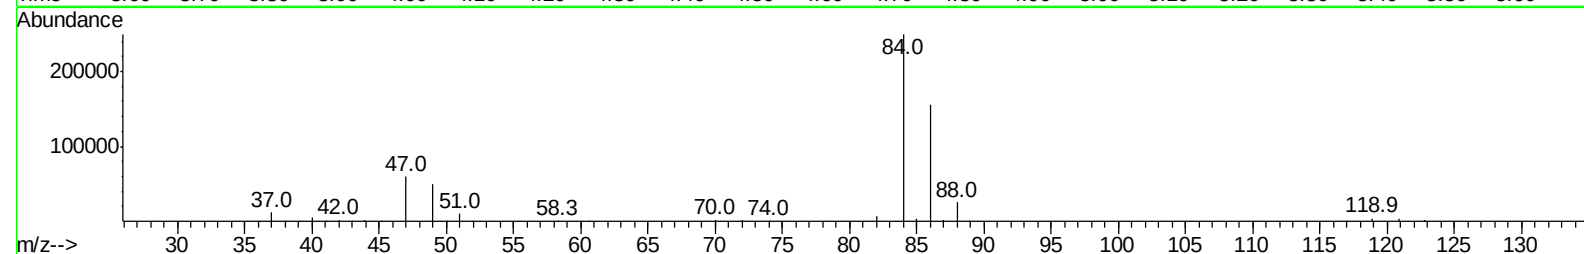


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU050619\
 Data File : VU031777.D
 Acq On : 06 May 2019 13:59
 Operator : JC/SP
 Sample : K2695-04 25X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: May 07 08:49:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 07 08:38:32 2019
 Response via : Initial Calibration

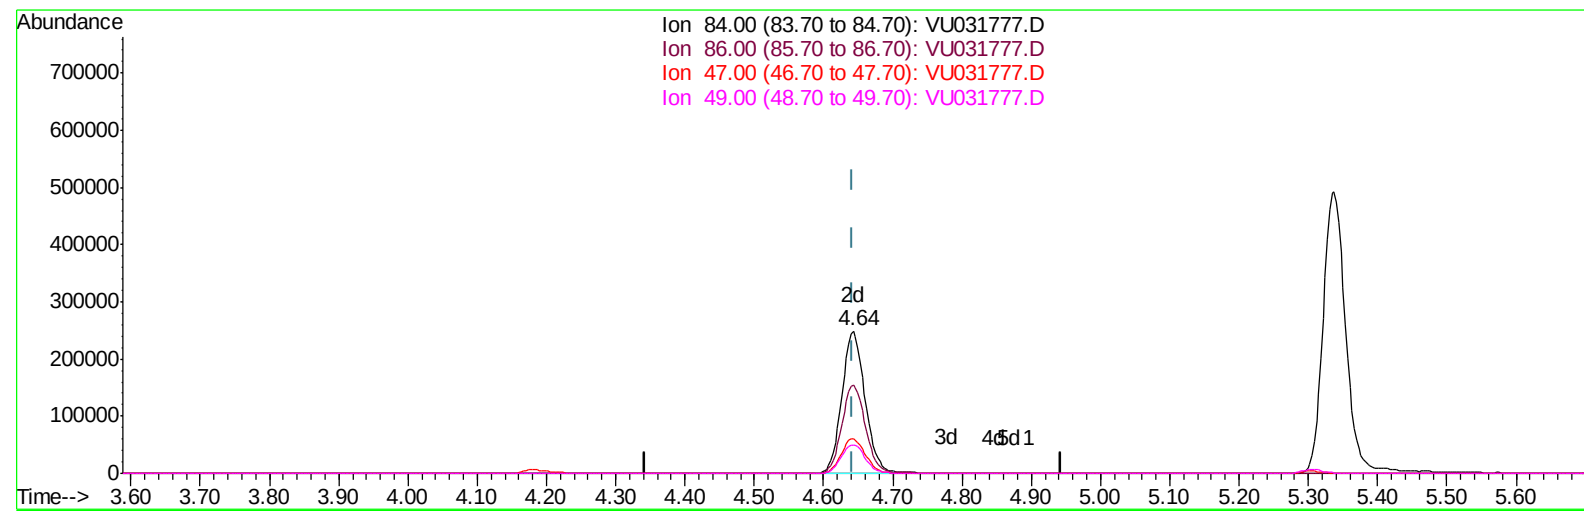

TIC: VU031777.D

(24) Chloroform-d (S)

4.643min (-0.000) 50.88ug/L m

response 572188

Ion	Exp%	Act%
84.00	100	100
86.00	62.50	0.03#
47.00	45.70	0.02#
49.00	27.20	0.01#