

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031768.D
 Acq On : 06 May 2019 10:29
 Operator : JC/SP
 Sample : K2690-25
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5169

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB5	18636	19067	0.56%	0.073%
2	1.395	88	95	107	rVB	441262	471736	13.95%	1.815%
3	1.678	176	183	200	rVB	359102	458794	13.56%	1.765%
4	2.270	356	367	378	rBV	728338	1117011	33.03%	4.298%
5	2.334	378	387	408	rVB	205912	420395	12.43%	1.618%
6	2.701	490	501	514	rVB	68357	119624	3.54%	0.460%
7	2.804	530	533	534	rBV3	1802	971	0.03%	0.004%
8	2.839	535	544	558	rVB2	7312	17579	0.52%	0.068%
9	2.929	569	572	582	rVB8	1293	1578	0.05%	0.006%
10	2.977	584	587	590	rBV2	1471	1093	0.03%	0.004%
11	3.074	614	617	625	rVB7	1908	2598	0.08%	0.010%
12	3.116	625	630	633	rBV3	1797	1539	0.05%	0.006%
13	3.202	654	657	665	rVB3	2078	2090	0.06%	0.008%
14	3.309	686	690	694	rBV4	1001	943	0.03%	0.004%
15	3.395	713	717	720	rBV2	1111	910	0.03%	0.004%
16	3.479	739	743	746	rBV2	1343	1260	0.04%	0.005%
17	3.624	785	788	793	rVB2	1686	1271	0.04%	0.005%
18	3.653	793	797	801	rBV3	2315	1857	0.05%	0.007%
19	3.698	808	811	815	rBV2	1386	995	0.03%	0.004%
20	3.778	832	836	839	rBV	2966	2214	0.07%	0.009%
21	3.804	839	844	851	rVV2	1882	2715	0.08%	0.010%
22	3.990	898	902	905	rBV2	1291	935	0.03%	0.004%
23	4.042	914	918	921	rBV3	1795	1208	0.04%	0.005%
24	4.183	947	962	982	rBV2	346793	1000519	29.58%	3.850%
25	4.643	1088	1105	1140	rBV	696507	1704614	50.40%	6.559%
26	5.144	1257	1261	1264	rBV3	1632	1368	0.04%	0.005%
27	5.202	1275	1279	1282	rVV3	1324	1327	0.04%	0.005%
28	5.334	1296	1320	1352	rBV2	1108916	3382265	100.00%	13.014%
29	5.714	1436	1438	1442	rVB3	1495	889	0.03%	0.003%
30	5.759	1448	1452	1455	rVB2	1154	1233	0.04%	0.005%
31	5.833	1472	1475	1477	rBV3	1596	1188	0.04%	0.005%
32	5.881	1477	1490	1531	rVV	881418	1866395	55.18%	7.181%
33	6.183	1574	1584	1594	rBV10	10246	21202	0.63%	0.082%
34	6.328	1614	1629	1652	rBV	772662	1589943	47.01%	6.117%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031768.D
 Acq On : 06 May 2019 10:29
 Operator : JC/SP
 Sample : K2690-25
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5169

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.707	1744	1747	1751	rVB4	1298	1060	0.03%	0.004%
36	6.742	1754	1758	1762	rVB4	1475	1026	0.03%	0.004%
37	6.797	1765	1775	1777	rBV4	2172	1926	0.06%	0.007%
38	6.845	1785	1790	1793	rBV2	1921	1576	0.05%	0.006%
39	6.910	1808	1810	1814	rVV2	2058	1593	0.05%	0.006%
40	6.935	1815	1818	1827	rVB4	1546	2097	0.06%	0.008%
41	7.022	1840	1845	1848	rBV6	1150	1071	0.03%	0.004%
42	7.061	1855	1857	1863	rVB4	1799	1302	0.04%	0.005%
43	7.099	1863	1869	1871	rBV3	1686	1462	0.04%	0.006%
44	7.225	1897	1908	1936	rBV	388346	728040	21.53%	2.801%
45	7.466	1975	1983	1986	rBV8	4670	6424	0.19%	0.025%
46	7.562	2000	2013	2042	rBV	1241198	2309327	68.28%	8.885%
47	7.849	2090	2102	2138	rBV2	265255	502042	14.84%	1.932%
48	8.173	2188	2203	2216	rVV3	28612	59303	1.75%	0.228%
49	8.260	2227	2230	2234	rBV5	1717	1182	0.03%	0.005%
50	8.308	2234	2245	2285	rBV	1104062	2192893	64.84%	8.437%
51	8.469	2287	2295	2312	rVB3	55126	108665	3.21%	0.418%
52	8.697	2363	2366	2367	rBV4	1716	1008	0.03%	0.004%
53	8.739	2377	2379	2386	rBV6	1360	1454	0.04%	0.006%
54	8.781	2390	2392	2395	rVB4	1800	1071	0.03%	0.004%
55	8.890	2420	2426	2428	rBV2	2081	1867	0.06%	0.007%
56	8.922	2433	2436	2441	rBV4	1529	1289	0.04%	0.005%
57	8.955	2441	2446	2448	rVB4	1443	934	0.03%	0.004%
58	8.990	2455	2457	2463	rVB4	1597	912	0.03%	0.004%
59	9.032	2468	2470	2474	rVB2	1708	938	0.03%	0.004%
60	9.086	2474	2487	2530	rBV	1294510	2303164	68.10%	8.862%
61	9.366	2571	2574	2576	rBV4	1611	980	0.03%	0.004%
62	9.501	2614	2616	2619	rBV3	1663	1153	0.03%	0.004%
63	9.614	2649	2651	2655	rVB2	1420	997	0.03%	0.004%
64	9.668	2665	2668	2670	rBV3	1496	949	0.03%	0.004%
65	9.707	2677	2680	2682	rBV2	1429	944	0.03%	0.004%
66	9.935	2745	2751	2753	rBV4	3022	2588	0.08%	0.010%
67	9.996	2768	2770	2776	rVB4	2117	1585	0.05%	0.006%
68	10.038	2776	2783	2792	rBV7	8540	15789	0.47%	0.061%
69	10.186	2824	2829	2831	rBV5	1346	1100	0.03%	0.004%
70	10.202	2831	2834	2839	rBV2	1561	1614	0.05%	0.006%
71	10.241	2839	2846	2852	rBV9	7385	12651	0.37%	0.049%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031768.D
 Acq On : 06 May 2019 10:29
 Operator : JC/SP
 Sample : K2690-25
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5169

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.321	2869	2871	2875	rVB3	1877	1015	0.03%	0.004%
73	10.427	2890	2904	2929	rBV	1024843	1657378	49.00%	6.377%
74	10.604	2950	2959	2975	rVB6	20211	36264	1.07%	0.140%
75	10.662	2975	2977	2981	rVB2	2032	1324	0.04%	0.005%
76	10.704	2981	2990	2994	rBV2	3960	6240	0.18%	0.024%
77	10.723	2994	2996	3002	rVV4	1792	1271	0.04%	0.005%
78	10.765	3005	3009	3013	rBV5	1592	1609	0.05%	0.006%
79	10.955	3064	3068	3073	rVV4	1616	1878	0.06%	0.007%
80	10.977	3073	3075	3077	rVV	1973	1062	0.03%	0.004%
81	10.990	3077	3079	3085	rVB4	1300	942	0.03%	0.004%
82	11.221	3148	3151	3156	rBV4	1704	1445	0.04%	0.006%
83	11.266	3162	3165	3168	rVB4	1953	1316	0.04%	0.005%
84	11.283	3168	3170	3172	rBV2	1617	990	0.03%	0.004%
85	11.376	3195	3199	3202	rBV4	5070	4510	0.13%	0.017%
86	11.479	3219	3231	3258	rBV	1110855	1819759	53.80%	7.002%
87	11.771	3314	3322	3334	rVB9	5840	12938	0.38%	0.050%
88	11.855	3336	3348	3372	rBV	1146957	1919566	56.75%	7.386%
89	12.218	3455	3461	3463	rBV5	3863	4342	0.13%	0.017%
90	12.443	3528	3531	3534	rBV3	2304	2181	0.06%	0.008%
91	12.533	3555	3559	3562	rBV5	1993	1826	0.05%	0.007%
92	12.591	3570	3577	3579	rBV6	3410	4240	0.13%	0.016%
93	12.723	3614	3618	3620	rBV5	1953	1872	0.06%	0.007%
94	13.289	3791	3794	3795	rBV3	2331	1366	0.04%	0.005%
95	13.392	3823	3826	3830	rBV3	2611	2177	0.06%	0.008%
96	13.504	3857	3861	3863	rBV2	2293	1869	0.06%	0.007%
97	13.877	3975	3977	3982	rVB4	1855	1539	0.05%	0.006%
98	14.089	4038	4043	4045	rBV3	2062	1936	0.06%	0.007%
99	14.128	4053	4055	4062	rBV6	1442	1913	0.06%	0.007%
100	14.977	4316	4319	4323	rBV3	2087	2253	0.07%	0.009%


Sum of corrected areas: 25990323

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031768.D
Acq On : 06 May 2019 10:29
Operator : JC/SP
Sample : K2690-25
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
A5169

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

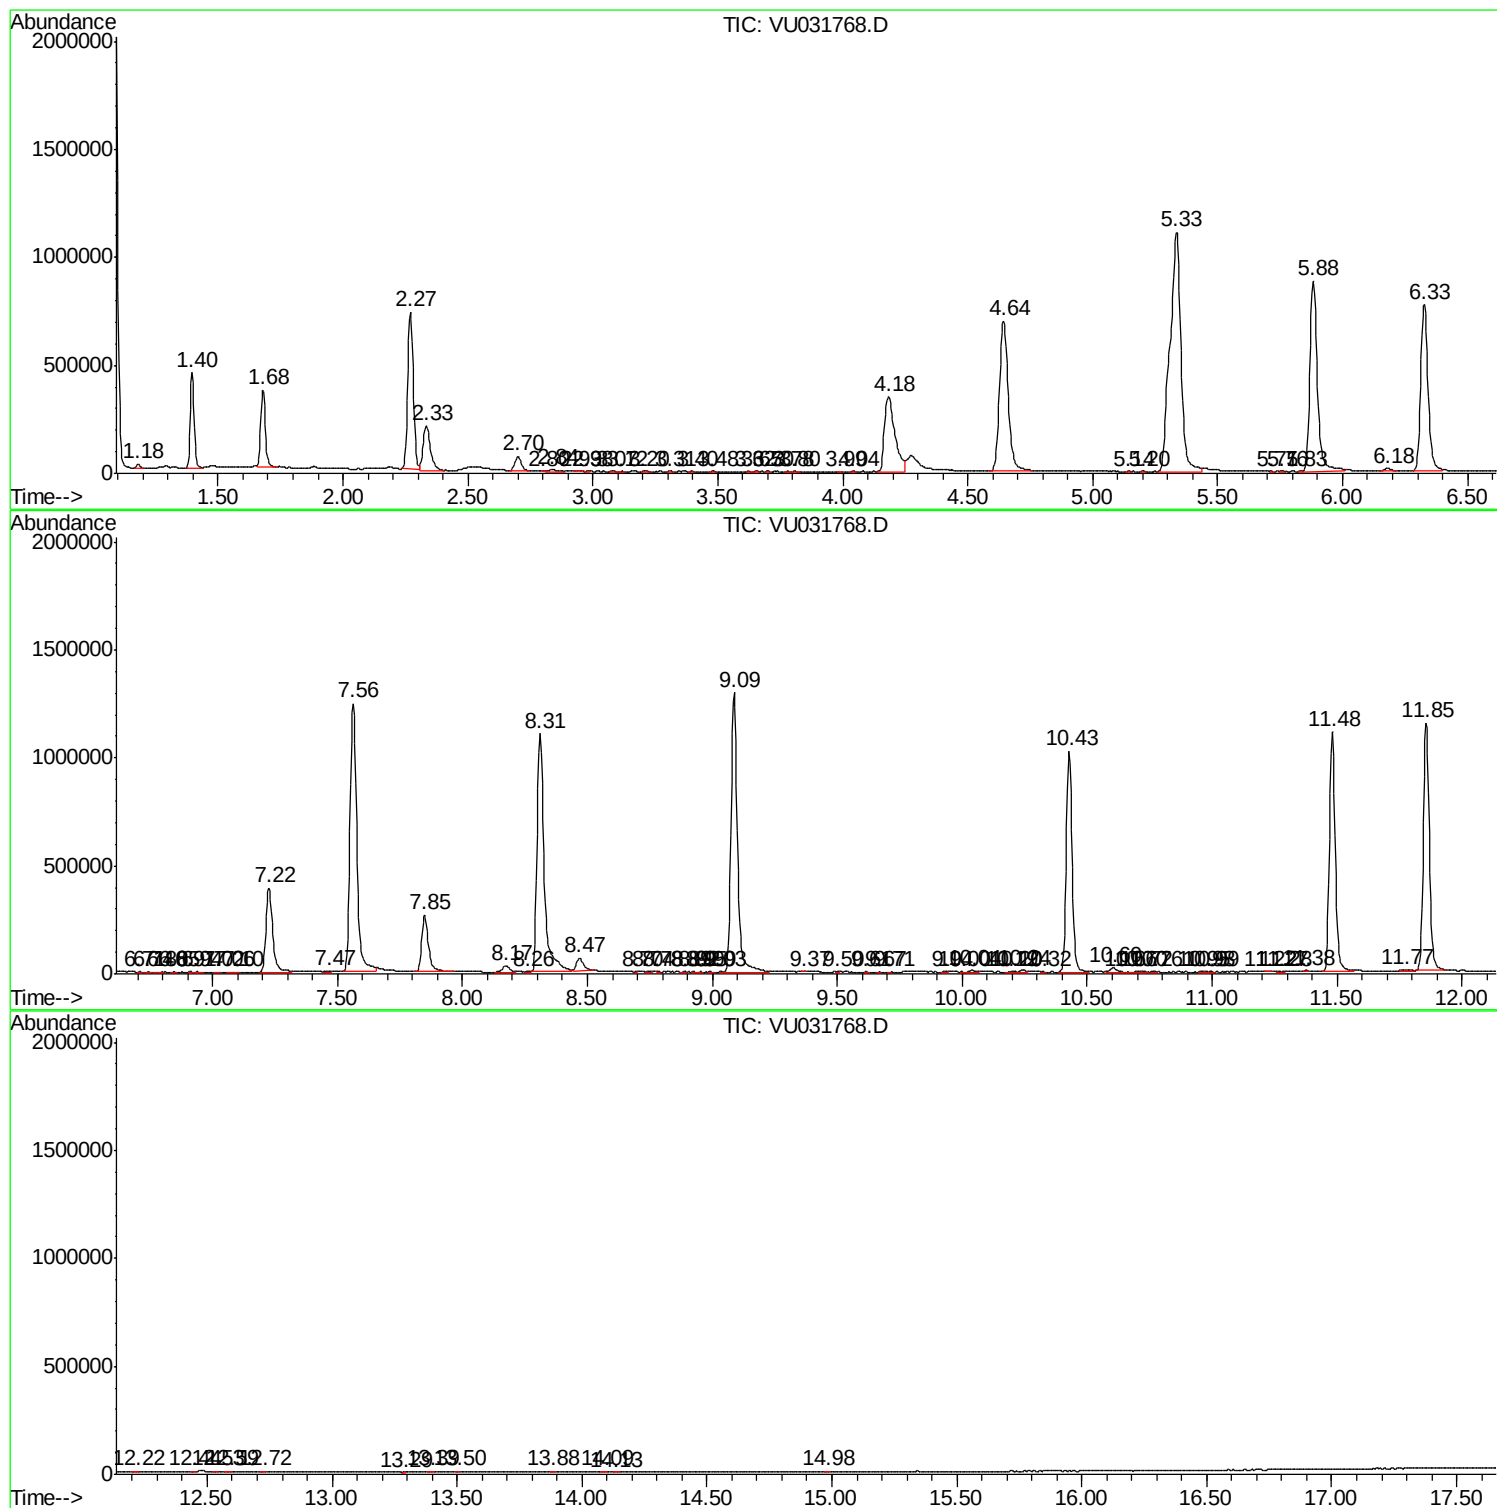

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031768.D
Acq On : 06 May 2019 10:29
Operator : JC/SP
Sample : K2690-25
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5169

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031768.D
Acq On : 06 May 2019 10:29
Operator : JC/SP
Sample : K2690-25
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5169

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
