

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031769.D
 Acq On : 06 May 2019 10:53
 Operator : JC/SP
 Sample : K2690-26
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	88	95	107	rBV	398620	432815	13.90%	1.872%
2	1.679	176	183	202	rVB	329860	414404	13.31%	1.792%
3	2.270	356	367	381	rBV	663872	1008222	32.38%	4.360%
4	2.476	425	431	434	rBV6	2595	3401	0.11%	0.015%
5	2.698	497	500	507	rVB4	4991	5215	0.17%	0.023%
6	2.897	560	562	573	rVB4	1162	1450	0.05%	0.006%
7	2.974	582	586	587	rBV2	2001	1488	0.05%	0.006%
8	2.987	587	590	591	rBV2	1693	1010	0.03%	0.004%
9	3.055	606	611	612	rBV3	1604	1491	0.05%	0.006%
10	3.164	642	645	650	rVB5	1106	919	0.03%	0.004%
11	3.232	663	666	670	rBV2	1484	1052	0.03%	0.005%
12	3.257	670	674	676	rVB3	1344	930	0.03%	0.004%
13	3.277	676	680	684	rBV3	1706	1550	0.05%	0.007%
14	3.383	710	713	717	rBV3	1426	1018	0.03%	0.004%
15	3.424	723	726	729	rBV	1308	982	0.03%	0.004%
16	3.553	763	766	772	rVB2	1589	1470	0.05%	0.006%
17	3.640	790	793	798	rBV2	1476	1473	0.05%	0.006%
18	3.717	812	817	820	rBV3	1153	1302	0.04%	0.006%
19	3.752	826	828	832	rVB3	1271	800	0.03%	0.003%
20	3.775	832	835	840	rBV3	1544	1674	0.05%	0.007%
21	3.839	853	855	861	rVB3	829	910	0.03%	0.004%
22	3.878	861	867	871	rBV4	1772	2084	0.07%	0.009%
23	3.958	888	892	896	rBV4	1660	1770	0.06%	0.008%
24	4.061	919	924	930	rVB4	950	1145	0.04%	0.005%
25	4.183	950	962	991	rBV	327467	962881	30.92%	4.164%
26	4.643	1089	1105	1134	rBV	513586	1222202	39.25%	5.285%
27	4.981	1204	1210	1219	rVV9	3046	5966	0.19%	0.026%
28	5.067	1234	1237	1242	rBV4	1872	1379	0.04%	0.006%
29	5.106	1242	1249	1252	rBV3	2291	2758	0.09%	0.012%
30	5.125	1252	1255	1261	rVV5	1488	1873	0.06%	0.008%
31	5.174	1267	1270	1274	rBV4	1674	1653	0.05%	0.007%
32	5.334	1295	1320	1347	rBV2	1020319	3113993	100.00%	13.466%
33	5.659	1418	1421	1423	rBV5	1883	1309	0.04%	0.006%
34	5.710	1434	1437	1442	rVB2	1996	1378	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031769.D
 Acq On : 06 May 2019 10:53
 Operator : JC/SP
 Sample : K2690-26
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.791	1459	1462	1465	rVB5	1473	1039	0.03%	0.004%
36	5.884	1473	1491	1519	rBV	824882	1727536	55.48%	7.470%
37	6.177	1573	1582	1593	rBV8	11442	25569	0.82%	0.111%
38	6.325	1612	1628	1657	rBV2	720786	1498297	48.11%	6.479%
39	6.518	1685	1688	1692	rBV4	1525	1463	0.05%	0.006%
40	6.636	1720	1725	1728	rVB5	2275	2317	0.07%	0.010%
41	6.672	1732	1736	1739	rBV3	1290	881	0.03%	0.004%
42	6.717	1746	1750	1752	rBV4	1615	1237	0.04%	0.005%
43	6.762	1759	1764	1767	rBV7	2010	2037	0.07%	0.009%
44	6.833	1782	1786	1789	rVB4	1384	985	0.03%	0.004%
45	6.894	1801	1805	1807	rBV5	1234	932	0.03%	0.004%
46	6.961	1821	1826	1828	rBV2	1206	986	0.03%	0.004%
47	6.974	1828	1830	1832	rVV2	1097	702	0.02%	0.003%
48	7.071	1857	1860	1863	rVB2	1345	1097	0.04%	0.005%
49	7.096	1863	1868	1869	rBV2	1564	1163	0.04%	0.005%
50	7.225	1894	1908	1933	rBV	360924	687837	22.09%	2.974%
51	7.386	1956	1958	1962	rVB2	1395	822	0.03%	0.004%
52	7.431	1969	1972	1976	rBV5	1020	790	0.03%	0.003%
53	7.563	2000	2013	2052	rBV	1136083	2142935	68.82%	9.267%
54	7.849	2091	2102	2123	rBV	243285	450097	14.45%	1.946%
55	8.141	2188	2193	2195	rBV4	1528	1400	0.04%	0.006%
56	8.225	2215	2219	2220	rBV3	2821	1901	0.06%	0.008%
57	8.308	2234	2245	2290	rBV	1056150	2116662	67.97%	9.153%
58	8.688	2359	2363	2369	rVB4	1740	2118	0.07%	0.009%
59	8.714	2369	2371	2375	rVB4	2090	1272	0.04%	0.006%
60	8.739	2375	2379	2382	rBV4	2085	1716	0.06%	0.007%
61	8.755	2382	2384	2387	rVB	1778	814	0.03%	0.004%
62	8.797	2395	2397	2404	rVB4	1478	990	0.03%	0.004%
63	8.829	2404	2407	2410	rBV3	1103	728	0.02%	0.003%
64	8.919	2432	2435	2439	rBV4	1428	1320	0.04%	0.006%
65	8.958	2444	2447	2449	rBV2	1285	841	0.03%	0.004%
66	8.971	2449	2451	2458	rVB5	1288	1081	0.03%	0.005%
67	9.013	2461	2464	2467	rBV2	1181	873	0.03%	0.004%
68	9.087	2474	2487	2534	rBV	1220847	2187693	70.25%	9.460%
69	9.784	2697	2704	2706	rBV5	3375	4003	0.13%	0.017%
70	9.845	2719	2723	2728	rVB7	1627	1689	0.05%	0.007%
71	9.878	2728	2733	2734	rBV4	1201	1055	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031769.D
 Acq On : 06 May 2019 10:53
 Operator : JC/SP
 Sample : K2690-26
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.003	2768	2772	2775	rBV3	870	763	0.02%	0.003%
73	10.106	2802	2804	2808	rVB2	1071	836	0.03%	0.004%
74	10.141	2808	2815	2817	rBV4	1727	1941	0.06%	0.008%
75	10.167	2817	2823	2830	rVV7	3498	4975	0.16%	0.022%
76	10.234	2841	2844	2847	rBV2	1206	877	0.03%	0.004%
77	10.251	2847	2849	2852	rVB3	1354	755	0.02%	0.003%
78	10.350	2875	2880	2881	rBV3	971	760	0.02%	0.003%
79	10.427	2891	2904	2923	rBV	957419	1560341	50.11%	6.747%
80	10.578	2947	2951	2952	rBV3	1519	1024	0.03%	0.004%
81	10.749	3001	3004	3007	rVB2	1222	828	0.03%	0.004%
82	10.787	3012	3016	3019	rBV	2471	2000	0.06%	0.009%
83	10.887	3045	3047	3050	rBV2	1130	768	0.02%	0.003%
84	10.926	3055	3059	3060	rBV	1097	778	0.02%	0.003%
85	10.942	3061	3064	3069	rVB2	1288	1027	0.03%	0.004%
86	10.968	3069	3072	3075	rBV2	1300	812	0.03%	0.004%
87	11.029	3088	3091	3094	rVB2	1514	963	0.03%	0.004%
88	11.080	3103	3107	3113	rVV8	1950	2138	0.07%	0.009%
89	11.160	3129	3132	3135	rBV3	1201	842	0.03%	0.004%
90	11.257	3156	3162	3171	rBV	2403	3923	0.13%	0.017%
91	11.479	3219	3231	3257	rBV	1004677	1680381	53.96%	7.266%
92	11.855	3336	3348	3366	rBV	1044365	1762599	56.60%	7.622%
93	12.373	3506	3509	3511	rBV2	1193	955	0.03%	0.004%
94	12.479	3534	3542	3546	rBV6	6188	8798	0.28%	0.038%
95	12.652	3593	3596	3597	rBV2	1719	1006	0.03%	0.004%
96	12.758	3627	3629	3636	rVB5	1952	1575	0.05%	0.007%
97	13.228	3772	3775	3777	rBV2	1639	1011	0.03%	0.004%
98	13.729	3929	3931	3933	rBV2	1333	722	0.02%	0.003%
99	13.848	3965	3968	3972	rBV4	2603	1707	0.05%	0.007%
100	13.932	3992	3994	3997	rBV3	1626	1215	0.04%	0.005%


Sum of corrected areas: 23125165

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031769.D
Acq On : 06 May 2019 10:53
Operator : JC/SP
Sample : K2690-26
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

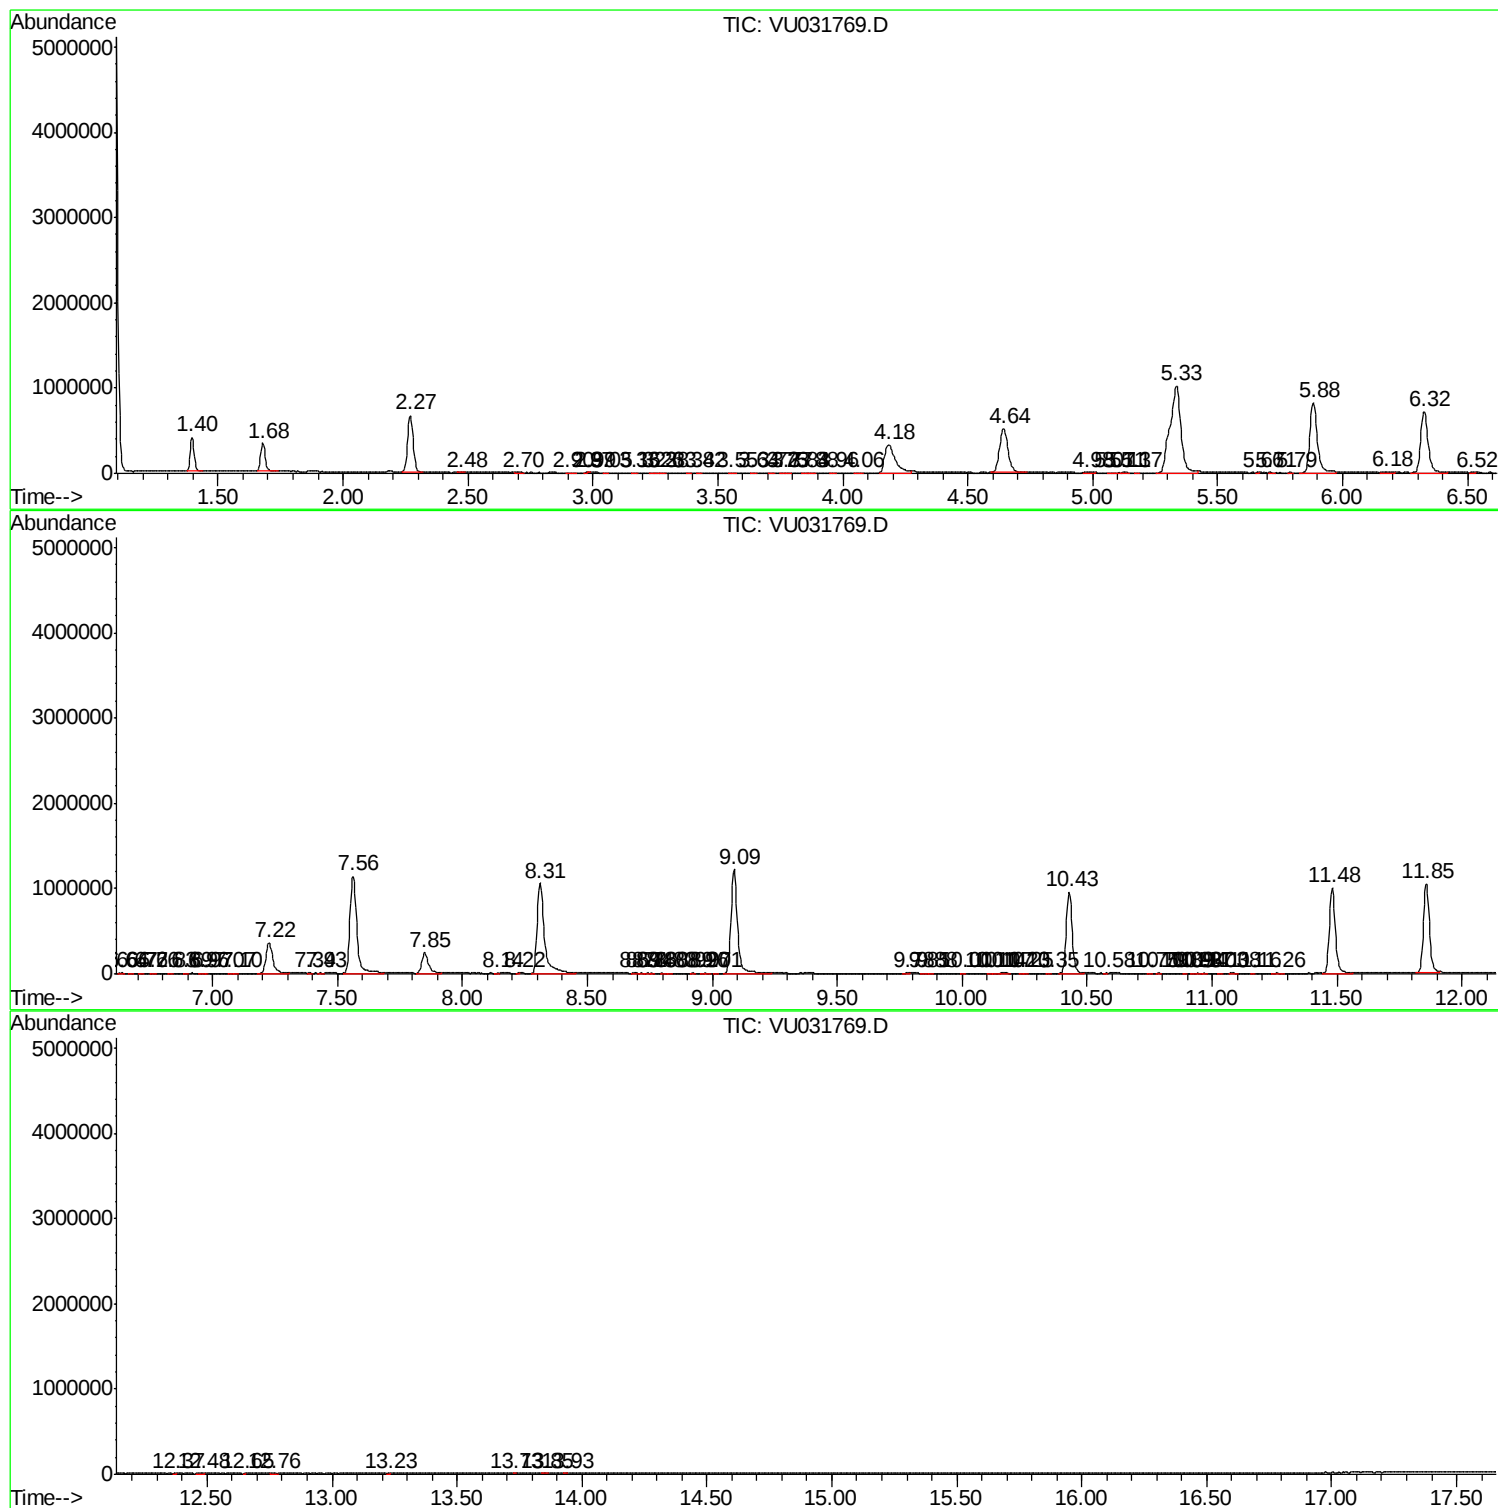

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031769.D
Acq On : 06 May 2019 10:53
Operator : JC/SP
Sample : K2690-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031769.D
Acq On : 06 May 2019 10:53
Operator : JC/SP
Sample : K2690-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc