

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031770.D
 Acq On : 06 May 2019 11:16
 Operator : JC/SP
 Sample : K2694-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB3	16389	15878	0.47%	0.064%
2	1.396	88	95	111	rBV	445988	478873	14.07%	1.925%
3	1.679	176	183	200	rVB	374522	456162	13.40%	1.833%
4	2.270	356	367	380	rVB	733194	1108248	32.56%	4.454%
5	2.550	452	454	457	rVB2	1841	971	0.03%	0.004%
6	2.637	478	481	482	rBV3	1065	591	0.02%	0.002%
7	2.701	496	501	503	rBV3	1575	1650	0.05%	0.007%
8	2.740	510	513	521	rVB5	1462	1651	0.05%	0.007%
9	2.781	521	526	531	rBV4	1475	2001	0.06%	0.008%
10	2.826	533	540	541	rBV6	3252	2957	0.09%	0.012%
11	2.913	561	567	573	rBV6	1347	2125	0.06%	0.009%
12	2.949	573	578	584	rVB4	1375	1550	0.05%	0.006%
13	3.013	597	598	604	rVB4	1001	710	0.02%	0.003%
14	3.148	638	640	644	rBV3	956	606	0.02%	0.002%
15	3.222	661	663	666	rVB2	1303	758	0.02%	0.003%
16	3.257	666	674	676	rBV4	743	820	0.02%	0.003%
17	3.296	683	686	688	rBV2	1041	680	0.02%	0.003%
18	3.344	697	701	705	rBV4	901	741	0.02%	0.003%
19	3.396	714	717	723	rVB3	1645	1199	0.04%	0.005%
20	3.441	726	731	734	rVV4	846	862	0.03%	0.003%
21	3.457	734	736	743	rVB3	1239	1176	0.03%	0.005%
22	3.508	747	752	753	rBV2	709	673	0.02%	0.003%
23	3.614	781	785	787	rBV2	1301	1012	0.03%	0.004%
24	3.650	792	796	800	rVB	1161	963	0.03%	0.004%
25	3.711	812	815	818	rBV2	938	599	0.02%	0.002%
26	3.833	847	853	859	rBV6	1402	1918	0.06%	0.008%
27	3.862	859	862	865	rVV2	1225	803	0.02%	0.003%
28	3.894	870	872	876	rVB	1295	707	0.02%	0.003%
29	4.010	900	908	910	rBV3	1666	1864	0.05%	0.007%
30	4.084	928	931	932	rBV2	1122	586	0.02%	0.002%
31	4.122	940	943	946	rVB	1038	588	0.02%	0.002%
32	4.183	946	962	1003	rBV	347596	1094316	32.15%	4.398%
33	4.511	1061	1064	1066	rBV3	1086	743	0.02%	0.003%
34	4.643	1087	1105	1133	rBV	561851	1333439	39.17%	5.360%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031770.D
 Acq On : 06 May 2019 11:16
 Operator : JC/SP
 Sample : K2694-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.887	1174	1181	1186	rVB5	2722	2829	0.08%	0.011%
36	4.939	1194	1197	1198	rBV3	1098	639	0.02%	0.003%
37	4.978	1206	1209	1210	rBV3	1188	738	0.02%	0.003%
38	5.071	1234	1238	1243	rBV6	1653	1521	0.04%	0.006%
39	5.151	1260	1263	1266	rVB3	979	690	0.02%	0.003%
40	5.170	1266	1269	1271	rBV3	955	648	0.02%	0.003%
41	5.212	1280	1282	1286	rVB3	862	584	0.02%	0.002%
42	5.238	1286	1290	1292	rBV	1178	870	0.03%	0.003%
43	5.334	1297	1320	1355	rBV2	1100511	3403862	100.00%	13.681%
44	5.592	1398	1400	1404	rBV4	1336	817	0.02%	0.003%
45	5.740	1443	1446	1448	rBV3	925	613	0.02%	0.002%
46	5.884	1477	1491	1527	rBV	870925	1855157	54.50%	7.457%
47	6.190	1571	1586	1601	rBV9	20472	51825	1.52%	0.208%
48	6.325	1615	1628	1658	rBV	762992	1583000	46.51%	6.363%
49	6.717	1746	1750	1751	rBV4	1030	783	0.02%	0.003%
50	6.733	1751	1755	1760	rVV3	2485	2202	0.06%	0.009%
51	6.775	1764	1768	1770	rBV2	863	667	0.02%	0.003%
52	6.801	1773	1776	1782	rVB6	1718	1344	0.04%	0.005%
53	6.836	1782	1787	1789	rBV3	1435	1144	0.03%	0.005%
54	6.923	1811	1814	1817	rVB2	1848	1095	0.03%	0.004%
55	6.961	1823	1826	1828	rVB2	1300	610	0.02%	0.002%
56	7.058	1852	1856	1859	rVB	1601	1205	0.04%	0.005%
57	7.077	1859	1862	1867	rBV3	1275	979	0.03%	0.004%
58	7.106	1867	1871	1872	rBV3	1492	923	0.03%	0.004%
59	7.225	1893	1908	1933	rBV	384721	735393	21.60%	2.956%
60	7.463	1979	1982	1987	rVB6	1779	1243	0.04%	0.005%
61	7.511	1994	1997	1998	rBV2	1113	657	0.02%	0.003%
62	7.563	2000	2013	2046	rBV	1240164	2328837	68.42%	9.360%
63	7.849	2090	2102	2129	rBV2	262768	493155	14.49%	1.982%
64	8.048	2161	2164	2166	rBV3	1162	901	0.03%	0.004%
65	8.112	2181	2184	2191	rVB3	1758	1881	0.06%	0.008%
66	8.174	2192	2203	2213	rBV3	18196	36326	1.07%	0.146%
67	8.260	2224	2230	2231	rBV4	1024	1087	0.03%	0.004%
68	8.309	2234	2245	2284	rBV	1108918	2223551	65.32%	8.937%
69	8.755	2380	2384	2388	rBV6	1704	1469	0.04%	0.006%
70	8.897	2426	2428	2431	rVB3	1630	877	0.03%	0.004%
71	8.945	2439	2443	2447	rVB7	1284	1104	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031770.D
 Acq On : 06 May 2019 11:16
 Operator : JC/SP
 Sample : K2694-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	8.974	2447	2452	2455	rBV5	1337	1253	0.04%	0.005%
73	9.022	2465	2467	2471	rBV3	1770	1165	0.03%	0.005%
74	9.087	2471	2487	2527	rBV	1282247	2304238	67.69%	9.262%
75	9.524	2621	2623	2627	rVB3	1532	807	0.02%	0.003%
76	9.755	2690	2695	2696	rBV2	1445	1194	0.04%	0.005%
77	9.813	2709	2713	2715	rBV3	879	746	0.02%	0.003%
78	9.997	2764	2770	2772	rBV4	1905	1850	0.05%	0.007%
79	10.042	2780	2784	2786	rBV3	1535	1405	0.04%	0.006%
80	10.170	2821	2824	2829	rBV4	2023	1564	0.05%	0.006%
81	10.292	2859	2862	2864	rBV2	907	759	0.02%	0.003%
82	10.360	2879	2883	2884	rBV	1626	853	0.03%	0.003%
83	10.373	2884	2887	2888	rVV2	1268	726	0.02%	0.003%
84	10.427	2891	2904	2932	rVV	1012681	1654755	48.61%	6.651%
85	10.604	2949	2959	2973	rVB5	17174	28976	0.85%	0.116%
86	10.662	2973	2977	2980	rBV3	855	699	0.02%	0.003%
87	10.717	2991	2994	2998	rBV4	1159	638	0.02%	0.003%
88	10.755	3003	3006	3009	rVB2	1903	1041	0.03%	0.004%
89	10.849	3033	3035	3038	rBV2	1162	776	0.02%	0.003%
90	11.328	3181	3184	3187	rBV4	1305	930	0.03%	0.004%
91	11.376	3196	3199	3202	rBV2	1755	1275	0.04%	0.005%
92	11.479	3219	3231	3258	rBV	1042955	1741084	51.15%	6.998%
93	11.755	3315	3317	3319	rBV3	1588	808	0.02%	0.003%
94	11.855	3337	3348	3374	rBV	1100919	1861438	54.69%	7.482%
95	12.392	3512	3515	3518	rBV4	1563	1058	0.03%	0.004%
96	12.472	3534	3540	3541	rBV4	6624	5042	0.15%	0.020%
97	12.550	3562	3564	3567	rBV3	1782	915	0.03%	0.004%
98	12.604	3578	3581	3582	rBV2	2211	1330	0.04%	0.005%
99	12.968	3691	3694	3697	rBV3	2305	1367	0.04%	0.005%
100	13.591	3886	3888	3891	rBV2	1552	1172	0.03%	0.005%


Sum of corrected areas: 24879510

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031770.D
Acq On : 06 May 2019 11:16
Operator : JC/SP
Sample : K2694-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHG0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

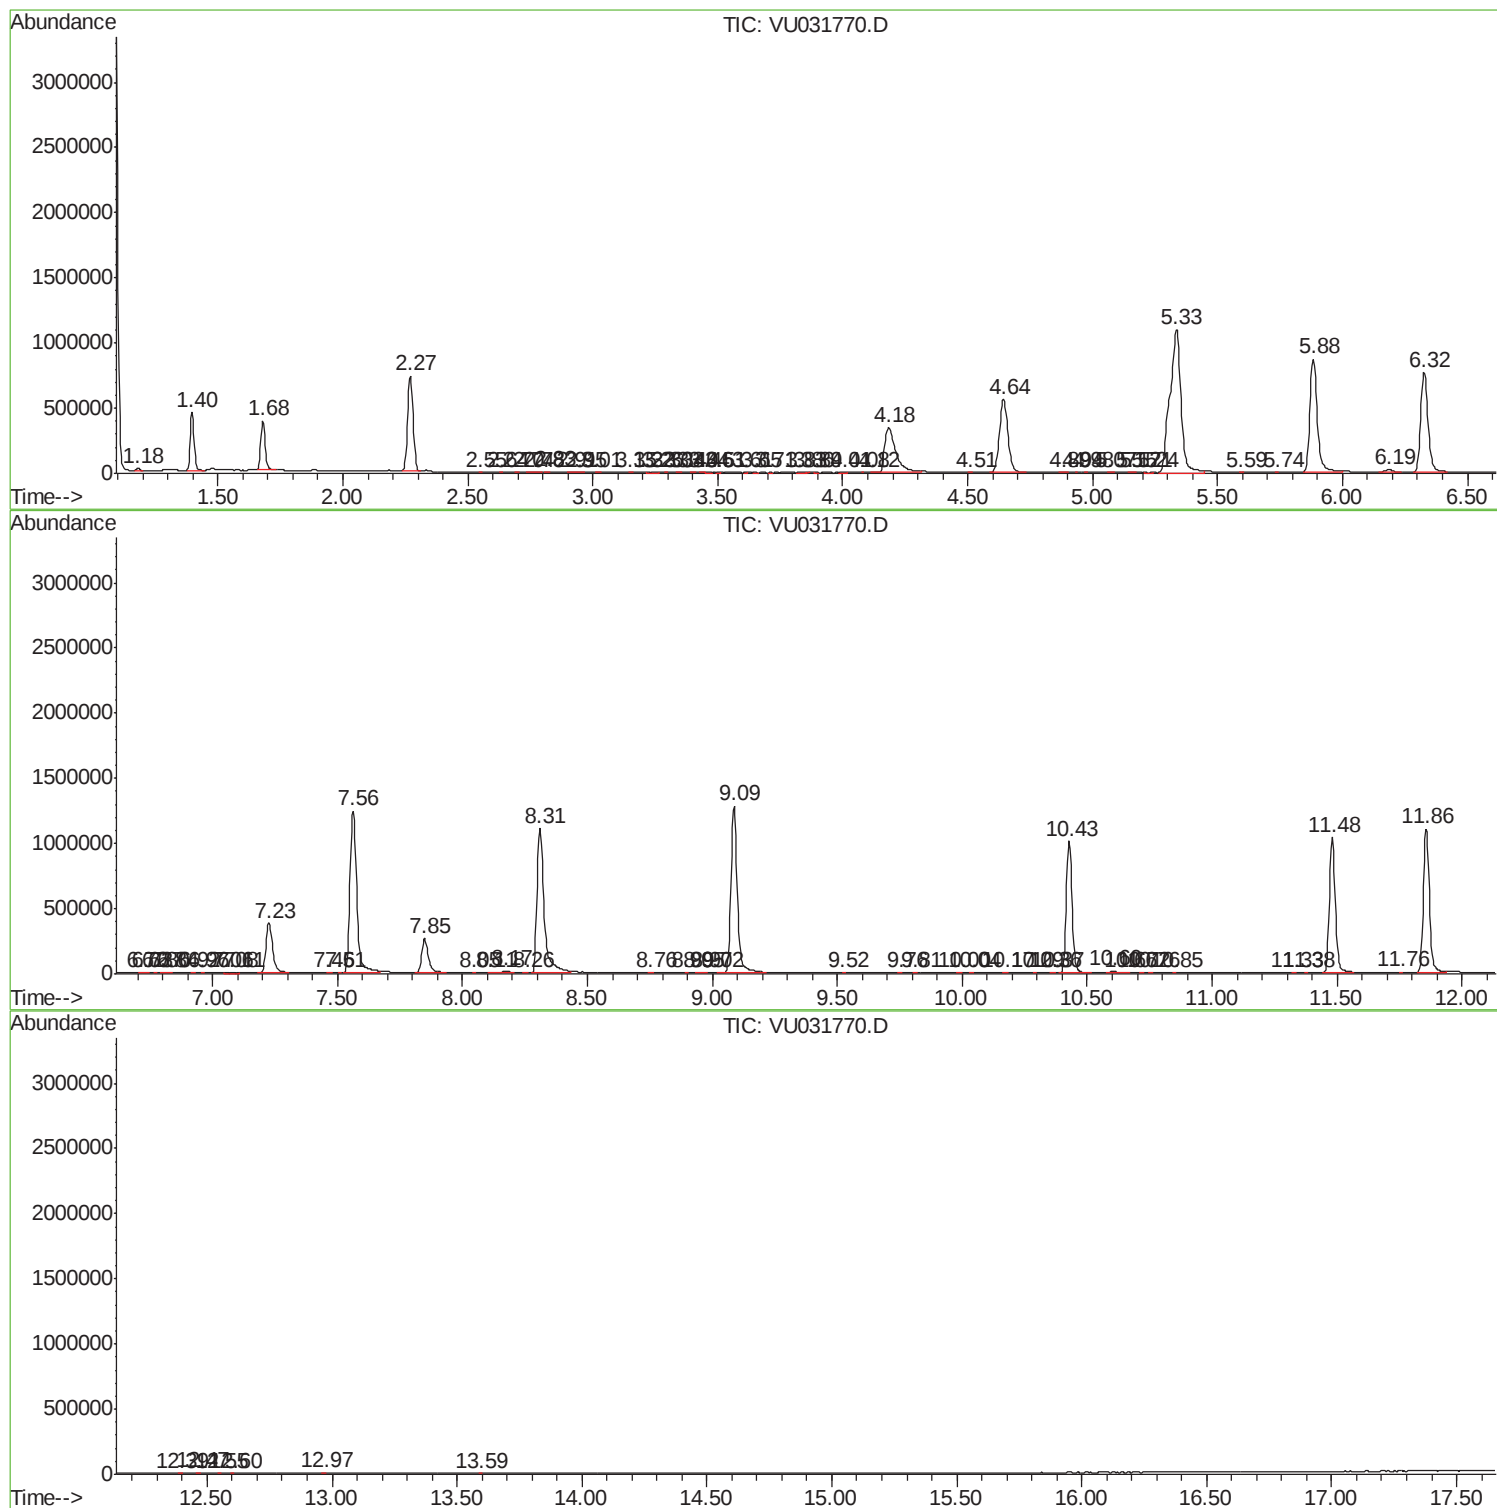

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031770.D
Acq On : 06 May 2019 11:16
Operator : JC/SP
Sample : K2694-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHG0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031770.D
Acq On : 06 May 2019 11:16
Operator : JC/SP
Sample : K2694-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHG0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc