

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031772.D
 Acq On : 06 May 2019 12:02
 Operator : JC/SP
 Sample : K2695-02 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.283	55	60	69	rBV2	42945	44356	1.26%	0.154%
2	1.395	88	95	109	rVB	449140	481308	13.71%	1.666%
3	1.678	176	183	197	rBV	364810	443195	12.62%	1.534%
4	1.881	241	246	254	rVB2	30906	37501	1.07%	0.130%
5	2.270	356	367	381	rBV	752206	1151279	32.79%	3.984%
6	2.434	416	418	421	rBV3	1792	1032	0.03%	0.004%
7	2.688	494	497	500	rVV4	1213	981	0.03%	0.003%
8	2.794	526	530	534	rBV5	1346	1189	0.03%	0.004%
9	2.874	552	555	561	rVV6	939	899	0.03%	0.003%
10	2.977	584	587	589	rBV2	1118	871	0.02%	0.003%
11	3.038	600	606	608	rBV4	1447	1702	0.05%	0.006%
12	3.093	615	623	626	rBV4	2054	2447	0.07%	0.008%
13	3.145	636	639	645	rVB2	1050	879	0.03%	0.003%
14	3.174	645	648	651	rBV5	999	799	0.02%	0.003%
15	3.209	655	659	661	rBV2	1481	1168	0.03%	0.004%
16	3.251	667	672	677	rBV5	1212	1224	0.03%	0.004%
17	3.296	682	686	687	rBV2	1447	914	0.03%	0.003%
18	3.521	753	756	760	rVB2	1773	1590	0.05%	0.006%
19	3.556	760	767	771	rBV4	2386	2827	0.08%	0.010%
20	3.585	771	776	779	rBV3	1136	1030	0.03%	0.004%
21	3.649	791	796	797	rBV2	835	746	0.02%	0.003%
22	3.685	804	807	808	rBV	1328	772	0.02%	0.003%
23	3.698	809	811	815	rVV	1773	1304	0.04%	0.005%
24	3.743	821	825	829	rBV2	1805	1477	0.04%	0.005%
25	3.781	833	837	840	rVB2	2276	1595	0.05%	0.006%
26	3.800	840	843	846	rBV2	1886	1521	0.04%	0.005%
27	3.897	870	873	878	rBV2	1300	1065	0.03%	0.004%
28	3.929	881	883	888	rBV2	1058	780	0.02%	0.003%
29	4.009	904	908	910	rBV3	938	795	0.02%	0.003%
30	4.122	938	943	948	rVB4	967	850	0.02%	0.003%
31	4.186	949	963	1006	rBV	349126	1122652	31.97%	3.885%
32	4.514	1062	1065	1067	rBV3	1685	1227	0.03%	0.004%
33	4.550	1073	1076	1079	rBV3	1988	1040	0.03%	0.004%
34	4.582	1082	1086	1087	rBV3	1025	759	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031772.D
 Acq On : 06 May 2019 12:02
 Operator : JC/SP
 Sample : K2695-02 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.643	1088	1105	1133	rBV	579615	1379824	39.30%	4.775%
36	5.106	1244	1249	1251	rVB3	1297	938	0.03%	0.003%
37	5.125	1251	1255	1260	rBV5	1479	1240	0.04%	0.004%
38	5.231	1285	1288	1291	rBV	1170	948	0.03%	0.003%
39	5.334	1297	1320	1357	rBV2	1144389	3511094	100.00%	12.151%
40	5.694	1429	1432	1435	rVB3	2048	1068	0.03%	0.004%
41	5.733	1441	1444	1447	rBV3	1209	852	0.02%	0.003%
42	5.826	1467	1473	1475	rBV5	970	1197	0.03%	0.004%
43	5.881	1477	1490	1513	rBV	912725	1877834	53.48%	6.499%
44	6.183	1569	1584	1614	rBV	1653219	3353189	95.50%	11.604%
45	6.324	1616	1628	1653	rVB	791152	1637430	46.64%	5.667%
46	6.762	1761	1764	1768	rBV2	1047	831	0.02%	0.003%
47	6.784	1768	1771	1775	rVB3	1550	1178	0.03%	0.004%
48	6.807	1775	1778	1780	rBV2	1204	911	0.03%	0.003%
49	6.836	1784	1787	1791	rVB3	1348	843	0.02%	0.003%
50	6.878	1794	1800	1804	rBV6	1668	1992	0.06%	0.007%
51	6.906	1804	1809	1811	rVV4	1629	1377	0.04%	0.005%
52	6.942	1818	1820	1825	rVB5	1678	1248	0.04%	0.004%
53	6.971	1826	1829	1833	rBV4	1506	1020	0.03%	0.004%
54	6.990	1833	1835	1839	rVB3	1485	930	0.03%	0.003%
55	7.112	1870	1873	1877	rVB3	1090	1017	0.03%	0.004%
56	7.138	1877	1881	1885	rBV3	1152	1181	0.03%	0.004%
57	7.160	1885	1888	1892	rVB3	1593	1405	0.04%	0.005%
58	7.225	1896	1908	1934	rBV	411617	771881	21.98%	2.671%
59	7.498	1988	1993	1995	rBV4	1806	1659	0.05%	0.006%
60	7.562	2000	2013	2036	rBV	1300930	2386438	67.97%	8.259%
61	7.849	2090	2102	2131	rBV	271185	514811	14.66%	1.782%
62	7.971	2137	2140	2143	rBV4	1332	913	0.03%	0.003%
63	8.228	2212	2220	2232	rVB7	12836	23676	0.67%	0.082%
64	8.312	2235	2246	2293	rBV	1133261	2309118	65.77%	7.991%
65	8.717	2370	2372	2375	rBV4	1659	1029	0.03%	0.004%
66	8.820	2401	2404	2406	rBV2	1436	1067	0.03%	0.004%
67	8.868	2416	2419	2421	rBV4	1267	797	0.02%	0.003%
68	8.913	2431	2433	2438	rVB5	1623	1285	0.04%	0.004%
69	8.977	2450	2453	2455	rBV2	1320	787	0.02%	0.003%
70	9.019	2463	2466	2468	rBV2	1674	1164	0.03%	0.004%
71	9.035	2468	2471	2474	rBV2	1156	741	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031772.D
 Acq On : 06 May 2019 12:02
 Operator : JC/SP
 Sample : K2695-02 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.086	2474	2487	2532	rBV	1325327	2361154	67.25%	8.171%
73	9.305	2553	2555	2558	rVB2	1285	737	0.02%	0.003%
74	9.582	2638	2641	2648	rBV3	2300	2431	0.07%	0.008%
75	9.662	2664	2666	2670	rVB2	1406	982	0.03%	0.003%
76	9.781	2698	2703	2705	rBV2	1361	1241	0.04%	0.004%
77	9.865	2725	2729	2731	rBV	1084	808	0.02%	0.003%
78	10.138	2809	2814	2818	rVB2	1604	1313	0.04%	0.005%
79	10.167	2819	2823	2826	rBV	1269	1119	0.03%	0.004%
80	10.186	2826	2829	2832	rVB2	1431	879	0.03%	0.003%
81	10.427	2891	2904	2928	rBV	1036963	1698267	48.37%	5.877%
82	10.594	2952	2956	2957	rBV2	1618	1129	0.03%	0.004%
83	10.675	2974	2981	2985	rVB4	1614	1847	0.05%	0.006%
84	10.932	3056	3061	3064	rBV4	2231	2087	0.06%	0.007%
85	10.996	3079	3081	3086	rVB3	1341	854	0.02%	0.003%
86	11.025	3086	3090	3092	rBV2	1121	956	0.03%	0.003%
87	11.122	3117	3120	3124	rVB2	1425	750	0.02%	0.003%
88	11.382	3197	3201	3204	rBV2	1720	1216	0.03%	0.004%
89	11.401	3204	3207	3211	rBV4	1345	1219	0.03%	0.004%
90	11.482	3220	3232	3258	rBV	1062159	1778503	50.65%	6.155%
91	11.855	3336	3348	3378	rBV	1118766	1911500	54.44%	6.615%
92	12.257	3468	3473	3475	rBV5	1807	1715	0.05%	0.006%
93	12.347	3498	3501	3509	rBV7	1918	2432	0.07%	0.008%
94	12.385	3509	3513	3515	rBV3	1617	1082	0.03%	0.004%
95	12.434	3526	3528	3531	rBV3	1097	880	0.03%	0.003%
96	12.472	3536	3540	3542	rBV3	4421	3446	0.10%	0.012%
97	12.630	3584	3589	3594	rBV4	2093	2708	0.08%	0.009%
98	13.016	3706	3709	3715	rBV2	2059	2097	0.06%	0.007%
99	13.823	3957	3960	3963	rBV2	2422	1791	0.05%	0.006%
100	14.006	4012	4017	4020	rBV3	1862	1984	0.06%	0.007%


Sum of corrected areas: 28895814

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031772.D
Acq On : 06 May 2019 12:02
Operator : JC/SP
Sample : K2695-02 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

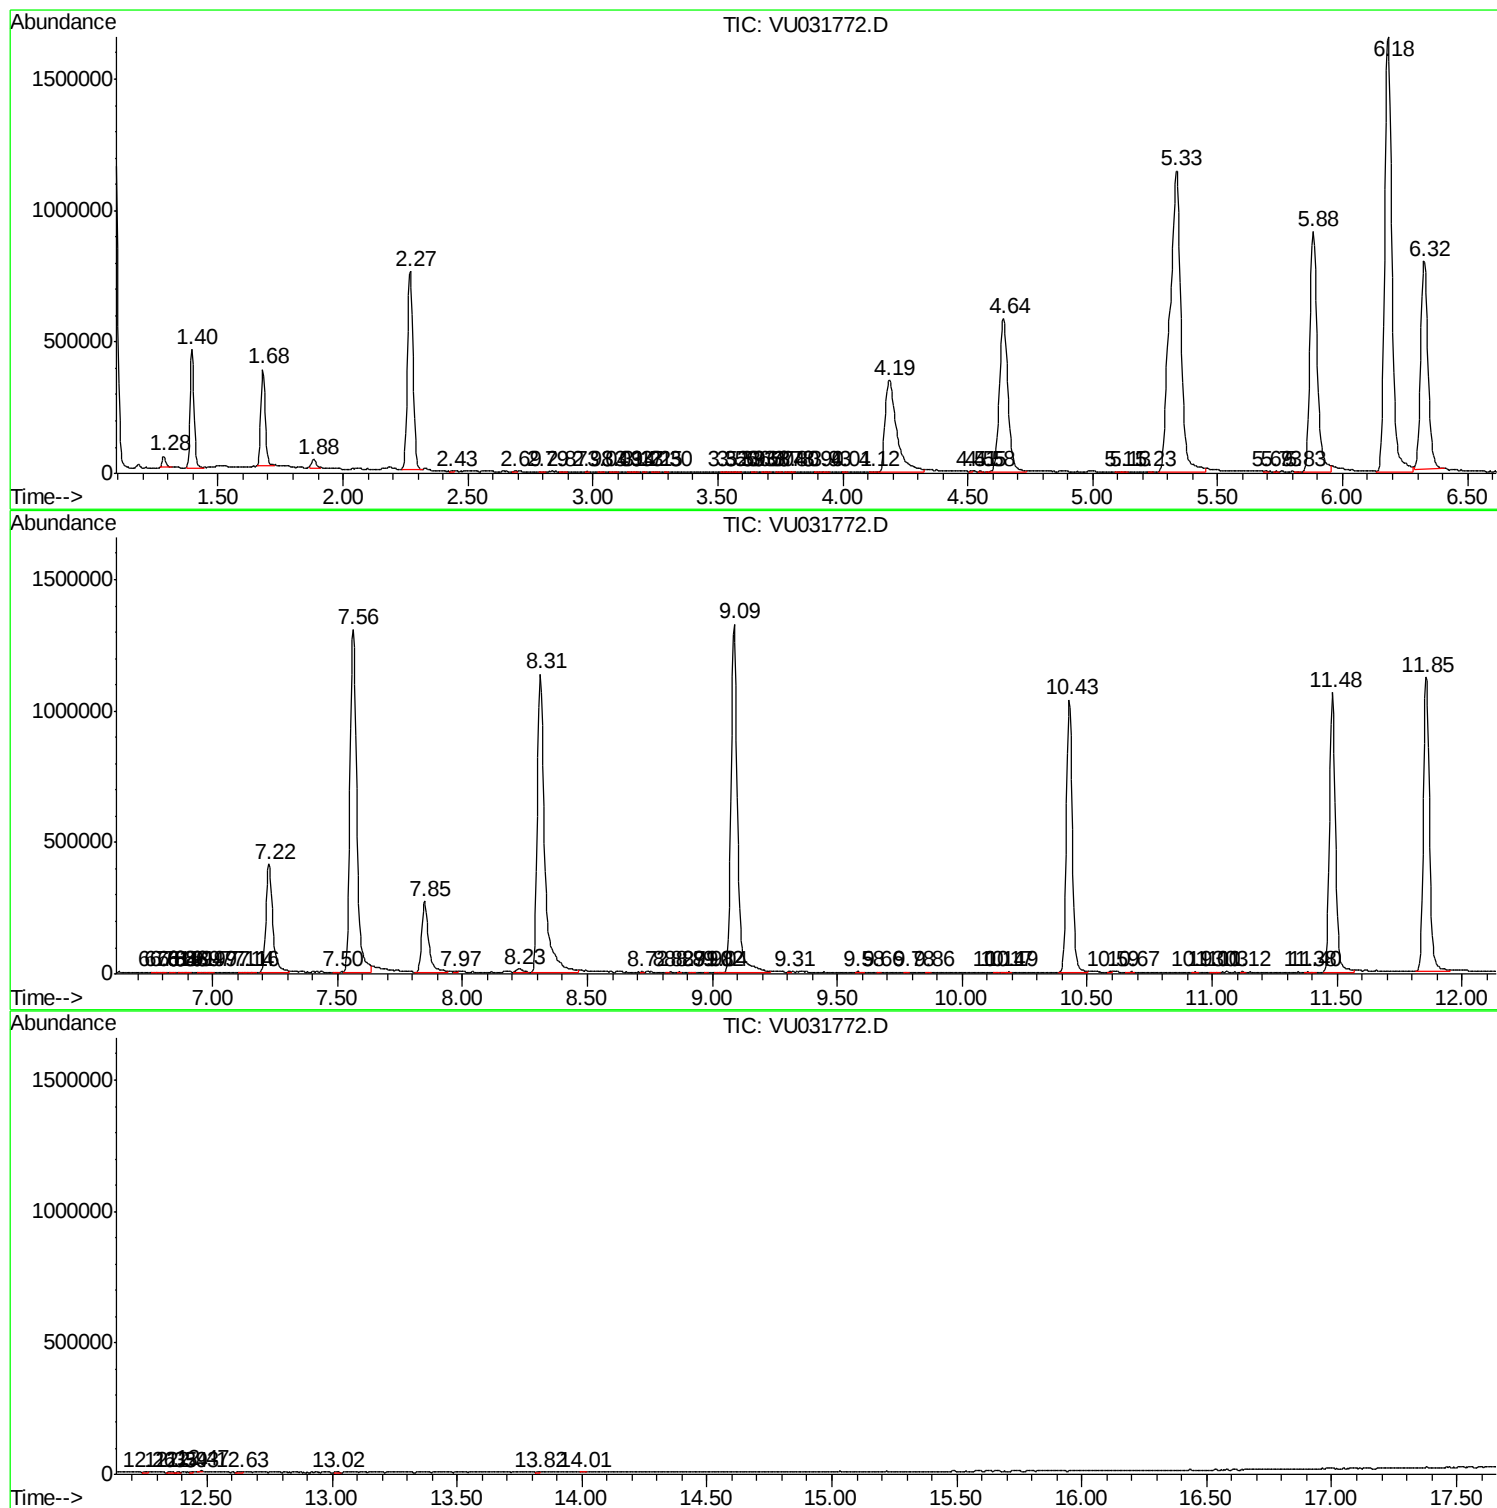

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031772.D
Acq On : 06 May 2019 12:02
Operator : JC/SP
Sample : K2695-02 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031772.D
Acq On : 06 May 2019 12:02
Operator : JC/SP
Sample : K2695-02 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X70

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc