

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031773.D
 Acq On : 06 May 2019 12:26
 Operator : JC/SP
 Sample : K2695-13 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rVB2	16153	16377	0.48%	0.059%
2	1.283	55	60	68	rBV2	51742	54244	1.59%	0.194%
3	1.396	88	95	106	rBV	433569	470456	13.77%	1.684%
4	1.679	175	183	215	rVB	379282	509373	14.91%	1.824%
5	2.270	356	367	380	rVB	738295	1136773	33.27%	4.070%
6	2.650	482	485	488	rVB2	1056	768	0.02%	0.003%
7	2.695	493	499	500	rBV5	2679	2184	0.06%	0.008%
8	2.752	515	517	519	rBV2	1214	678	0.02%	0.002%
9	2.788	524	528	531	rBV3	1158	872	0.03%	0.003%
10	2.830	535	541	543	rBV5	2789	3273	0.10%	0.012%
11	2.910	561	566	569	rBV5	1577	1736	0.05%	0.006%
12	2.965	580	583	588	rBV3	1025	843	0.02%	0.003%
13	2.990	588	591	595	rBV2	1337	739	0.02%	0.003%
14	3.035	600	605	608	rBV3	1649	1466	0.04%	0.005%
15	3.322	687	694	700	rBV6	1673	2548	0.07%	0.009%
16	3.425	722	726	728	rBV3	832	666	0.02%	0.002%
17	3.524	752	757	759	rBV3	780	712	0.02%	0.003%
18	3.569	764	771	774	rBV4	1238	1625	0.05%	0.006%
19	3.588	774	777	779	rBV2	1217	788	0.02%	0.003%
20	3.743	822	825	829	rVB3	1086	814	0.02%	0.003%
21	3.765	829	832	835	rVB2	1647	1149	0.03%	0.004%
22	3.788	835	839	841	rBV2	1327	1007	0.03%	0.004%
23	3.920	873	880	886	rVB5	1569	2199	0.06%	0.008%
24	3.968	892	895	899	rVB3	993	735	0.02%	0.003%
25	4.026	907	913	916	rBV2	1565	1256	0.04%	0.004%
26	4.084	926	931	935	rVB3	1330	1078	0.03%	0.004%
27	4.138	943	948	949	rBV3	1033	799	0.02%	0.003%
28	4.183	949	962	996	rBV	350231	1100641	32.22%	3.941%
29	4.643	1088	1105	1127	rBV	567003	1354120	39.64%	4.848%
30	4.862	1169	1173	1176	rBV2	1832	1641	0.05%	0.006%
31	5.045	1228	1230	1233	rBV3	1313	634	0.02%	0.002%
32	5.064	1233	1236	1241	rVV4	1168	1023	0.03%	0.004%
33	5.113	1247	1251	1254	rBV2	1189	831	0.02%	0.003%
34	5.132	1254	1257	1261	rVB3	1615	1071	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031773.D
 Acq On : 06 May 2019 12:26
 Operator : JC/SP
 Sample : K2695-13 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.161	1261	1266	1271	rBV4	1437	1848	0.05%	0.007%
36	5.186	1271	1274	1281	rVB5	1062	983	0.03%	0.004%
37	5.225	1281	1286	1289	rBV2	1703	1563	0.05%	0.006%
38	5.244	1289	1292	1297	rVB3	1451	1289	0.04%	0.005%
39	5.334	1297	1320	1343	rBV2	1126484	3416449	100.00%	12.232%
40	5.646	1415	1417	1420	rBV4	981	741	0.02%	0.003%
41	5.743	1442	1447	1450	rBV4	1354	1315	0.04%	0.005%
42	5.778	1453	1458	1463	rVB7	2756	2700	0.08%	0.010%
43	5.823	1469	1472	1474	rBV2	1354	1007	0.03%	0.004%
44	5.884	1477	1491	1523	rBV	907241	1890613	55.34%	6.769%
45	6.180	1569	1583	1609	rBV	1411058	2862178	83.78%	10.247%
46	6.325	1616	1628	1653	rVB	789148	1586793	46.45%	5.681%
47	6.643	1722	1727	1729	rBV4	718	610	0.02%	0.002%
48	6.698	1740	1744	1746	rBV4	1723	1251	0.04%	0.004%
49	6.711	1746	1748	1754	rVB4	1477	1092	0.03%	0.004%
50	6.794	1768	1774	1778	rBV5	1300	1598	0.05%	0.006%
51	6.884	1796	1802	1805	rBV4	1863	2260	0.07%	0.008%
52	6.903	1805	1808	1810	rBV3	1335	895	0.03%	0.003%
53	6.993	1834	1836	1841	rVB2	1484	891	0.03%	0.003%
54	7.026	1841	1846	1851	rBV5	1139	1277	0.04%	0.005%
55	7.225	1897	1908	1931	rBV	390539	744157	21.78%	2.664%
56	7.563	1998	2013	2045	rBV	1262103	2382326	69.73%	8.529%
57	7.849	2091	2102	2132	rBV	265541	497602	14.56%	1.782%
58	7.987	2143	2145	2148	rBV3	1402	931	0.03%	0.003%
59	8.109	2180	2183	2185	rBV2	1960	1331	0.04%	0.005%
60	8.161	2192	2199	2200	rBV5	2130	2286	0.07%	0.008%
61	8.231	2212	2221	2229	rBV7	5692	10862	0.32%	0.039%
62	8.312	2235	2246	2287	rBV	1118694	2233828	65.38%	7.998%
63	8.784	2391	2393	2396	rBV3	1203	653	0.02%	0.002%
64	8.842	2409	2411	2414	rBV3	1241	616	0.02%	0.002%
65	8.948	2441	2444	2447	rBV	1181	950	0.03%	0.003%
66	8.964	2447	2449	2454	rVB4	1248	865	0.03%	0.003%
67	9.087	2471	2487	2510	rBV	1318368	2305861	67.49%	8.256%
68	9.363	2571	2573	2576	rBV2	1347	765	0.02%	0.003%
69	9.527	2621	2624	2626	rBV2	1513	1084	0.03%	0.004%
70	9.546	2626	2630	2635	rVV4	1458	1349	0.04%	0.005%
71	9.591	2641	2644	2648	rVV3	1695	1187	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031773.D
 Acq On : 06 May 2019 12:26
 Operator : JC/SP
 Sample : K2695-13 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.611	2648	2650	2653	rVV4	1109	706	0.02%	0.003%
73	9.643	2657	2660	2663	rBV2	1488	991	0.03%	0.004%
74	9.749	2687	2693	2696	rBV6	994	1249	0.04%	0.004%
75	9.839	2715	2721	2725	rVB4	1811	1713	0.05%	0.006%
76	9.862	2725	2728	2731	rBV2	1165	1030	0.03%	0.004%
77	9.974	2758	2763	2767	rBV6	1179	1595	0.05%	0.006%
78	10.080	2793	2796	2801	rVB4	736	595	0.02%	0.002%
79	10.125	2807	2810	2815	rVB4	1045	891	0.03%	0.003%
80	10.167	2819	2823	2826	rBV4	1262	1075	0.03%	0.004%
81	10.238	2842	2845	2851	rBV6	1045	1280	0.04%	0.005%
82	10.273	2853	2856	2859	rBV3	2016	1545	0.05%	0.006%
83	10.427	2892	2904	2932	rBV	1017743	1661440	48.63%	5.948%
84	10.604	2953	2959	2963	rBV6	2149	2783	0.08%	0.010%
85	10.717	2990	2994	3003	rVB5	1811	2647	0.08%	0.009%
86	10.807	3019	3022	3023	rBV2	1011	636	0.02%	0.002%
87	10.897	3047	3050	3055	rBV4	1556	1690	0.05%	0.006%
88	11.025	3087	3090	3094	rBV2	1880	1154	0.03%	0.004%
89	11.350	3188	3191	3195	rBV2	1699	1357	0.04%	0.005%
90	11.427	3212	3215	3218	rVB	1768	991	0.03%	0.004%
91	11.482	3219	3232	3256	rBV	1052555	1743916	51.04%	6.244%
92	11.855	3337	3348	3367	rBV	1101112	1842557	53.93%	6.597%
93	12.315	3488	3491	3492	rBV3	1959	1045	0.03%	0.004%
94	12.405	3516	3519	3524	rVB5	2088	1331	0.04%	0.005%
95	12.450	3531	3533	3535	rBV2	1598	909	0.03%	0.003%
96	12.476	3538	3541	3558	rVB4	5792	10134	0.30%	0.036%
97	12.623	3585	3587	3590	rBV3	1673	1171	0.03%	0.004%
98	13.530	3866	3869	3874	rBV4	1958	1639	0.05%	0.006%
99	13.720	3924	3928	3931	rBV2	2710	2109	0.06%	0.008%
100	15.418	4453	4456	4457	rBV2	2731	1564	0.05%	0.006%


Sum of corrected areas: 27930868

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031773.D
Acq On : 06 May 2019 12:26
Operator : JC/SP
Sample : K2695-13 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

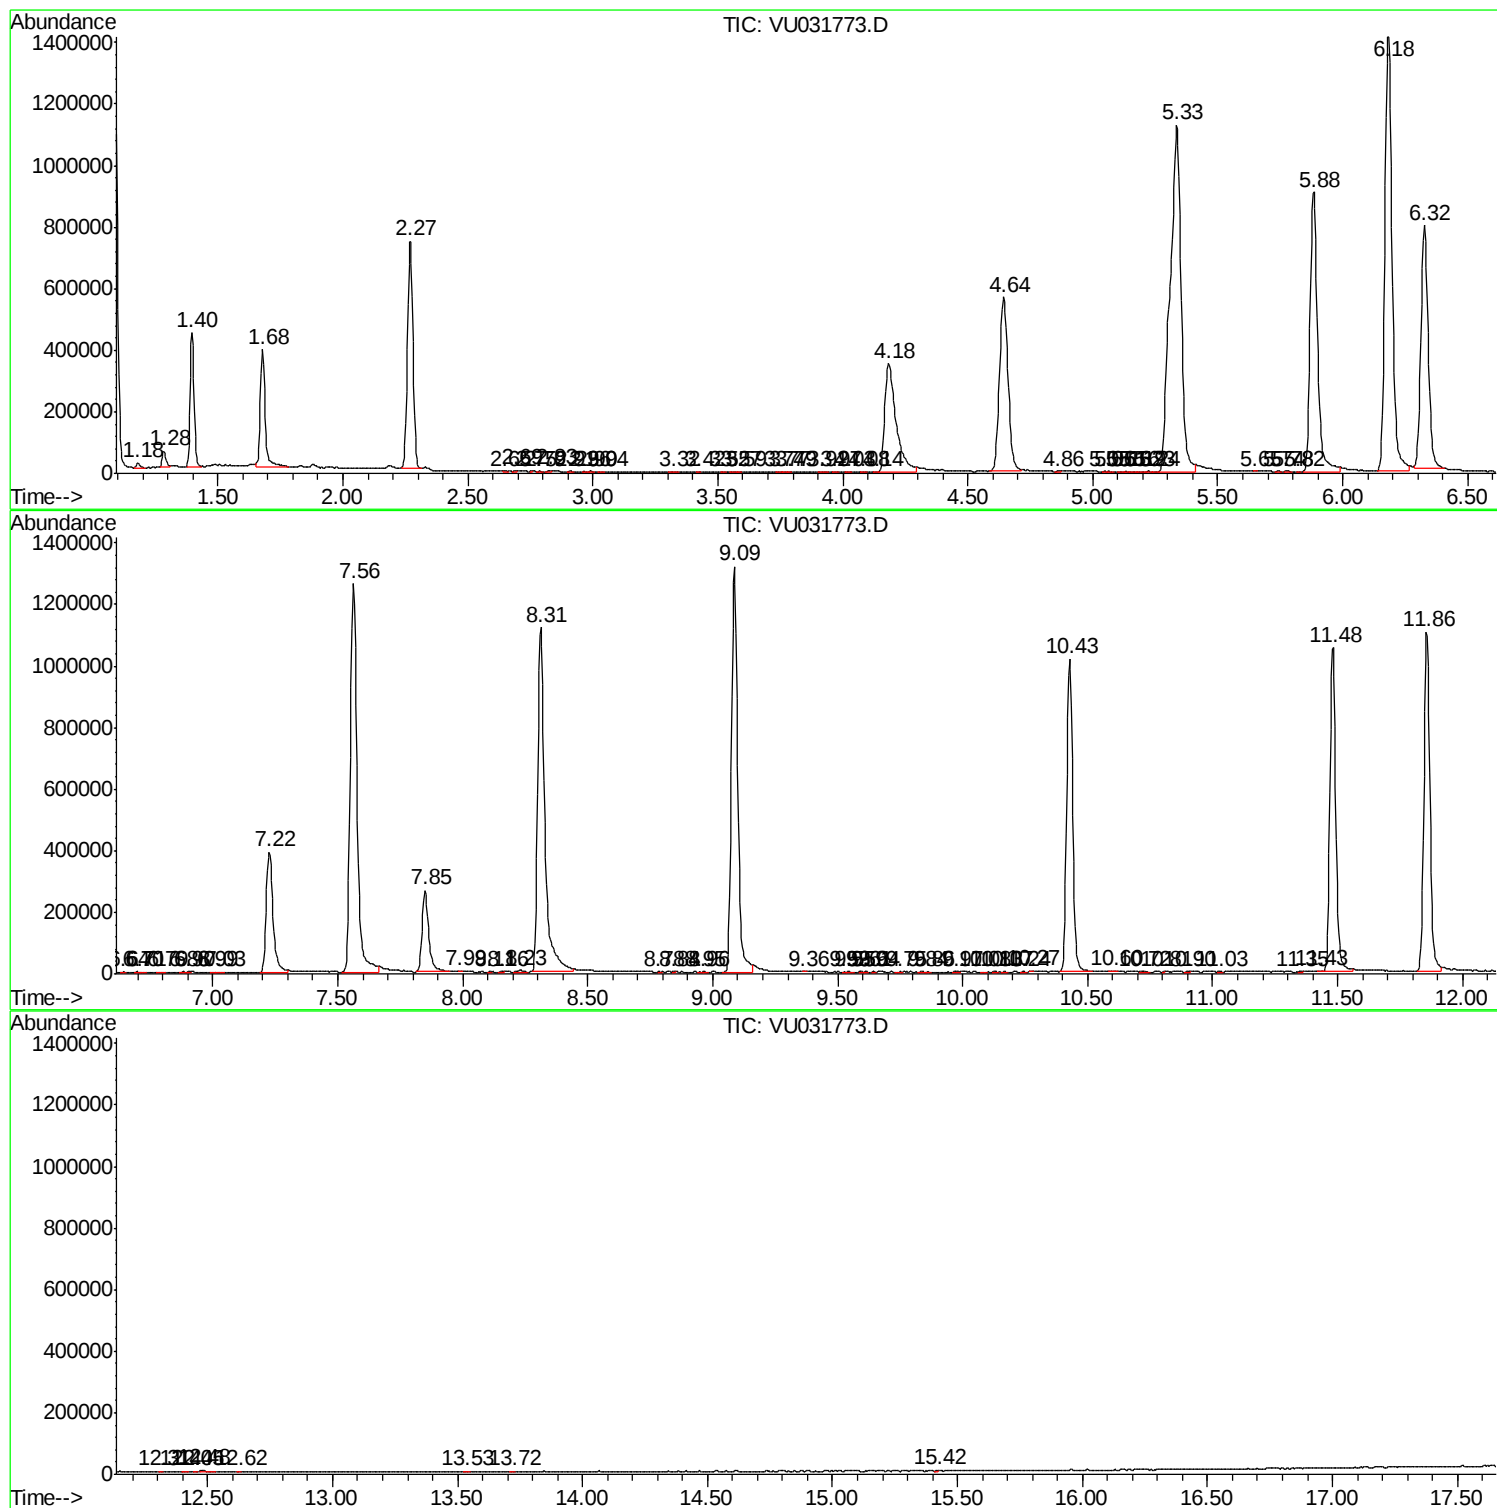

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031773.D
Acq On : 06 May 2019 12:26
Operator : JC/SP
Sample : K2695-13 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031773.D
Acq On : 06 May 2019 12:26
Operator : JC/SP
Sample : K2695-13 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc