

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031774.D
 Acq On : 06 May 2019 12:49
 Operator : JC/SP
 Sample : K2695-11 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	36	rVB2	14787	14030	0.40%	0.049%
2	1.283	55	60	69	rBV2	45190	47062	1.36%	0.165%
3	1.395	88	95	107	rBV	437328	473809	13.66%	1.659%
4	1.678	176	183	199	rVB	377736	453151	13.07%	1.587%
5	1.881	241	246	257	rVB2	29963	39820	1.15%	0.139%
6	2.270	356	367	380	rVB	733823	1129290	32.56%	3.955%
7	2.402	405	408	411	rVB3	1729	1040	0.03%	0.004%
8	2.540	448	451	457	rVB5	1582	1426	0.04%	0.005%
9	2.704	492	502	505	rBV9	3440	5258	0.15%	0.018%
10	2.733	508	511	517	rVB5	1613	1202	0.03%	0.004%
11	2.772	517	523	526	rVB4	2176	2434	0.07%	0.009%
12	2.833	536	542	543	rBV4	1963	1723	0.05%	0.006%
13	2.897	560	562	569	rVB5	1494	1321	0.04%	0.005%
14	3.006	592	596	599	rBV	2441	1917	0.06%	0.007%
15	3.100	622	625	627	rBV2	1739	1401	0.04%	0.005%
16	3.248	664	671	673	rBV4	1228	1386	0.04%	0.005%
17	3.402	715	719	725	rVB2	1605	1658	0.05%	0.006%
18	3.437	726	730	733	rBV4	917	888	0.03%	0.003%
19	3.476	740	742	748	rVB3	927	826	0.02%	0.003%
20	3.511	750	753	756	rVB3	1188	778	0.02%	0.003%
21	3.534	756	760	764	rBV3	997	925	0.03%	0.003%
22	3.592	774	778	781	rBV2	962	1064	0.03%	0.004%
23	3.756	826	829	833	rVB3	1460	1153	0.03%	0.004%
24	3.797	838	842	844	rBV3	1216	1018	0.03%	0.004%
25	3.852	855	859	863	rVB3	1129	997	0.03%	0.003%
26	3.881	863	868	872	rBV2	1429	1488	0.04%	0.005%
27	4.135	944	947	950	rBV3	1042	995	0.03%	0.003%
28	4.183	950	962	1006	rVV	345340	1086331	31.32%	3.805%
29	4.521	1064	1067	1072	rBV4	1307	1088	0.03%	0.004%
30	4.553	1072	1077	1078	rBV2	1496	1201	0.03%	0.004%
31	4.643	1087	1105	1128	rBV	574403	1359441	39.20%	4.761%
32	4.874	1173	1177	1179	rBV3	2480	2022	0.06%	0.007%
33	4.984	1207	1211	1212	rBV3	2021	1480	0.04%	0.005%
34	5.051	1228	1232	1234	rBV3	897	773	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031774.D
 Acq On : 06 May 2019 12:49
 Operator : JC/SP
 Sample : K2695-11 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.334	1297	1320	1361	rBV2	1130461	3468095	100.00%	12.146%
36	5.820	1468	1471	1476	rVB5	1611	1420	0.04%	0.005%
37	5.884	1476	1491	1533	rBV	917039	1919894	55.36%	6.724%
38	6.122	1561	1565	1567	rBV4	1897	1348	0.04%	0.005%
39	6.183	1569	1584	1615	rVV	1655743	3349955	96.59%	11.732%
40	6.328	1617	1629	1657	rVB	786618	1622895	46.79%	5.684%
41	6.691	1737	1742	1744	rBV	1024	786	0.02%	0.003%
42	6.714	1744	1749	1751	rBV3	1286	1156	0.03%	0.004%
43	6.807	1772	1778	1784	rBV4	1710	2171	0.06%	0.008%
44	6.897	1802	1806	1807	rBV4	1527	1048	0.03%	0.004%
45	6.964	1825	1827	1832	rBV3	1481	1298	0.04%	0.005%
46	6.997	1832	1837	1847	rVB6	2002	2721	0.08%	0.010%
47	7.128	1873	1878	1882	rVB3	1725	1988	0.06%	0.007%
48	7.161	1882	1888	1889	rBV3	1373	1242	0.04%	0.004%
49	7.225	1896	1908	1936	rBV	397516	750377	21.64%	2.628%
50	7.562	1998	2013	2048	rBV	1279684	2404489	69.33%	8.421%
51	7.849	2091	2102	2123	rBV	266643	493004	14.22%	1.727%
52	8.109	2180	2183	2186	rVV3	2011	1458	0.04%	0.005%
53	8.170	2195	2202	2210	rBV7	3586	5454	0.16%	0.019%
54	8.228	2212	2220	2230	rVB7	11292	17251	0.50%	0.060%
55	8.312	2234	2246	2279	rBV2	1122499	2231339	64.34%	7.815%
56	8.652	2348	2352	2356	rVB6	2691	2472	0.07%	0.009%
57	8.675	2356	2359	2362	rBV3	1545	939	0.03%	0.003%
58	8.701	2362	2367	2369	rBV4	1150	1030	0.03%	0.004%
59	8.778	2388	2391	2394	rBV3	1382	898	0.03%	0.003%
60	8.849	2409	2413	2415	rBV4	1231	954	0.03%	0.003%
61	8.894	2424	2427	2431	rVB5	1846	1290	0.04%	0.005%
62	8.980	2452	2454	2458	rVB3	1185	783	0.02%	0.003%
63	9.086	2474	2487	2514	rBV	1312603	2315523	66.77%	8.110%
64	9.312	2555	2557	2561	rVB4	1363	869	0.03%	0.003%
65	9.402	2580	2585	2587	rBV5	1387	1393	0.04%	0.005%
66	9.434	2591	2595	2596	rBV4	1392	1015	0.03%	0.004%
67	9.495	2608	2614	2616	rBV4	1520	1404	0.04%	0.005%
68	9.511	2616	2619	2622	rVB	1507	884	0.03%	0.003%
69	9.540	2622	2628	2631	rBV6	1634	1572	0.05%	0.006%
70	9.559	2631	2634	2637	rBV3	1265	1025	0.03%	0.004%
71	9.611	2648	2650	2656	rVB3	1187	999	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031774.D
 Acq On : 06 May 2019 12:49
 Operator : JC/SP
 Sample : K2695-11 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.643	2657	2660	2666	rVB4	1367	1649	0.05%	0.006%
73	9.688	2669	2674	2679	rVB7	1119	1321	0.04%	0.005%
74	9.726	2680	2686	2689	rBV3	1057	1093	0.03%	0.004%
75	9.775	2697	2701	2704	rBV	814	819	0.02%	0.003%
76	9.939	2749	2752	2755	rBV4	1492	1159	0.03%	0.004%
77	9.977	2761	2764	2769	rVB5	1193	829	0.02%	0.003%
78	10.041	2779	2784	2787	rVB4	1463	1226	0.04%	0.004%
79	10.074	2787	2794	2798	rBV5	1451	2016	0.06%	0.007%
80	10.183	2825	2828	2831	rBV3	1251	925	0.03%	0.003%
81	10.427	2889	2904	2926	rBV	1024030	1660426	47.88%	5.815%
82	10.919	3052	3057	3061	rBV3	2175	2108	0.06%	0.007%
83	11.045	3093	3096	3103	rBV2	2805	3132	0.09%	0.011%
84	11.193	3137	3142	3144	rBV3	1316	1300	0.04%	0.005%
85	11.405	3204	3208	3212	rBV5	1821	1871	0.05%	0.007%
86	11.482	3220	3232	3257	rBV	1062837	1747662	50.39%	6.121%
87	11.736	3309	3311	3318	rVB6	1880	1451	0.04%	0.005%
88	11.855	3336	3348	3370	rBV	1089710	1854352	53.47%	6.494%
89	12.356	3501	3504	3506	rBV3	1375	1049	0.03%	0.004%
90	12.453	3531	3534	3535	rBV3	1678	954	0.03%	0.003%
91	12.475	3536	3541	3542	rBV4	3610	3035	0.09%	0.011%
92	12.565	3566	3569	3571	rBV3	1377	1018	0.03%	0.004%
93	12.668	3598	3601	3603	rBV4	1173	843	0.02%	0.003%
94	12.729	3617	3620	3623	rBV2	1514	934	0.03%	0.003%
95	13.080	3725	3729	3732	rBV3	1331	1180	0.03%	0.004%
96	13.189	3760	3763	3765	rBV2	1469	922	0.03%	0.003%
97	13.408	3828	3831	3835	rBV2	2082	1634	0.05%	0.006%
98	13.733	3927	3932	3935	rBV4	2319	2162	0.06%	0.008%
99	13.781	3943	3947	3950	rBV3	2316	1871	0.05%	0.007%
100	13.990	4010	4012	4015	rBV2	1540	1090	0.03%	0.004%


Sum of corrected areas: 28552866

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031774.D
Acq On : 06 May 2019 12:49
Operator : JC/SP
Sample : K2695-11 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

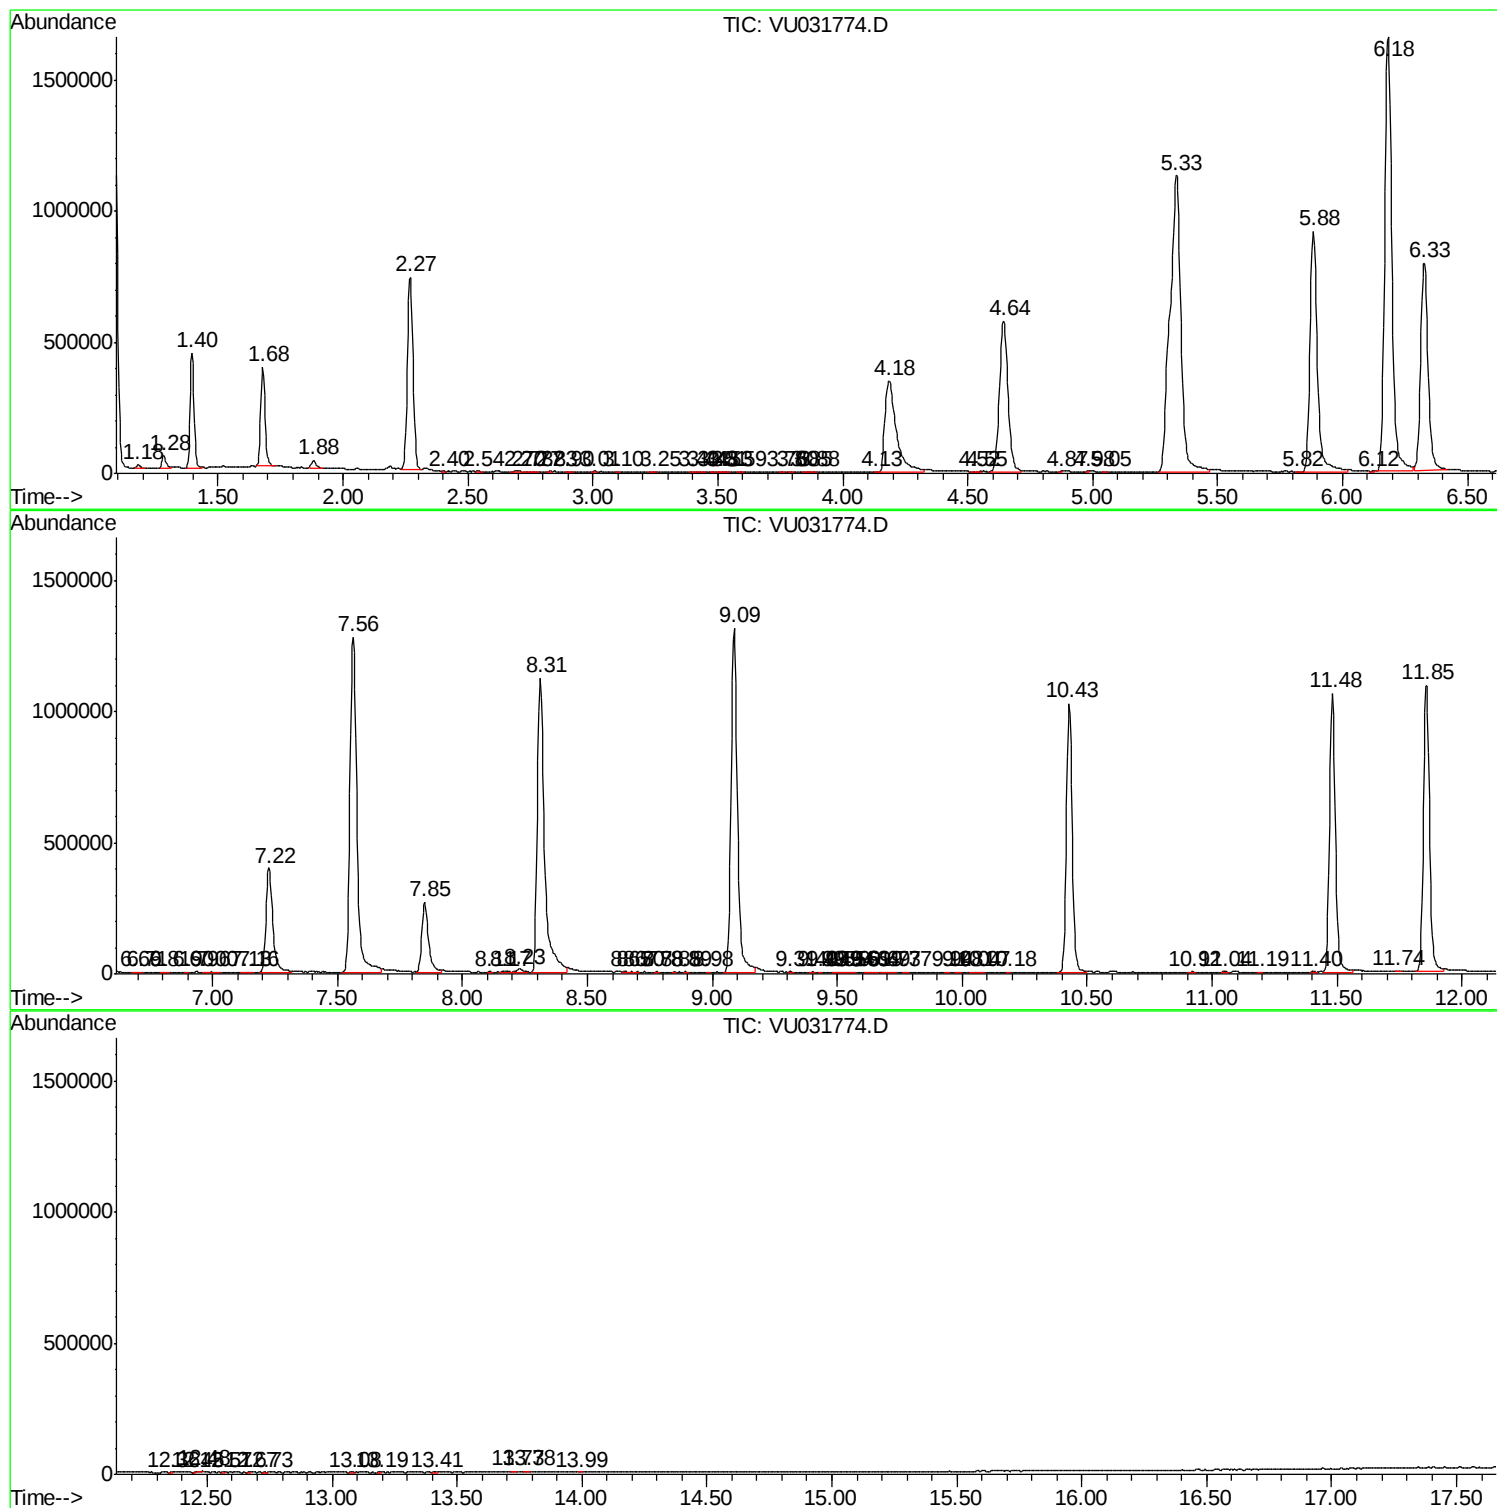

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031774.D
Acq On : 06 May 2019 12:49
Operator : JC/SP
Sample : K2695-11 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031774.D
Acq On : 06 May 2019 12:49
Operator : JC/SP
Sample : K2695-11 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc