

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031775.D
 Acq On : 06 May 2019 13:13
 Operator : JC/SP
 Sample : K2695-03 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	36	rVB2	15845	14670	0.43%	0.053%
2	1.283	55	60	67	rBV2	46433	46695	1.37%	0.168%
3	1.396	88	95	107	rBV	431622	470177	13.75%	1.691%
4	1.679	176	183	202	rVB	371964	456420	13.35%	1.642%
5	2.267	356	366	380	rVB	731074	1121098	32.79%	4.032%
6	2.701	497	501	504	rBV4	2392	1639	0.05%	0.006%
7	2.785	525	527	532	rVB4	1323	906	0.03%	0.003%
8	2.830	532	541	544	rBV2	3498	5100	0.15%	0.018%
9	3.064	611	614	617	rVB2	1875	1144	0.03%	0.004%
10	3.090	617	622	625	rBV5	1200	910	0.03%	0.003%
11	3.138	635	637	641	rVV2	1121	696	0.02%	0.003%
12	3.219	659	662	666	rBV3	1119	814	0.02%	0.003%
13	3.299	684	687	690	rBV3	1312	1139	0.03%	0.004%
14	3.367	704	708	710	rVV3	1806	1453	0.04%	0.005%
15	3.379	710	712	719	rVB4	1587	1586	0.05%	0.006%
16	3.450	731	734	741	rVB2	1711	1699	0.05%	0.006%
17	3.521	753	756	759	rBV4	1051	792	0.02%	0.003%
18	3.559	762	768	771	rBV3	1897	2403	0.07%	0.009%
19	3.707	811	814	821	rVV	1159	1206	0.04%	0.004%
20	3.762	825	831	833	rBV3	820	853	0.02%	0.003%
21	3.807	841	845	850	rVB3	1502	1599	0.05%	0.006%
22	3.836	850	854	858	rBV3	1756	1548	0.05%	0.006%
23	4.035	912	916	919	rVB2	1160	880	0.03%	0.003%
24	4.055	919	922	926	rVB3	1301	988	0.03%	0.004%
25	4.087	926	932	936	rBV3	1559	1871	0.05%	0.007%
26	4.129	941	945	948	rBV2	823	773	0.02%	0.003%
27	4.186	950	963	1014	rBV	343984	1139030	33.31%	4.096%
28	4.511	1061	1064	1067	rVB3	1417	874	0.03%	0.003%
29	4.531	1067	1070	1075	rVB3	1865	1618	0.05%	0.006%
30	4.643	1088	1105	1131	rBV	565699	1349427	39.47%	4.853%
31	4.881	1174	1179	1182	rBV5	1195	1008	0.03%	0.004%
32	4.977	1207	1209	1212	rBV3	1594	1260	0.04%	0.005%
33	5.058	1231	1234	1237	rBV3	1133	903	0.03%	0.003%
34	5.077	1238	1240	1244	rVV2	967	731	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031775.D
 Acq On : 06 May 2019 13:13
 Operator : JC/SP
 Sample : K2695-03 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.145	1257	1261	1264	rVB3	862	779	0.02%	0.003%
36	5.177	1269	1271	1279	rVB4	1559	1456	0.04%	0.005%
37	5.225	1279	1286	1290	rBV2	1704	1743	0.05%	0.006%
38	5.334	1298	1320	1356	rBV2	1116518	3419148	100.00%	12.297%
39	5.669	1420	1424	1426	rBV4	1212	1172	0.03%	0.004%
40	5.714	1434	1438	1443	rVB6	2322	2074	0.06%	0.007%
41	5.881	1477	1490	1524	rBV	890595	1876497	54.88%	6.749%
42	6.183	1567	1584	1615	rBV	1429808	2899470	84.80%	10.428%
43	6.328	1616	1629	1659	rVB	784412	1625078	47.53%	5.845%
44	6.633	1721	1724	1728	rVB2	1894	1218	0.04%	0.004%
45	6.656	1728	1731	1734	rVB4	2034	1318	0.04%	0.005%
46	6.762	1762	1764	1769	rVB4	1396	931	0.03%	0.003%
47	6.907	1804	1809	1811	rBV2	1250	1111	0.03%	0.004%
48	6.993	1833	1836	1843	rVV4	1588	1716	0.05%	0.006%
49	7.048	1849	1853	1854	rVV2	1204	711	0.02%	0.003%
50	7.061	1854	1857	1860	rVV3	1106	895	0.03%	0.003%
51	7.157	1881	1887	1890	rBV4	1012	999	0.03%	0.004%
52	7.225	1895	1908	1936	rBV	389564	741863	21.70%	2.668%
53	7.563	2000	2013	2039	rBV	1255794	2329534	68.13%	8.378%
54	7.849	2092	2102	2128	rBV	262965	488831	14.30%	1.758%
55	8.035	2158	2160	2163	rBV2	1119	815	0.02%	0.003%
56	8.119	2183	2186	2191	rVB4	1644	1611	0.05%	0.006%
57	8.145	2191	2194	2197	rBV3	1786	1039	0.03%	0.004%
58	8.170	2197	2202	2204	rBV3	2980	2966	0.09%	0.011%
59	8.212	2212	2215	2216	rBV3	2005	1193	0.03%	0.004%
60	8.228	2216	2220	2234	rVB9	6420	9946	0.29%	0.036%
61	8.312	2234	2246	2287	rBV2	1086981	2231714	65.27%	8.026%
62	8.688	2360	2363	2368	rVB6	1722	1514	0.04%	0.005%
63	8.723	2372	2374	2378	rVB3	1714	999	0.03%	0.004%
64	8.900	2426	2429	2432	rBV3	991	802	0.02%	0.003%
65	9.087	2472	2487	2533	rBV	1307915	2313615	67.67%	8.321%
66	9.366	2569	2574	2580	rVB7	1652	1847	0.05%	0.007%
67	9.398	2580	2584	2587	rVB5	1749	1292	0.04%	0.005%
68	9.415	2587	2589	2591	rBV3	1499	839	0.02%	0.003%
69	9.694	2673	2676	2680	rBV4	1634	1176	0.03%	0.004%
70	9.733	2684	2688	2689	rBV3	1092	736	0.02%	0.003%
71	9.791	2703	2706	2709	rBV	870	769	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031775.D
 Acq On : 06 May 2019 13:13
 Operator : JC/SP
 Sample : K2695-03 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.871	2728	2731	2737	rVB6	1573	1442	0.04%	0.005%
73	10.003	2769	2772	2776	rVB3	1270	1088	0.03%	0.004%
74	10.119	2806	2808	2814	rVB4	933	740	0.02%	0.003%
75	10.257	2848	2851	2854	rBV2	899	708	0.02%	0.003%
76	10.315	2865	2869	2872	rBV2	1463	1256	0.04%	0.005%
77	10.382	2885	2890	2891	rBV3	1621	1199	0.04%	0.004%
78	10.427	2891	2904	2926	rVV	1012930	1635596	47.84%	5.882%
79	10.601	2954	2958	2963	rVV5	2124	2185	0.06%	0.008%
80	10.640	2967	2970	2973	rVB3	1189	842	0.02%	0.003%
81	10.665	2974	2978	2981	rBV4	1287	1125	0.03%	0.004%
82	10.810	3018	3023	3024	rVV2	1009	745	0.02%	0.003%
83	10.894	3046	3049	3051	rBV2	1041	740	0.02%	0.003%
84	10.964	3067	3071	3072	rBV3	1358	898	0.03%	0.003%
85	11.083	3106	3108	3117	rVB5	1670	1396	0.04%	0.005%
86	11.209	3144	3147	3150	rBV2	1319	737	0.02%	0.003%
87	11.479	3218	3231	3252	rBV	1040257	1705631	49.88%	6.134%
88	11.755	3314	3317	3320	rBV2	2761	2156	0.06%	0.008%
89	11.855	3336	3348	3370	rBV	1096801	1824914	53.37%	6.563%
90	12.308	3486	3489	3492	rBV4	1657	1025	0.03%	0.004%
91	12.434	3525	3528	3533	rBV4	1521	1307	0.04%	0.005%
92	12.479	3535	3542	3549	rVB5	4554	6759	0.20%	0.024%
93	12.594	3575	3578	3584	rBV4	1310	1190	0.03%	0.004%
94	12.771	3631	3633	3637	rVB5	1422	845	0.02%	0.003%
95	13.151	3748	3751	3753	rBV2	1670	1122	0.03%	0.004%
96	13.209	3767	3769	3775	rBV4	1137	918	0.03%	0.003%
97	13.250	3780	3782	3785	rBV3	1126	706	0.02%	0.003%
98	13.778	3942	3946	3950	rBV	1691	1503	0.04%	0.005%
99	14.054	4029	4032	4034	rVB2	1644	798	0.02%	0.003%
100	14.379	4130	4133	4137	rBV2	2405	2120	0.06%	0.008%


Sum of corrected areas: 27805018

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031775.D
Acq On : 06 May 2019 13:13
Operator : JC/SP
Sample : K2695-03 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

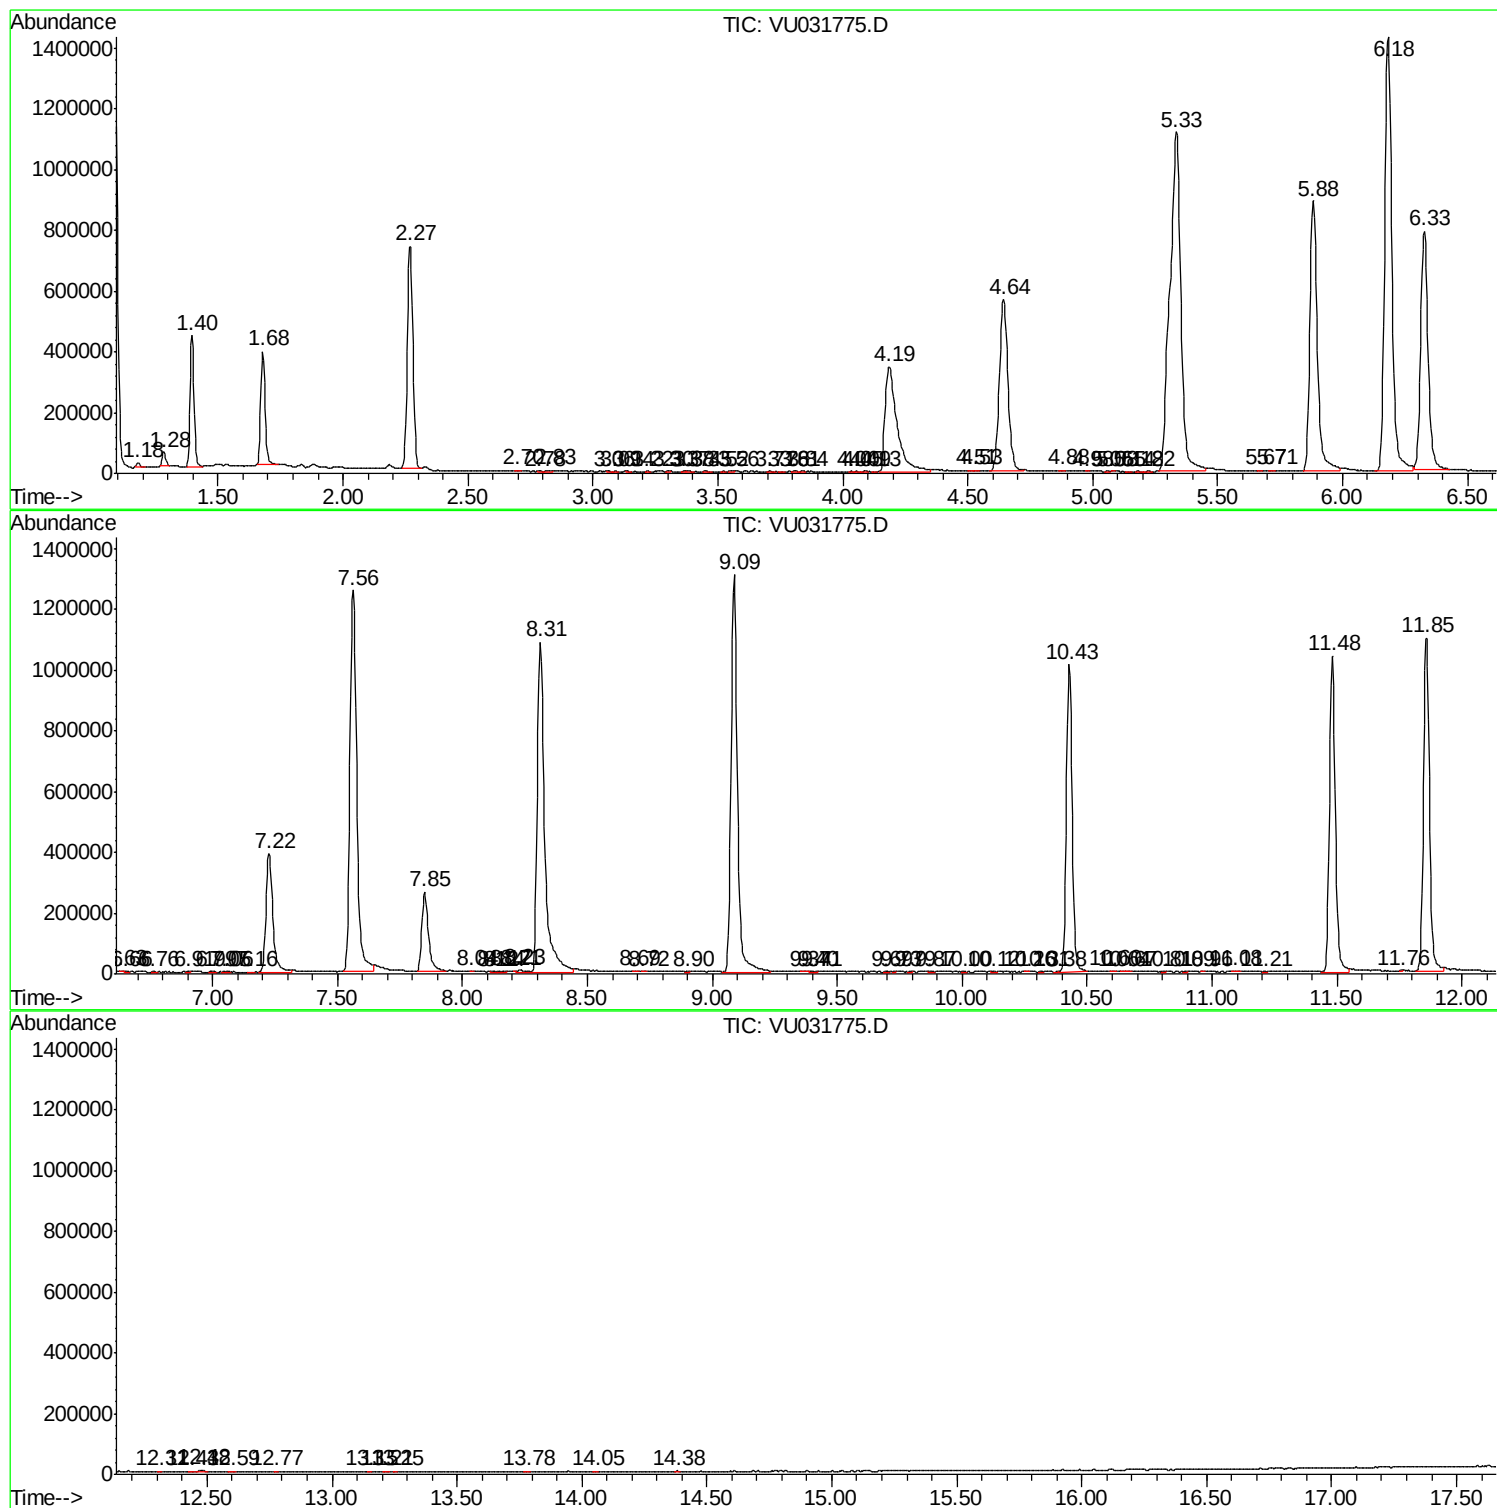

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031775.D
Acq On : 06 May 2019 13:13
Operator : JC/SP
Sample : K2695-03 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031775.D
Acq On : 06 May 2019 13:13
Operator : JC/SP
Sample : K2695-03 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X71

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc