

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031776.D
 Acq On : 06 May 2019 13:36
 Operator : JC/SP
 Sample : K2695-01 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.283	55	60	67	rVB2	46498	47213	0.87%	0.153%
2	1.396	88	95	109	rBV	439043	476499	8.76%	1.544%
3	1.679	175	183	201	rVB	368189	476881	8.77%	1.546%
4	1.881	240	246	259	rVB2	61398	84953	1.56%	0.275%
5	2.270	356	367	381	rVB	743520	1141417	20.99%	3.699%
6	2.662	486	489	493	rVB4	1385	1071	0.02%	0.003%
7	2.682	493	495	498	rBV	1359	990	0.02%	0.003%
8	2.781	524	526	529	rBV3	700	422	0.01%	0.001%
9	2.958	579	581	583	rBV3	378	220	0.00%	0.001%
10	2.978	583	587	588	rBV2	1150	786	0.01%	0.003%
11	3.019	597	600	602	rBV2	1262	650	0.01%	0.002%
12	3.039	602	606	613	rVB4	1621	1855	0.03%	0.006%
13	3.074	613	617	620	rBV	1133	855	0.02%	0.003%
14	3.135	630	636	640	rBV5	1878	1722	0.03%	0.006%
15	3.161	640	644	646	rVB3	1042	735	0.01%	0.002%
16	3.206	654	658	660	rBV3	976	775	0.01%	0.003%
17	3.219	660	662	664	rVV2	1023	408	0.01%	0.001%
18	3.238	665	668	671	rVB2	1628	885	0.02%	0.003%
19	3.261	671	675	676	rBV2	761	501	0.01%	0.002%
20	3.280	676	681	683	rBV3	1138	915	0.02%	0.003%
21	3.299	684	687	691	rVB4	1538	1130	0.02%	0.004%
22	3.392	714	716	719	rBV3	659	347	0.01%	0.001%
23	3.431	726	728	730	rBV4	601	223	0.00%	0.001%
24	3.482	742	744	745	rBV	536	242	0.00%	0.001%
25	3.508	750	752	754	rBV2	1144	586	0.01%	0.002%
26	3.550	762	765	769	rBV2	901	617	0.01%	0.002%
27	3.572	769	772	775	rVB2	970	638	0.01%	0.002%
28	3.592	775	778	780	rBV2	929	643	0.01%	0.002%
29	3.608	780	783	788	rVB3	1501	1204	0.02%	0.004%
30	3.634	788	791	794	rVB4	840	562	0.01%	0.002%
31	3.662	795	800	802	rBV3	1617	1440	0.03%	0.005%
32	3.691	808	809	810	rBB	163	86	0.00%	0.000%
33	3.736	821	823	825	rBV	686	413	0.01%	0.001%
34	3.820	846	849	853	rVB2	1644	1314	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031776.D
 Acq On : 06 May 2019 13:36
 Operator : JC/SP
 Sample : K2695-01 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	3.846	853	857	859	rBV2	1997	1636	0.03%	0.005%
36	3.859	859	861	864	rVV2	1227	929	0.02%	0.003%
37	3.884	864	869	872	rVV4	1263	1282	0.02%	0.004%
38	3.907	873	876	881	rVB4	677	696	0.01%	0.002%
39	3.933	882	884	886	rBV2	338	133	0.00%	0.000%
40	3.987	899	901	903	rVB3	771	358	0.01%	0.001%
41	4.016	903	910	913	rBV5	1369	1765	0.03%	0.006%
42	4.042	915	918	923	rVB	1180	916	0.02%	0.003%
43	4.068	923	926	928	rBV2	640	326	0.01%	0.001%
44	4.084	928	931	932	rBV2	831	428	0.01%	0.001%
45	4.113	937	940	944	rVB2	633	412	0.01%	0.001%
46	4.183	946	962	1002	rBV	362583	1103650	20.29%	3.577%
47	4.643	1090	1105	1133	rBV	566465	1338661	24.62%	4.339%
48	4.859	1170	1172	1179	rBV4	1631	1879	0.03%	0.006%
49	5.113	1248	1251	1252	rBV2	939	483	0.01%	0.002%
50	5.158	1263	1265	1271	rVB2	1250	855	0.02%	0.003%
51	5.190	1272	1275	1278	rVB2	1531	891	0.02%	0.003%
52	5.248	1290	1293	1296	rBV2	969	673	0.01%	0.002%
53	5.334	1296	1320	1361	rBV2	1128916	3483889	64.06%	11.291%
54	5.884	1477	1491	1520	rBV	904241	1878801	34.55%	6.089%
55	6.125	1564	1566	1568	rBV3	1708	965	0.02%	0.003%
56	6.180	1568	1583	1614	rVV	2727940	5438134	100.00%	17.625%
57	6.328	1617	1629	1651	rVB	793439	1623531	29.85%	5.262%
58	6.772	1764	1767	1770	rBV3	1508	1258	0.02%	0.004%
59	6.826	1779	1784	1791	rBV5	1762	2332	0.04%	0.008%
60	6.858	1791	1794	1795	rBV4	1138	666	0.01%	0.002%
61	6.887	1800	1803	1805	rBV3	1577	871	0.02%	0.003%
62	6.968	1826	1828	1831	rVB3	1340	601	0.01%	0.002%
63	7.035	1846	1849	1851	rBV3	904	609	0.01%	0.002%
64	7.225	1889	1908	1937	rBV	404076	770308	14.16%	2.497%
65	7.418	1966	1968	1969	rBV2	1190	482	0.01%	0.002%
66	7.514	1995	1998	1999	rBV2	1402	711	0.01%	0.002%
67	7.563	2000	2013	2051	rVV	1288090	2410200	44.32%	7.811%
68	7.849	2092	2102	2126	rBV	268085	490331	9.02%	1.589%
69	8.083	2172	2175	2180	rBV8	1528	1674	0.03%	0.005%
70	8.225	2208	2219	2235	rBV2	194124	340377	6.26%	1.103%
71	8.312	2235	2246	2289	rVV2	1117359	2219635	40.82%	7.194%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031776.D
 Acq On : 06 May 2019 13:36
 Operator : JC/SP
 Sample : K2695-01 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	8.891	2421	2426	2430	rBV6	1457	1871	0.03%	0.006%
73	9.087	2474	2487	2509	rBV	1317493	2278901	41.91%	7.386%
74	9.373	2570	2576	2579	rBV5	2257	2529	0.05%	0.008%
75	9.534	2623	2626	2627	rBV	951	649	0.01%	0.002%
76	9.694	2674	2676	2679	rBV2	777	420	0.01%	0.001%
77	9.791	2704	2706	2708	rBV2	1018	410	0.01%	0.001%
78	9.993	2767	2769	2770	rBV2	809	347	0.01%	0.001%
79	10.083	2795	2797	2800	rVB	872	456	0.01%	0.001%
80	10.167	2818	2823	2824	rBV	1048	838	0.02%	0.003%
81	10.235	2841	2844	2846	rBV3	981	614	0.01%	0.002%
82	10.427	2892	2904	2924	rBV	1006107	1641470	30.18%	5.320%
83	10.771	3008	3011	3014	rBV2	1182	818	0.02%	0.003%
84	10.894	3046	3049	3050	rBV	935	548	0.01%	0.002%
85	11.058	3097	3100	3103	rBV2	1515	1322	0.02%	0.004%
86	11.077	3104	3106	3107	rBV	1458	592	0.01%	0.002%
87	11.128	3119	3122	3127	rBV3	1707	1342	0.02%	0.004%
88	11.157	3128	3131	3136	rBV4	1500	1255	0.02%	0.004%
89	11.482	3219	3232	3255	rBV	1034452	1702070	31.30%	5.516%
90	11.855	3335	3348	3372	rBV	1091061	1845525	33.94%	5.981%
91	12.900	3669	3673	3679	rBV4	2379	2542	0.05%	0.008%


Sum of corrected areas: 30855065

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031776.D
Acq On : 06 May 2019 13:36
Operator : JC/SP
Sample : K2695-01 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X00

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

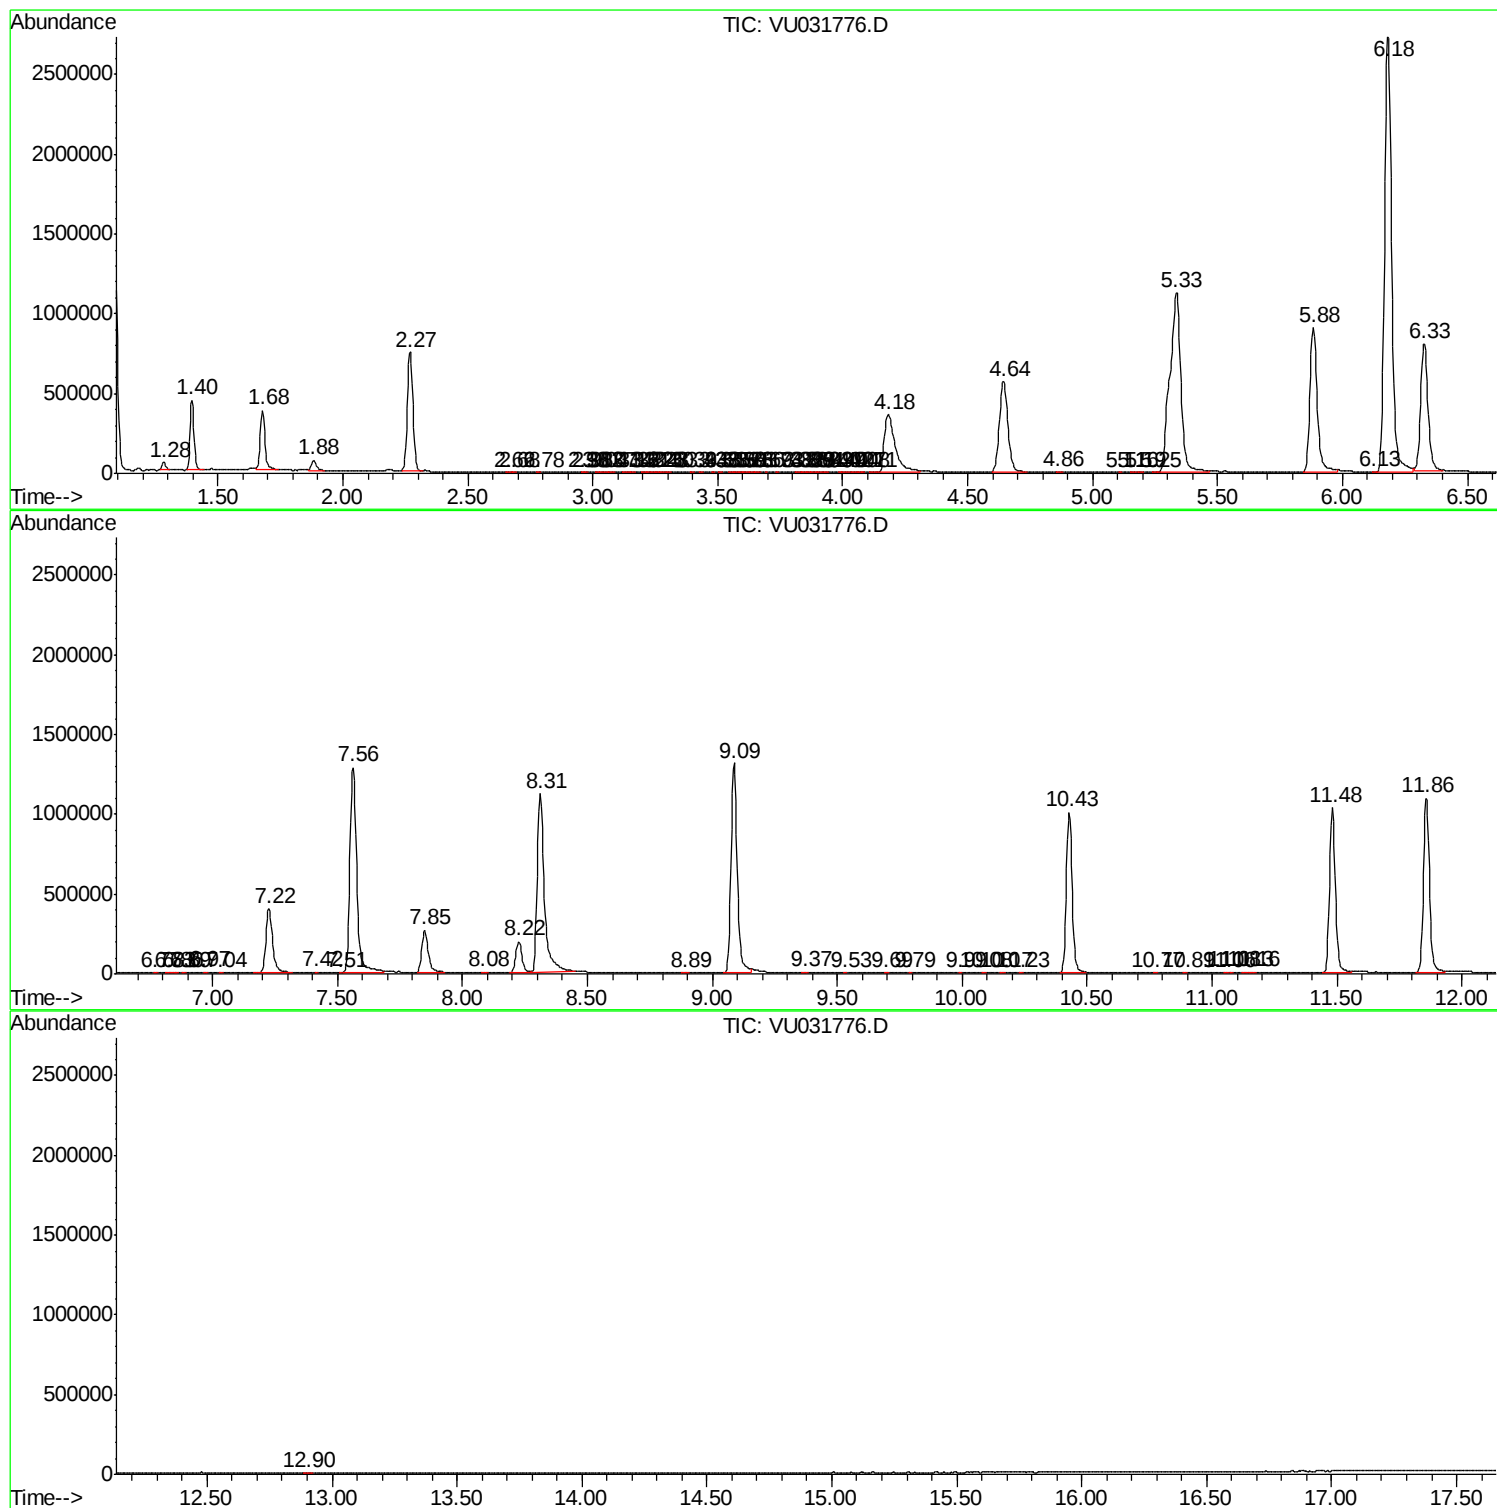

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031776.D
Acq On : 06 May 2019 13:36
Operator : JC/SP
Sample : K2695-01 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X00

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031776.D
Acq On : 06 May 2019 13:36
Operator : JC/SP
Sample : K2695-01 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X00

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc